

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG092515\
 Data File : BG018903.D
 Acq On : 26 Sep 2015 6:56
 Operator : UM/NP
 Sample : G3800-03
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C03G7

Quant Time: Sep 28 00:42:48 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG091015.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Sep 26 04:18:39 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.99	152	48841	20.00	ng/ul	0.00
18) Naphthalene-d8	10.79	136	204785	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.61	164	139672	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.35	188	378489	20.00	ng/ul	0.00
78) Chrysene-d12	21.60	240	432641	20.00	ng/ul	0.00
86) Perylene-d12	24.77	264	443099	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.44	96	1374	1.35	ng/uL	0.00
5) Phenol-d5	7.16	99	29903	7.46	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.31	67	65876	28.34	ng/ul	0.00
9) 2-Chlorophenol-d4	7.53	132	78624	25.88	ng/ul	0.00
13) 4-Methylphenol-d8	8.70	113	55714	17.12	ng/ul	0.00
19) Nitrobenzene-d5	9.15	128	47786	30.80	ng/ul	0.00
22) 2-Nitrophenol-d4	9.87	143	54385	34.86	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.41	165	99693	30.35	ng/ul	0.00
29) 4-Chloroaniline-d4	10.92	131	7590	1.99	ng/ul	0.00
44) Dimethylphthalate-d6	14.01	166	360418	32.06	ng/ul	0.00
47) Acenaphthylene-d8	14.31	160	285463	21.43	ng/ul	0.00
52) 4-Nitrophenol-d4	14.82	143	14062	6.52	ng/ul	0.00
58) Fluorene-d10	15.60	176	156663	15.94	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.72	200	37529	20.95	ng/ul	0.00
71) Anthracene-d10	17.45	188	84636	5.08	ng/ul	0.00
79) Pyrene-d10	19.74	212	215172	10.81	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.56	264	115435	5.35	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	14.06	163	18257	1.68	ng/ul#	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG092515\
Data File : BG018903.D
Acq On : 26 Sep 2015 6:56
Operator : UM/NP
Sample : G3800-03
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C03G7

Quant Time: Sep 28 00:42:48 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG091015.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Sep 26 04:18:39 2015
Response via : Initial Calibration

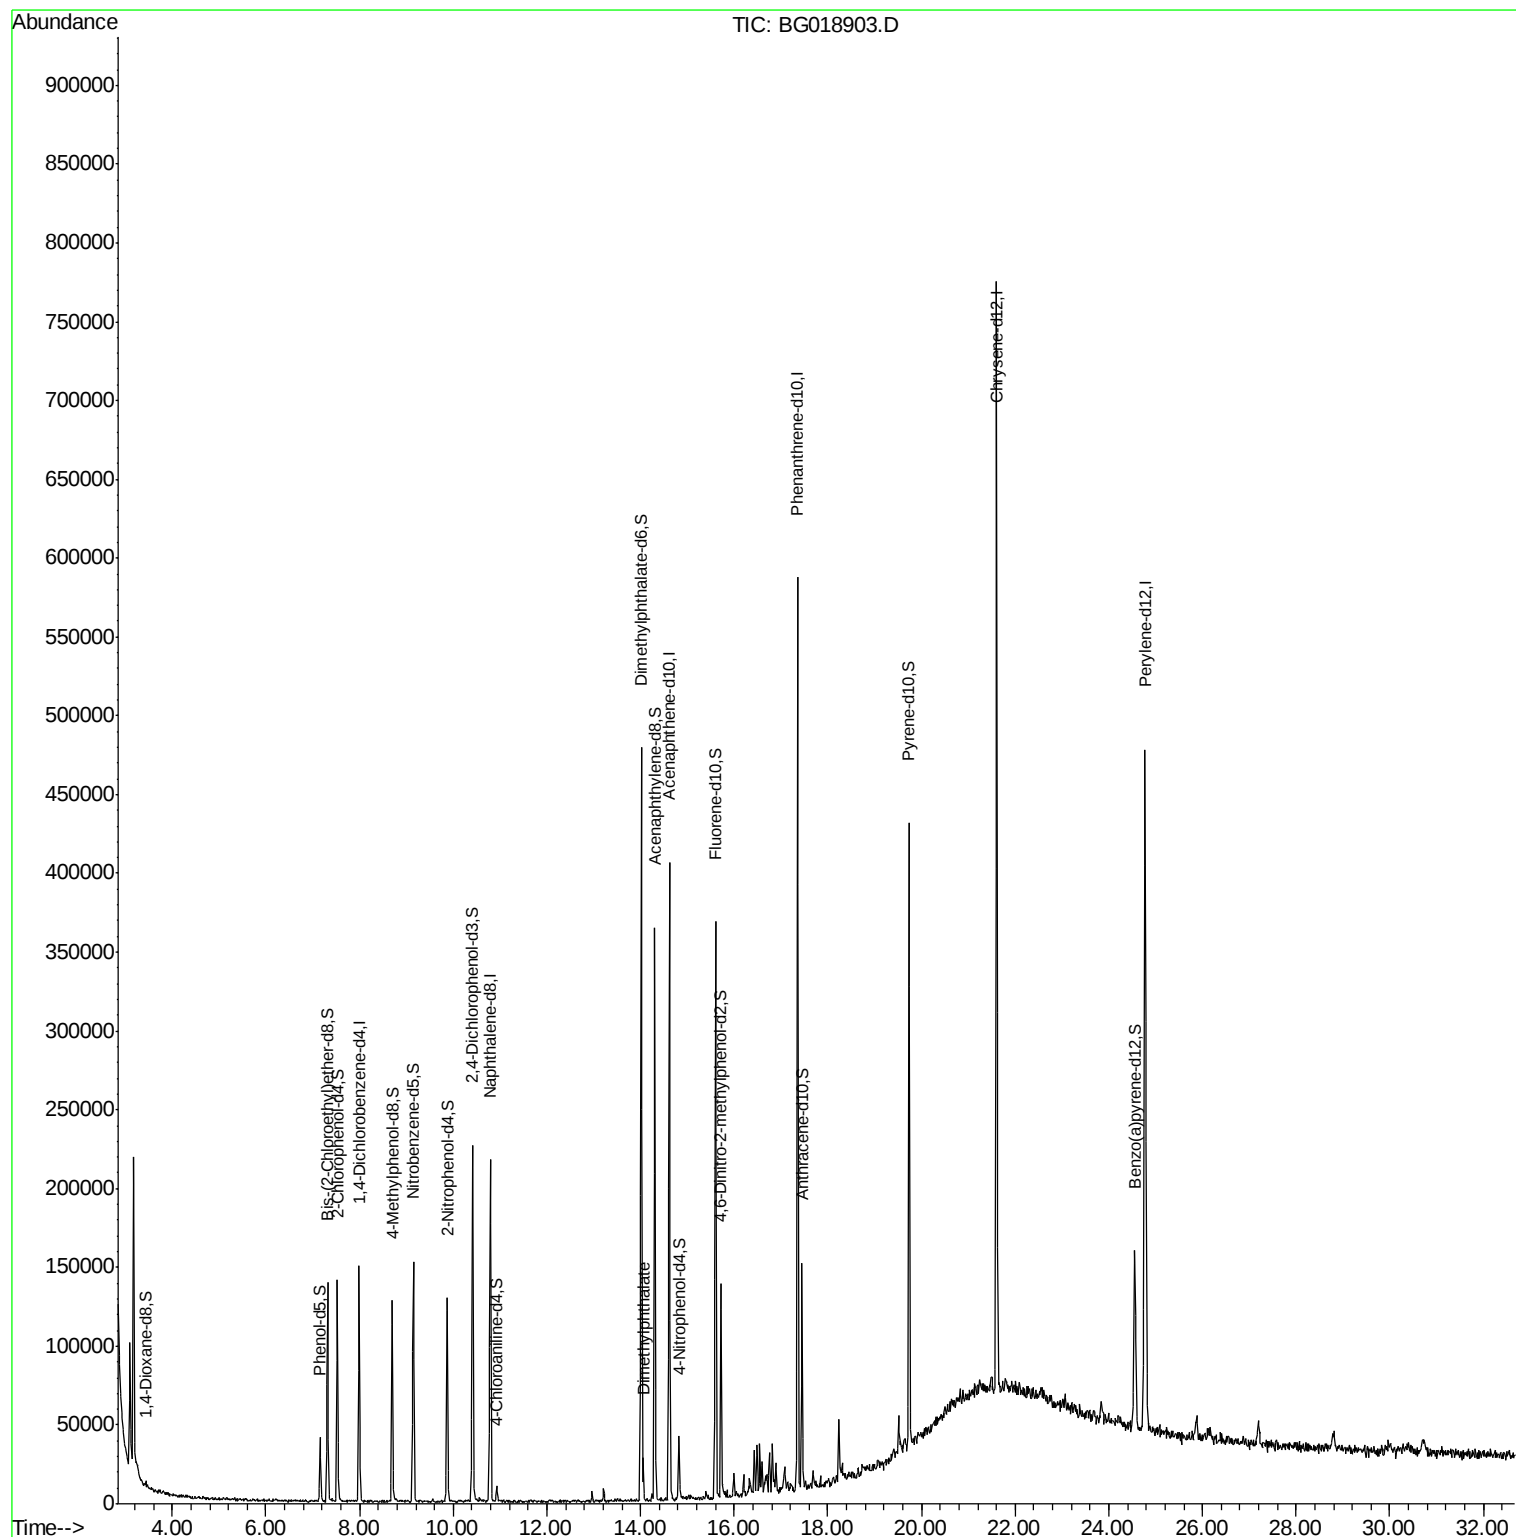

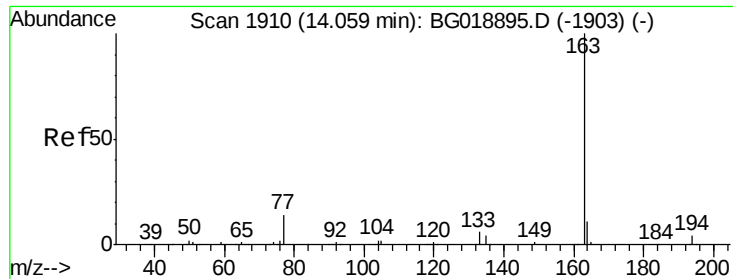

#45

Dimethylphthalate

Concen: 1.68 ng/ul

RT: 14.06 min Scan# 1910

Delta R.T. 0.00 min

Lab File: BG018903.D

Acq: 26 Sep 2015 6:56

Instrument :

BNA_G

ClientSampleId :

C03G7


Tgt Ion:163 Resp: 18257

Ion Ratio Lower Upper

163 100

194 5.3 2.9 4.3#

164 10.2 7.7 11.5

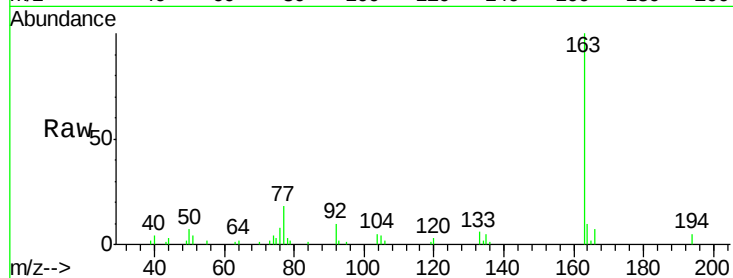

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

