

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG092515\
 Data File : BG018933.D
 Acq On : 27 Sep 2015 3:54
 Operator : UM/NP
 Sample : G3798-17
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 D9G71

Quant Time: Sep 28 04:38:02 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG091015.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Sep 28 04:33:51 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.00	152	58729	20.00	ng/ul	0.00
18) Naphthalene-d8	10.79	136	259164	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.62	164	169359	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.36	188	396495	20.00	ng/ul	0.00
78) Chrysene-d12	21.62	240	408928	20.00	ng/ul	0.00
86) Perylene-d12	24.80	264	416791	20.00	ng/ul	0.02

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.44	96	3301	2.70	ng/uL	0.00
5) Phenol-d5	7.17	99	80354	16.66	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.32	67	44896	16.06	ng/ul	0.00
9) 2-Chlorophenol-d4	7.53	132	67458	18.47	ng/ul	0.00
13) 4-Methylphenol-d8	8.71	113	66943	17.11	ng/ul	0.00
19) Nitrobenzene-d5	9.15	128	30011	15.28	ng/ul	0.00
22) 2-Nitrophenol-d4	9.88	143	36542	18.51	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.42	165	73113	17.59	ng/ul	0.00
29) 4-Chloroaniline-d4	10.93	131	83935	17.35	ng/ul	0.00
44) Dimethylphthalate-d6	14.02	166	214519	15.74	ng/ul	0.00
47) Acenaphthylene-d8	14.31	160	145178	8.99	ng/ul	0.00
52) 4-Nitrophenol-d4	14.83	143	31708	12.12	ng/ul	0.00
58) Fluorene-d10	15.61	176	68907	5.78	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.73	200	6143	3.27	ng/ul	0.02
71) Anthracene-d10	17.46	188	20803	1.19	ng/ul	0.00
79) Pyrene-d10	19.74	212	61564	3.27	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.58	264	18884	0.93	ng/ul	0.02


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	14.07	163	121448	9.19	ng/ul#	99




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG092515\
Data File : BG018933.D
Acq On : 27 Sep 2015 3:54
Operator : UM/NP
Sample : G3798-17
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
D9G71

Quant Time: Sep 28 04:38:02 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG091015.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Sep 28 04:33:51 2015
Response via : Initial Calibration

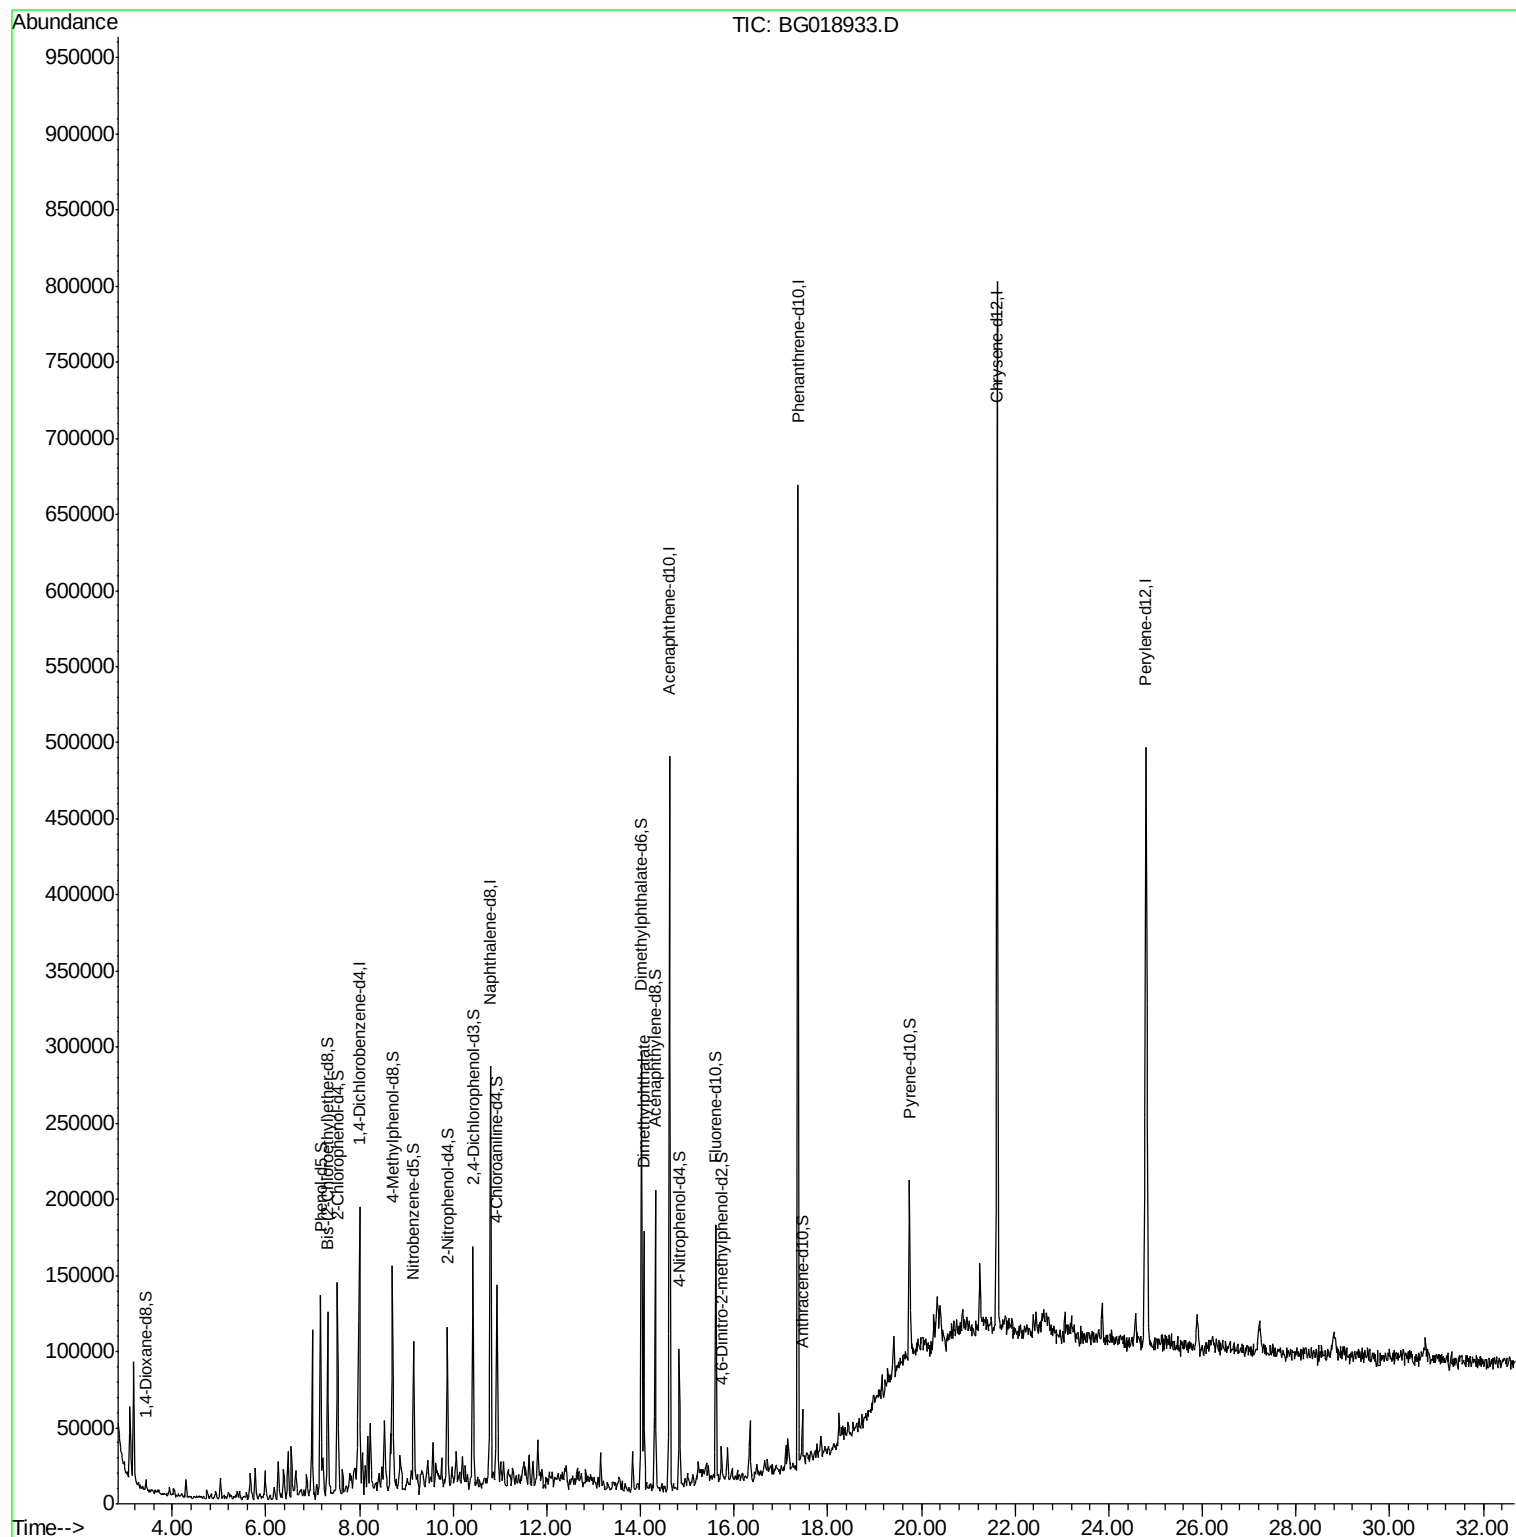

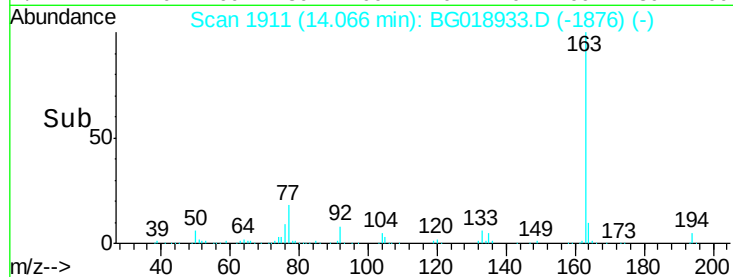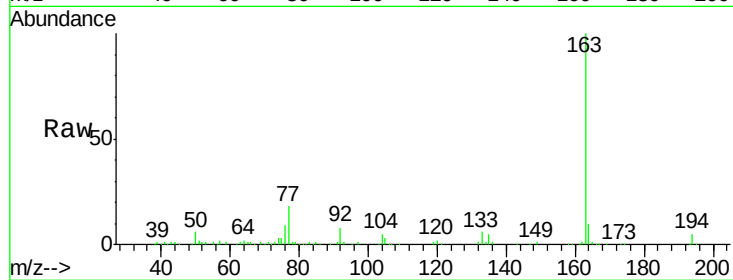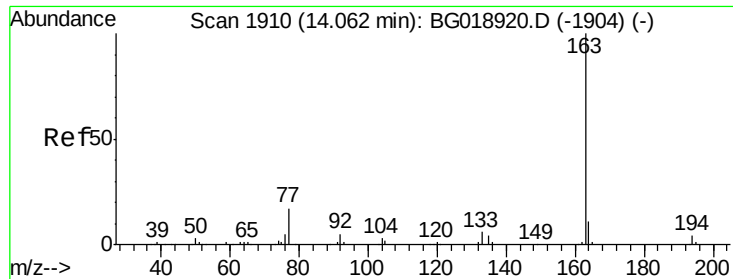

#45

Dimethylphthalate

Concen: 9.19 ng/ul

RT: 14.07 min Scan# 1911

Delta R.T. 0.00 min

Lab File: BG018933.D

Acq: 27 Sep 2015 3:54

Instrument :

BNA_G

ClientSampleId :

D9G71

Tgt Ion:163 Resp: 121448

Ion Ratio Lower Upper

163 100

194 4.5 2.9 4.3#

164 9.6 7.7 11.5

