


Data Path : Z:\HPCHEM1\BNA G\DATA\BG092517\
 Data File : BG028907.D
 Acq On : 25 Sep 2017 14:35
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG091217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 26 12:06:14 2017

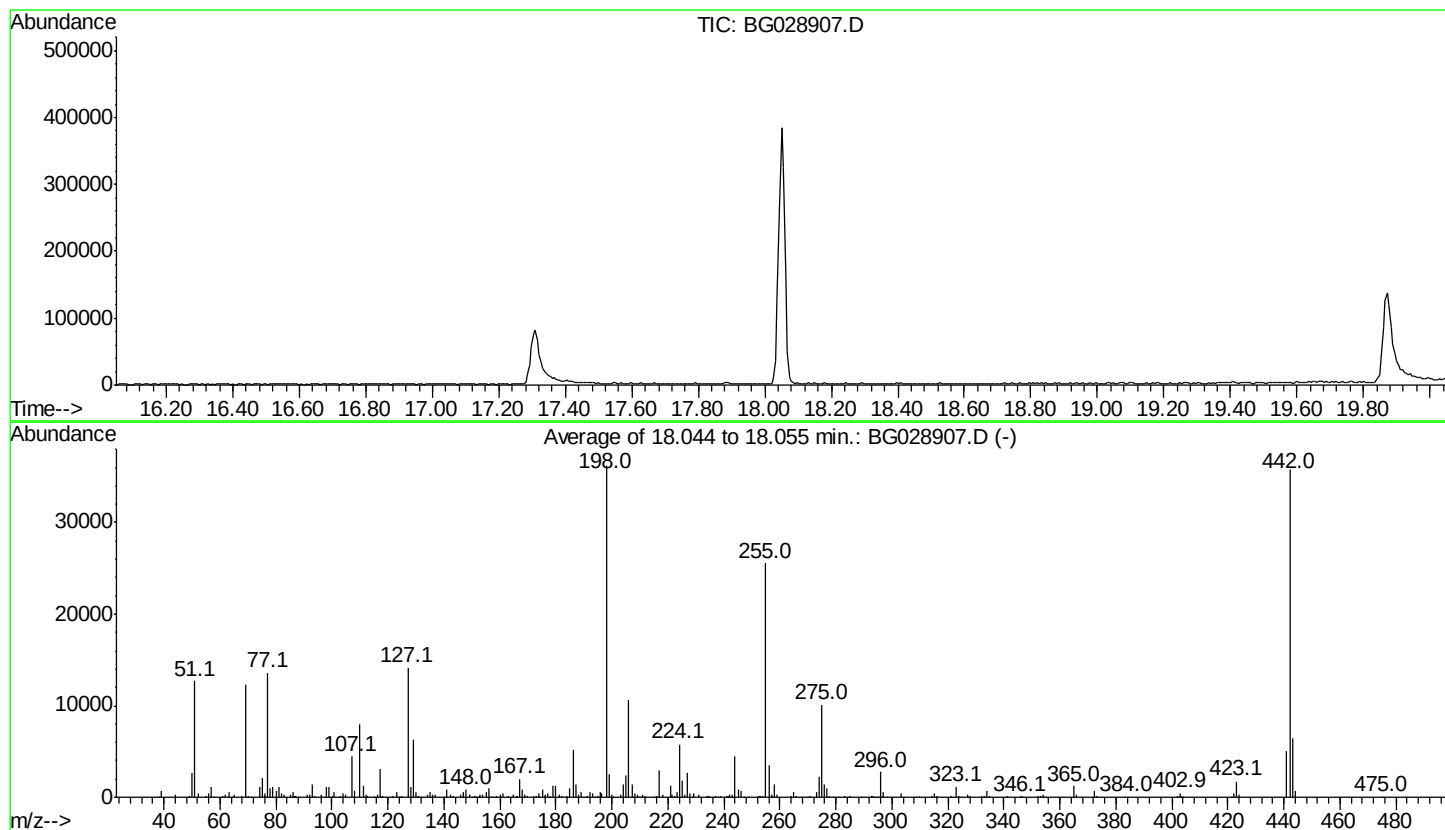

AutoFind: Scans 2460, 2461, 2462; Background Corrected with Scan 2453

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.1	12702	PASS
68	69	0.00	2	1.2	148	PASS
69	198	0.00	100	33.9	12274	PASS
70	69	0.00	2	1.1	132	PASS
127	198	10	80	39.1	14168	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	36216	PASS
199	198	5	9	7.1	2573	PASS
275	198	10	60	27.9	10114	PASS
365	198	1	100	3.4	1230	PASS
441	442	0.01	24	14.2	5100	PASS
442	198	50	100	98.8	35792	PASS
443	442	15	24	18.0	6443	PASS