


Data Path : Z:\HPCHEM1\BNA G\DATA\BG092517\
 Data File : BG028925.D
 Acq On : 26 Sep 2017 2:32
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG091217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 26 12:06:14 2017

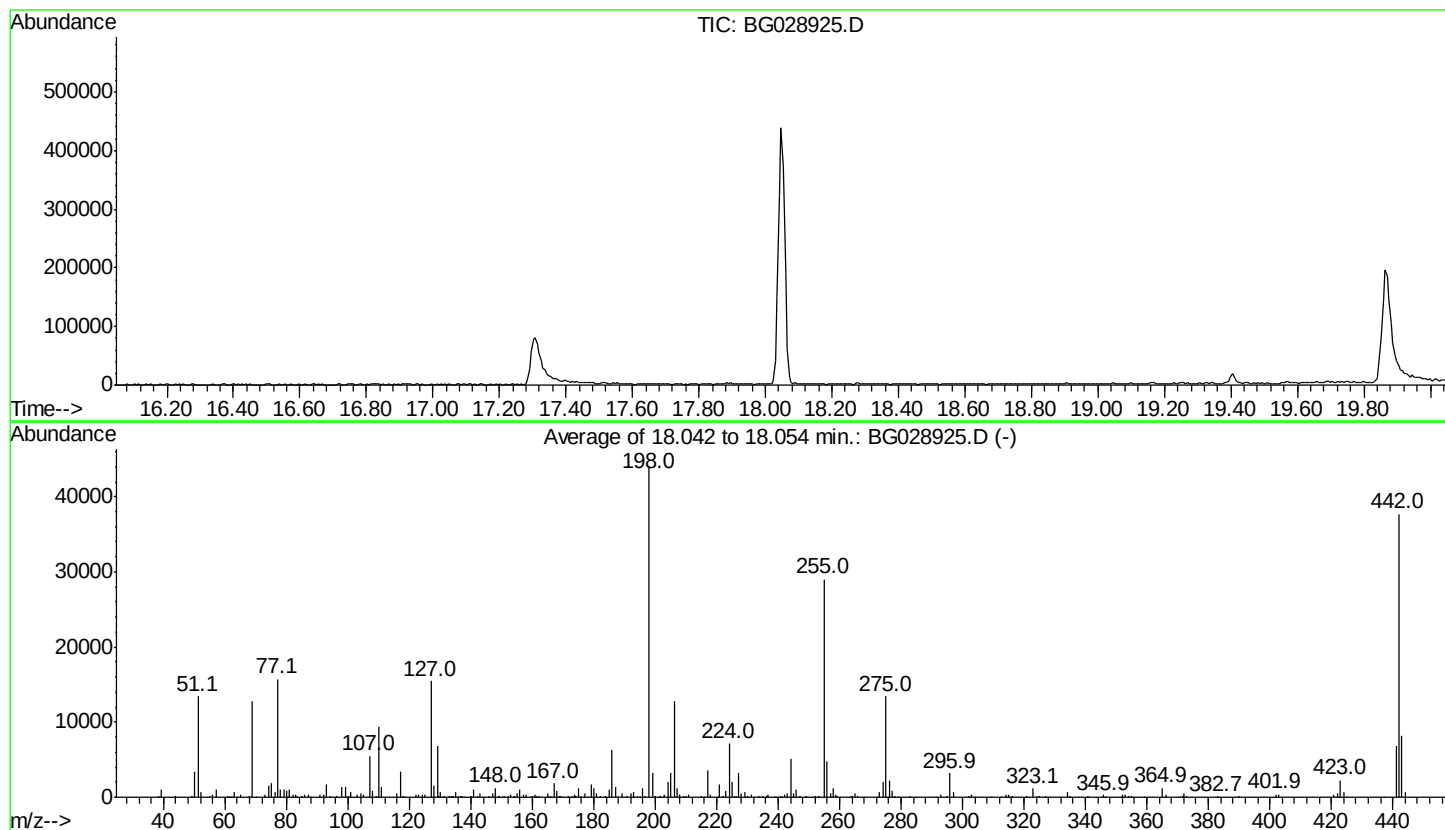

AutoFind: Scans 2460, 2461, 2462; Background Corrected with Scan 2454

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.5	13441	PASS
68	69	0.00	2	1.9	242	PASS
69	198	0.00	100	28.9	12763	PASS
70	69	0.00	2	0.5	64	PASS
127	198	10	80	35.0	15430	PASS
197	198	0.00	2	0.5	240	PASS
198	198	100	100	100.0	44136	PASS
199	198	5	9	7.2	3191	PASS
275	198	10	60	30.3	13391	PASS
365	198	1	100	2.8	1245	PASS
441	442	0.01	24	18.1	6821	PASS
442	198	50	100	85.5	37741	PASS
443	442	15	24	21.7	8192	PASS