
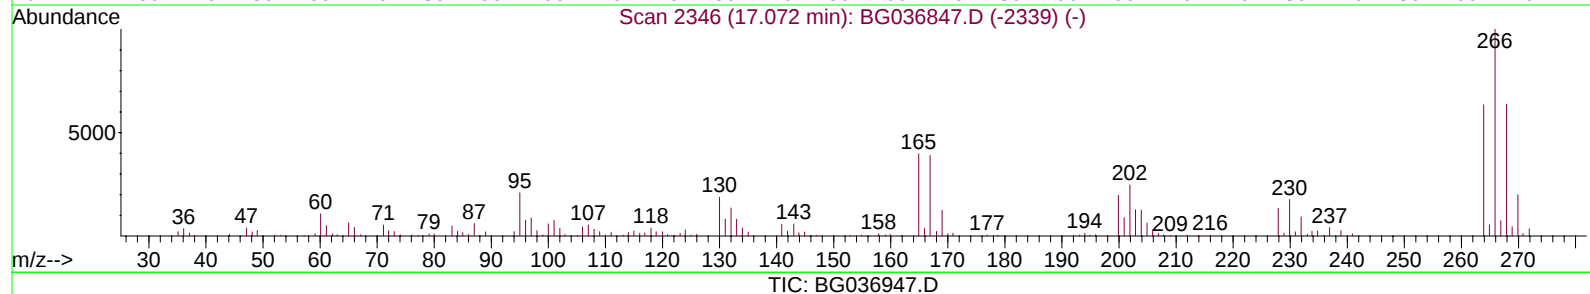
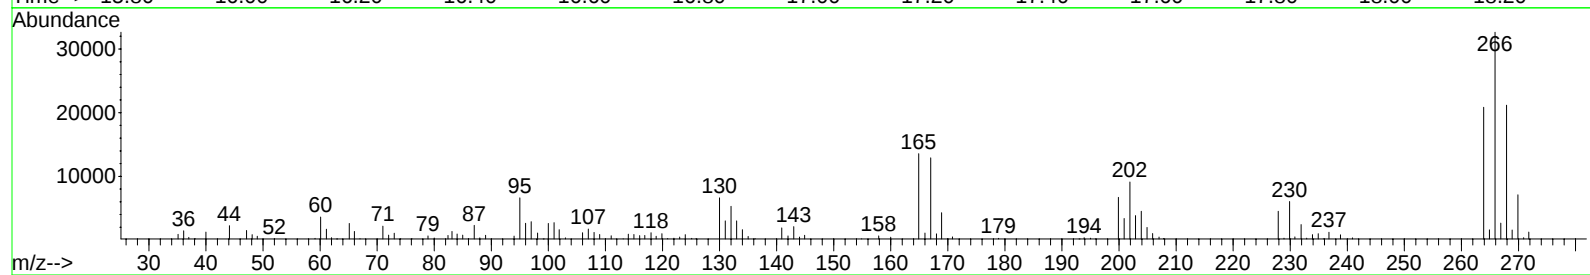


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG092518\
Data File : BG036947.D
Acq On : 25 Sep 2018 12:53
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 25 18:06:36 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG092018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 24 10:41:23 2018
Response via : Initial Calibration

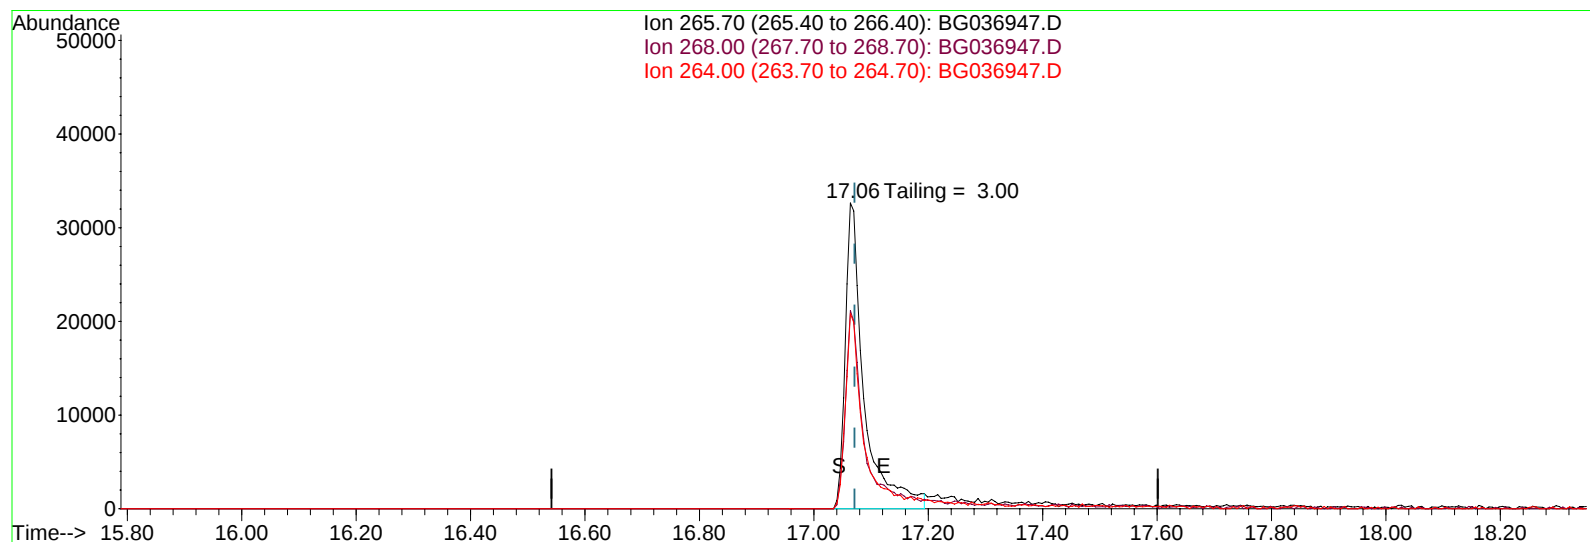

(69) Pentachlorophenol (C)




17.064min (-0.008) 4767.94ng

response 74097

Ion	Exp%	Act%
265.70	100	100
268.00	64.30	64.85
264.00	61.10	63.85
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG092518\
Data File : BG036947.D
Acq On : 25 Sep 2018 12:53
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 25 18:06:36 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG092018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 24 10:41:23 2018
Response via : Initial Calibration

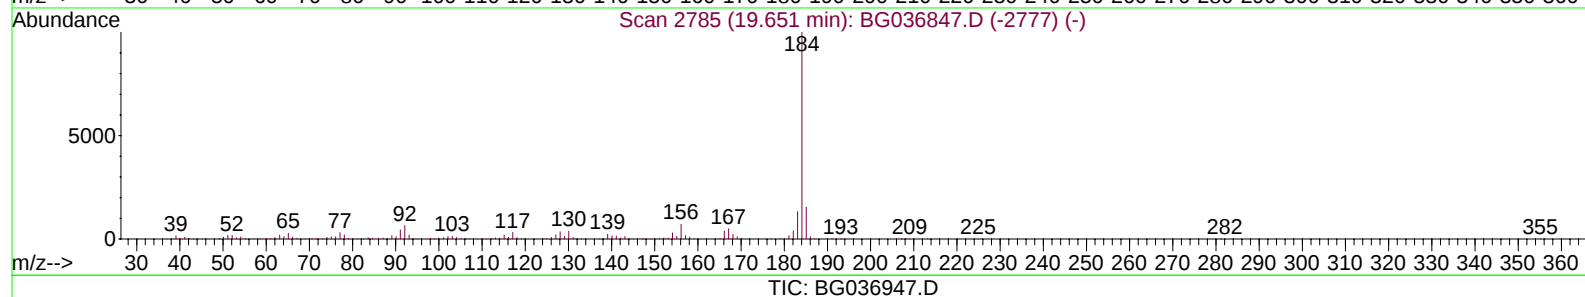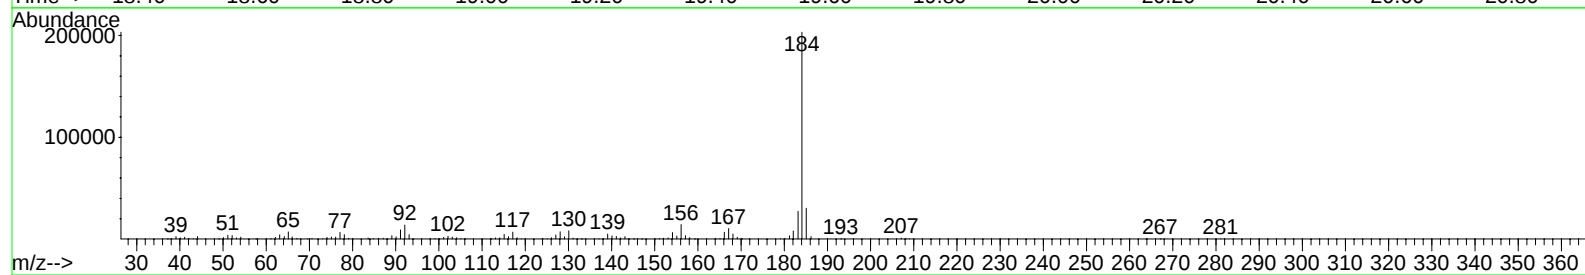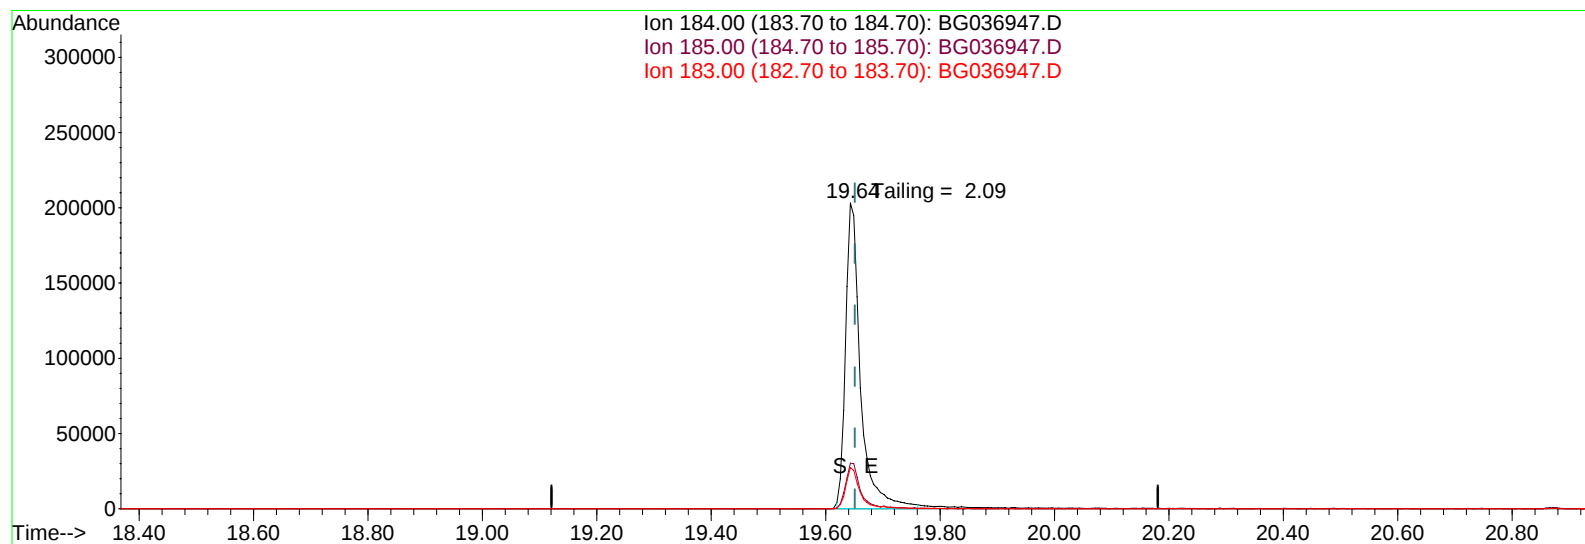

(76) Benzidine

19.643min (-0.008) 5739.67ng

response 374952

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.89
183.00	13.60	13.47
0.00	0.00	0.00