
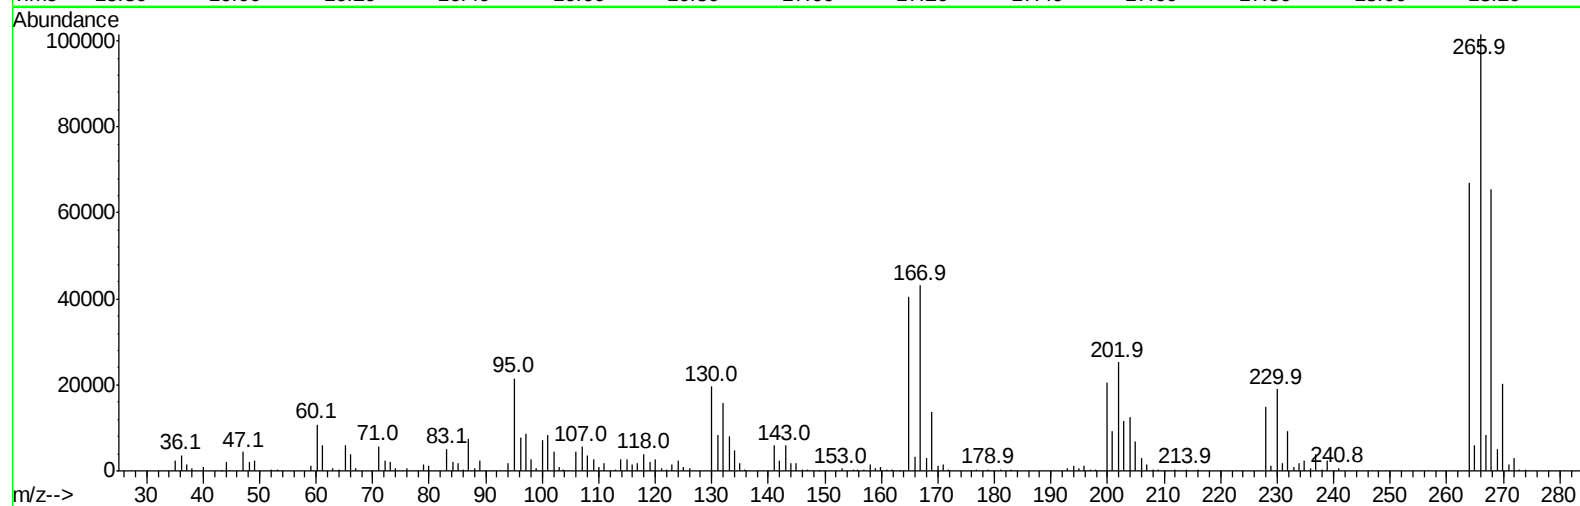


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG092518\
Data File : BG036964.D
Acq On : 26 Sep 2018 1:25
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 01 07:42:14 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG092018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 24 10:41:23 2018
Response via : Initial Calibration

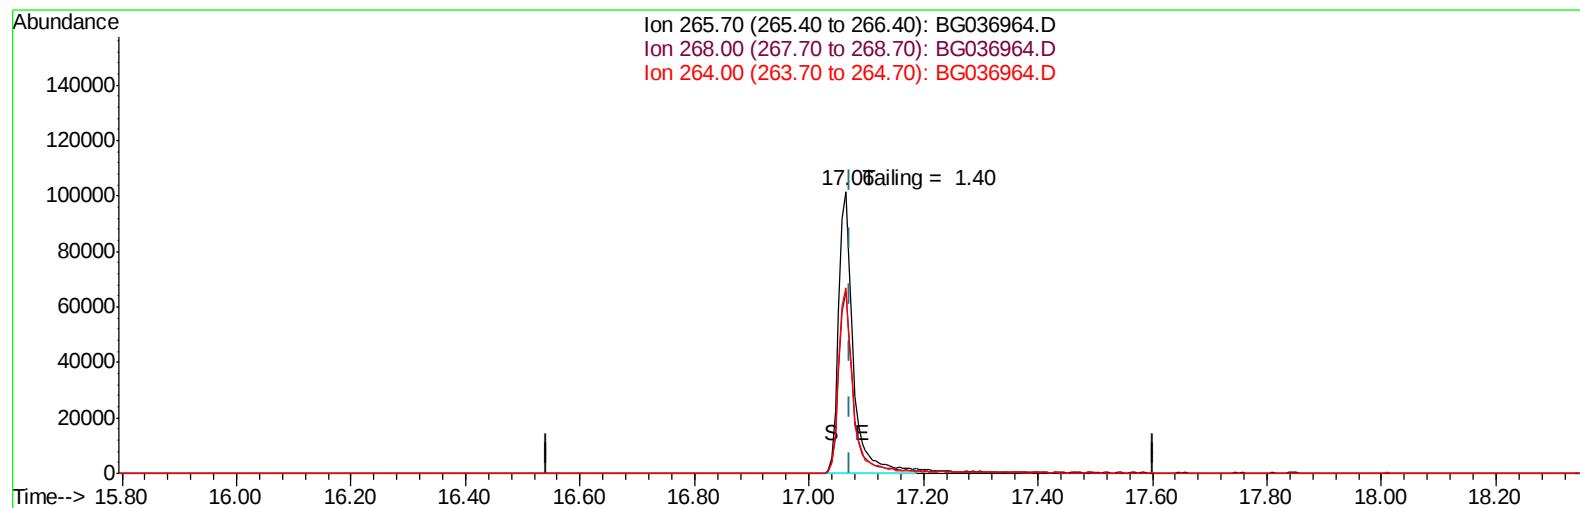

TIC: BG036964.D

(69) Pentachlorophenol (C)



17.063min (-0.008) 10773.60ng

response 183242

Ion	Exp%	Act%
265.70	100	100
268.00	64.30	64.45
264.00	61.10	65.85
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG092518\
Data File : BG036964.D
Acq On : 26 Sep 2018 1:25
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 01 07:42:14 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG092018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 24 10:41:23 2018
Response via : Initial Calibration

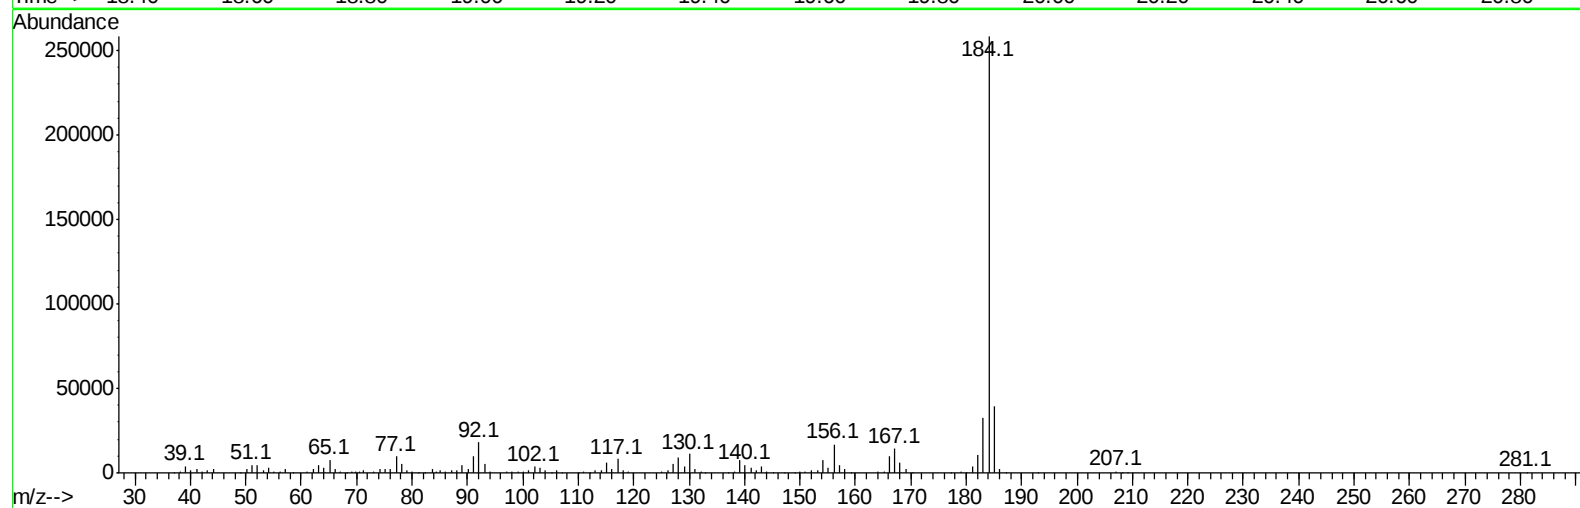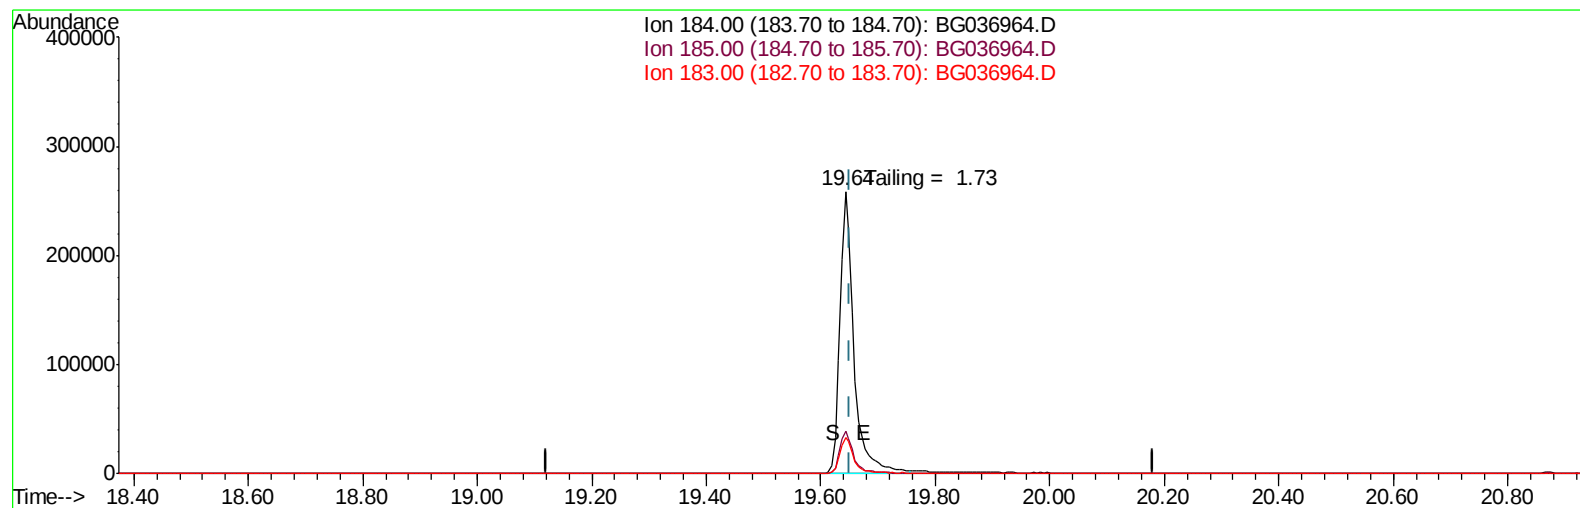

TIC: BG036964.D

(76) Benzidine

19.643min (-0.008) 4961.84ng

response 446235

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	15.14
183.00	13.60	12.60
0.00	0.00	0.00