


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092518\
 Data File : BG036964.D
 Acq On : 26 Sep 2018 1:25
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092018.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Sep 24 10:41:23 2018

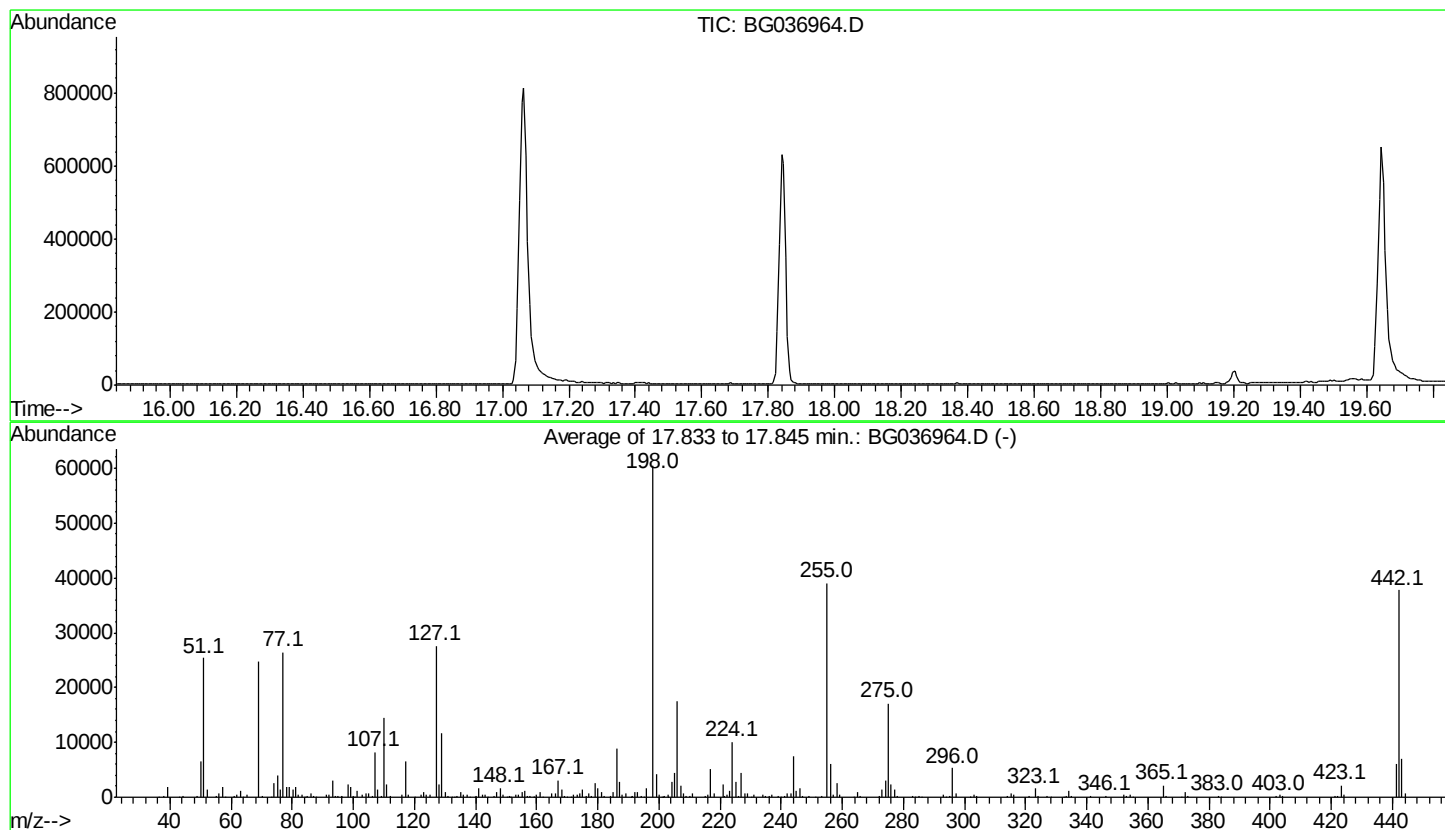

AutoFind: Scans 2475, 2476, 2477; Background Corrected with Scan 2469

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.9	25349	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	40.8	24690	PASS
70	69	0.00	2	0.7	168	PASS
127	198	10	80	45.7	27634	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	60472	PASS
199	198	5	9	7.0	4258	PASS
275	198	10	60	28.3	17140	PASS
365	198	1	100	3.6	2196	PASS
441	198	0.01	100	10.0	6048	PASS
442	198	50	100	62.5	37813	PASS
443	442	15	24	18.4	6943	PASS