


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092520\
 Data File : BG046696.D
 Acq On : 25 Sep 2020 10:38
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092220.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 22 21:47:28 2020

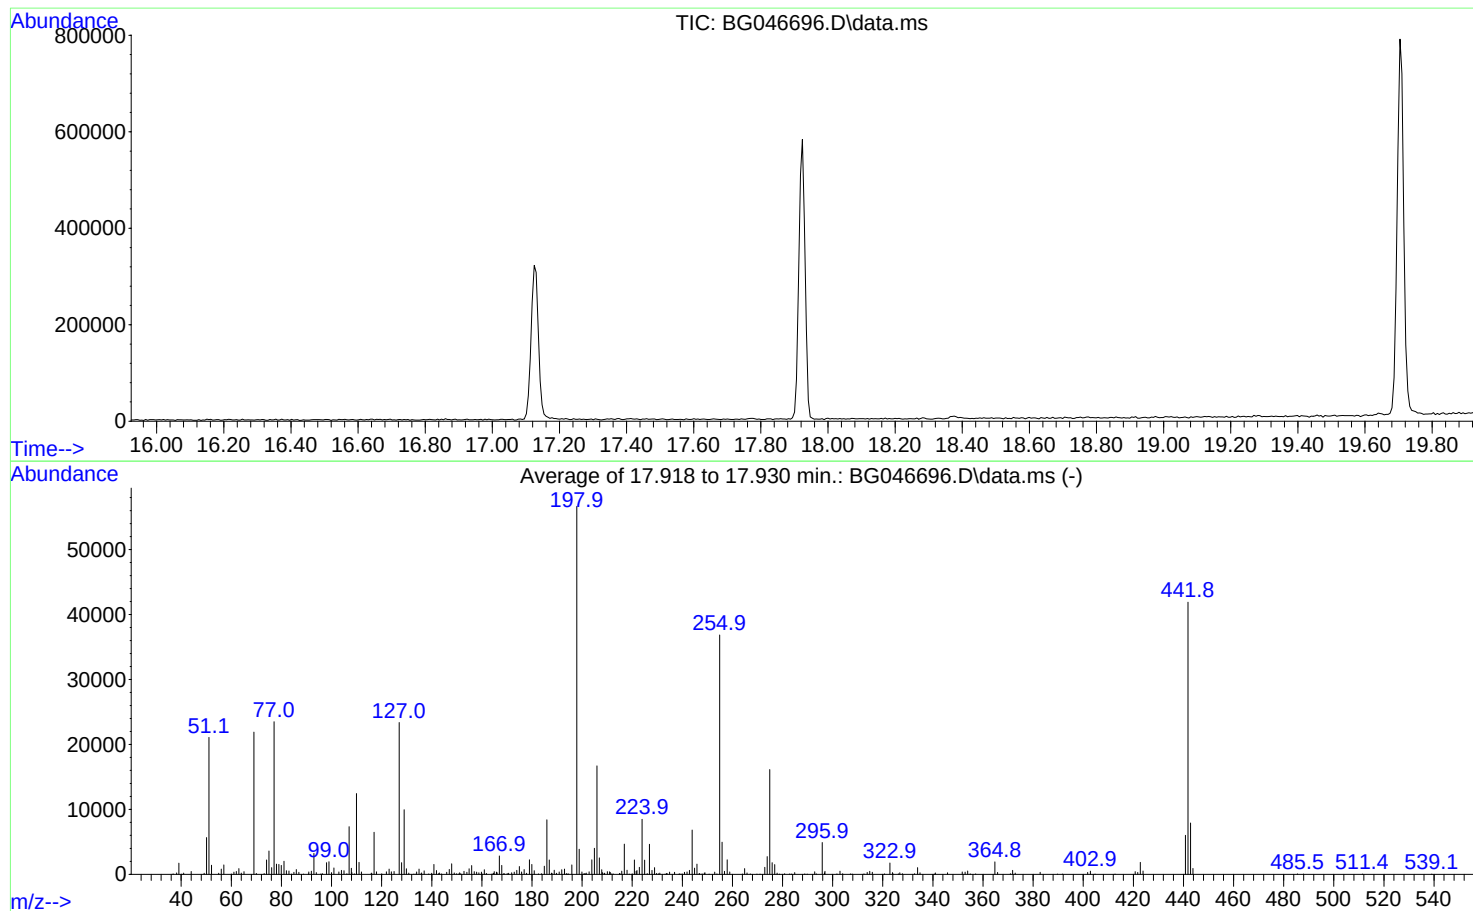

AutoFind: Scans 2524, 2525, 2526; Background Corrected with Scan 2517

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.2	21078	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	38.7	21894	PASS
70	69	0.00	2	0.7	146	PASS
127	198	10	80	41.3	23379	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	56632	PASS
199	198	5	9	6.8	3875	PASS
275	198	10	60	28.5	16126	PASS
365	198	1	100	3.4	1924	PASS
441	198	0.01	100	10.6	6022	PASS
442	198	50	100	74.0	41907	PASS
443	442	15	24	18.9	7914	PASS