
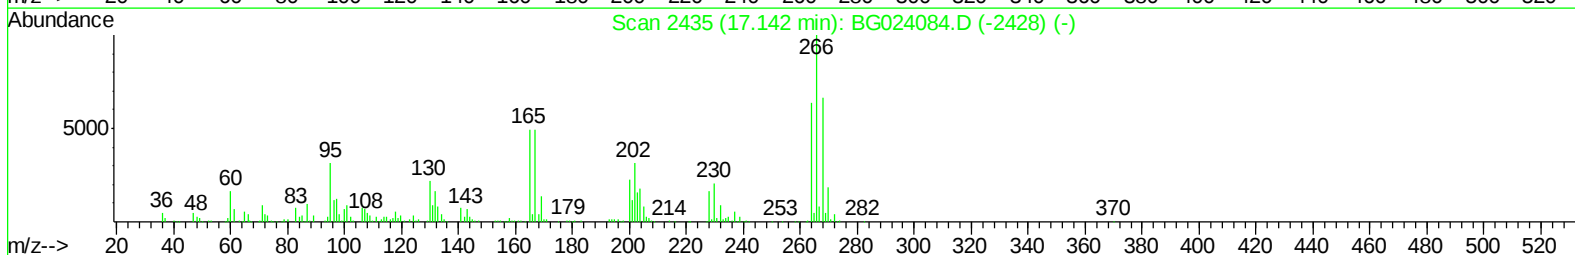
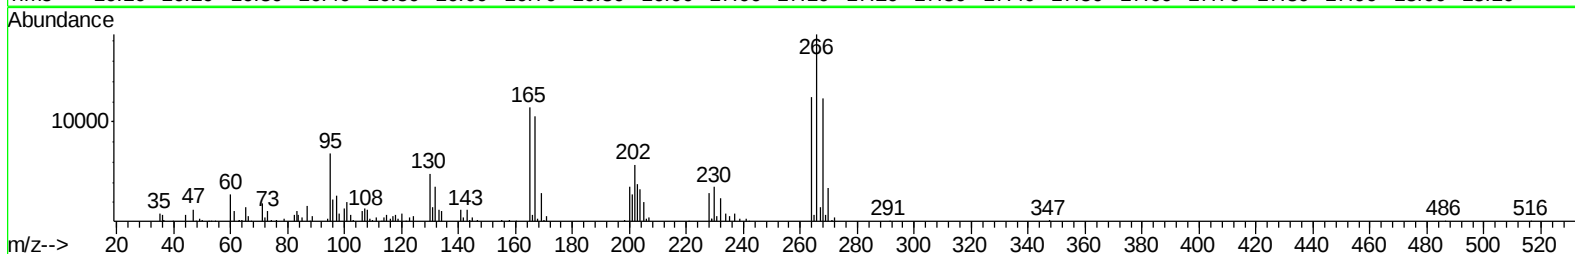


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG092616\
Data File : BG024134.D
Acq On : 26 Sep 2016 9:39
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 27 01:06:30 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG092316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 23 15:35:28 2016
Response via : Initial Calibration

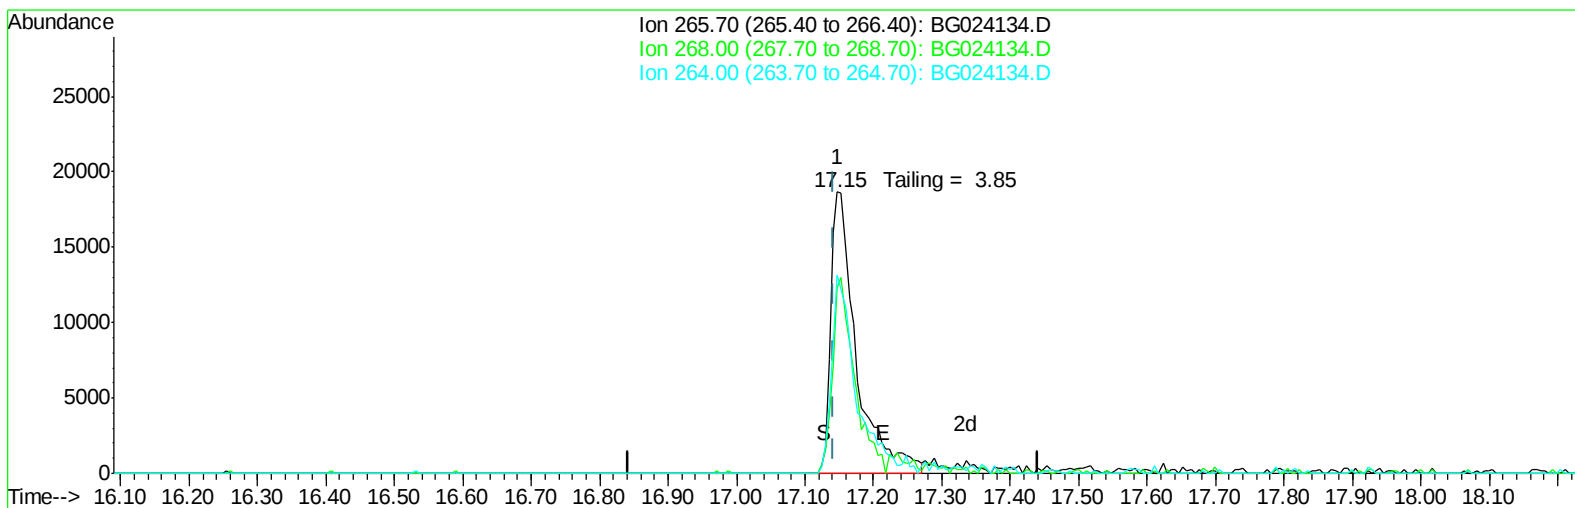

TIC: BG024134.D

(69) Pentachlorophenol (C)




17.147min (+0.005) 109305.75ng

response 45719

Ion	Exp%	Act%
265.70	100	100
268.00	64.90	65.77
264.00	63.20	70.63
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG092616\
Data File : BG024134.D
Acq On : 26 Sep 2016 9:39
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 27 01:06:30 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG092316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 23 15:35:28 2016
Response via : Initial Calibration

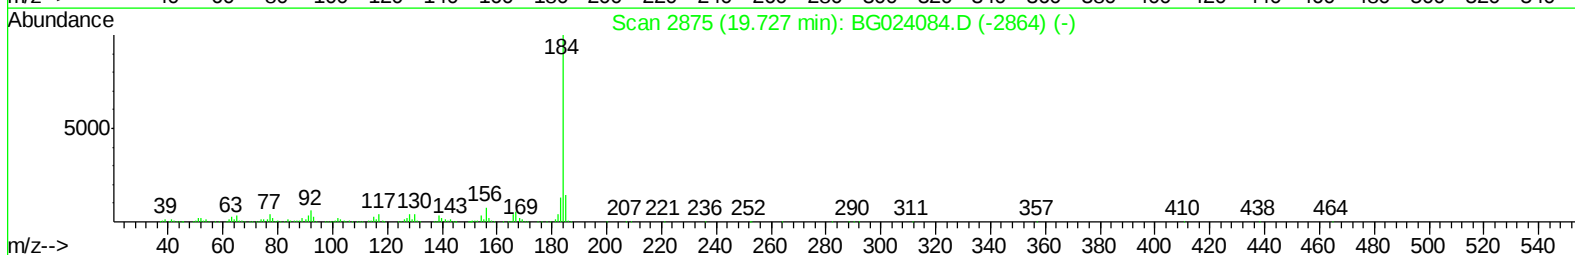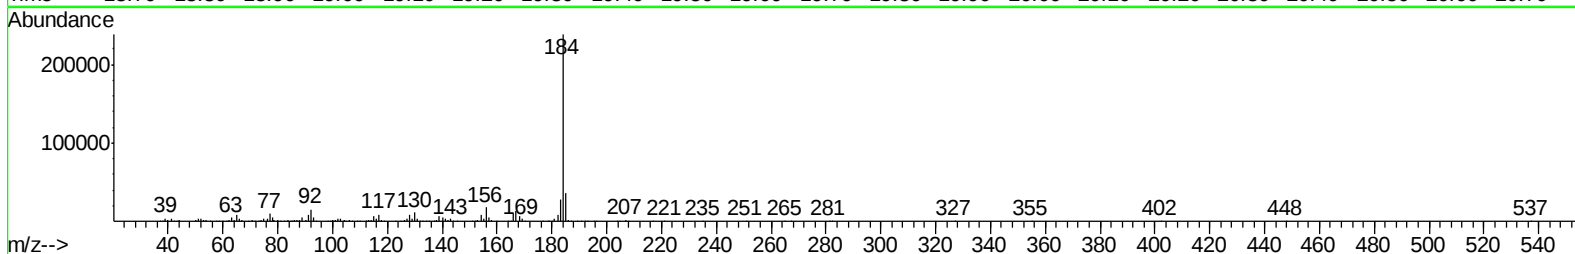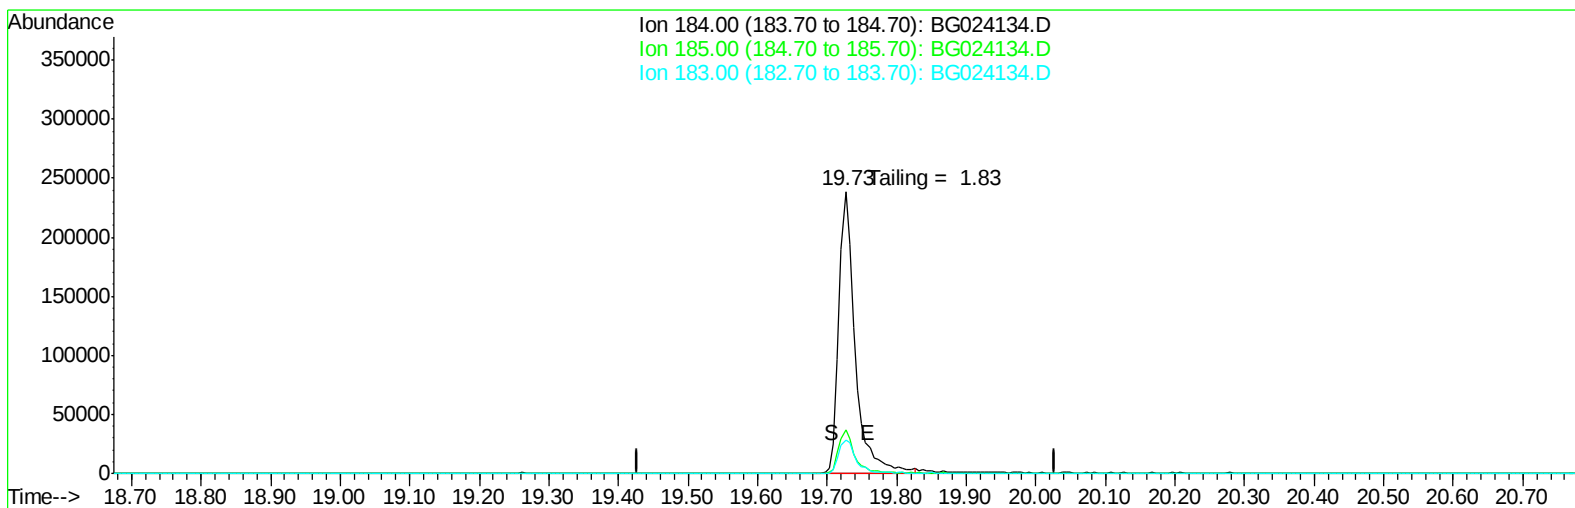

TIC: BG024134.D

(76) Benzidine

19.727min (-19.727) 0.00ng

response 0

Ion	Exp%	Act%
184.00	100	0.00
185.00	15.80	0.00#
183.00	13.40	0.00#
0.00	0.00	0.00