


Data Path : Z:\HPCHEM1\BNA G\DATA\BG092616\
 Data File : BG024134.D
 Acq On : 26 Sep 2016 9:39
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG092316.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 23 15:35:28 2016

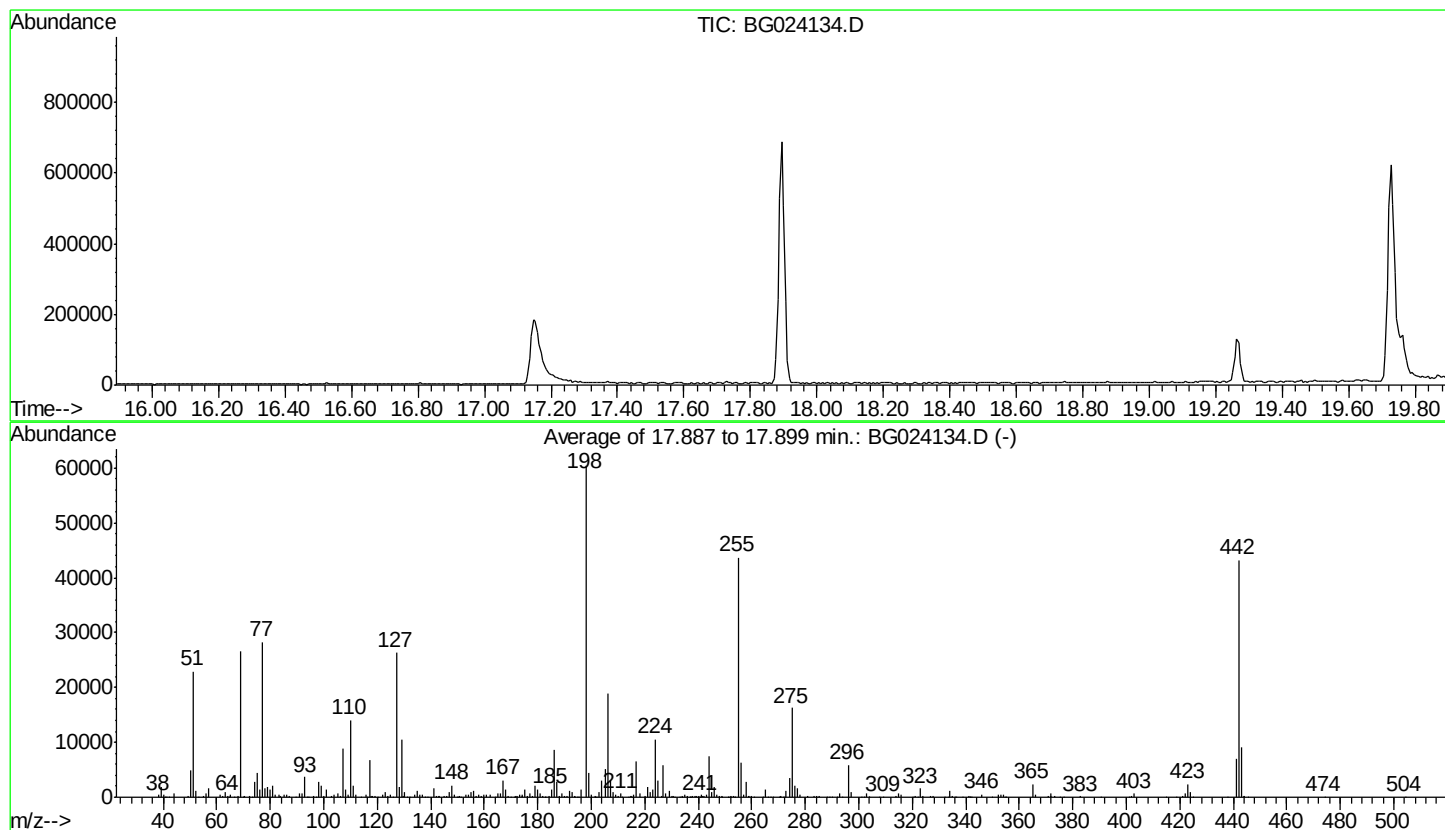

AutoFind: Scans 2562, 2563, 2564; Background Corrected with Scan 2556

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.0	22972	PASS
68	69	0.00	2	1.2	333	PASS
69	198	0.00	100	44.2	26720	PASS
70	69	0.00	2	0.5	130	PASS
127	198	10	80	43.5	26264	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	60442	PASS
199	198	5	9	7.2	4369	PASS
275	198	10	60	27.0	16295	PASS
365	198	1	100	3.9	2339	PASS
441	442	0.01	24	16.4	7096	PASS
442	198	50	100	71.6	43261	PASS
443	442	15	24	20.9	9026	PASS