

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG092618\
 Data File : BG036984.D
 Acq On : 26 Sep 2018 16:35
 Operator : JU/SJ
 Sample : J5068-25
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 CONCRETE-WALL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092018.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.557	211	216	227	rBV2	84190	145494	5.09%	0.927%
2	5.151	311	317	326	rBV	171502	281828	9.86%	1.796%
3	5.621	390	397	415	rBV	467380	880977	30.81%	5.614%
4	7.207	659	667	689	rBV	614401	1274802	44.58%	8.123%
5	7.577	722	730	754	rBV	513787	1027672	35.94%	6.548%
6	8.047	803	810	831	rVB	141653	300987	10.53%	1.918%
7	8.364	857	864	877	rBV	545379	1037746	36.29%	6.612%
8	9.205	999	1007	1029	rBV	418788	894968	31.30%	5.703%
9	10.850	1279	1287	1304	rBV	190195	391302	13.68%	2.493%
10	13.294	1695	1703	1719	rBV	1160263	2034526	71.15%	12.964%
11	13.552	1741	1747	1755	rVB	121037	192441	6.73%	1.226%
12	14.117	1836	1843	1853	rBV	215344	346793	12.13%	2.210%
13	14.669	1929	1937	1954	rBV2	314858	543064	18.99%	3.460%
14	16.155	2180	2190	2208	rBV	409845	731881	25.59%	4.663%
15	17.413	2397	2404	2413	rBV	402399	659784	23.07%	4.204%
16	20.021	2835	2848	2856	rBV	2014687	2859475	100.00%	18.220%
17	21.320	3064	3069	3073	rBV3	29103	45057	1.58%	0.287%
18	21.678	3124	3130	3142	rBV	440841	788786	27.58%	5.026%
19	21.866	3159	3162	3171	rVB	24295	36136	1.26%	0.230%
20	22.471	3261	3265	3271	rBV3	26884	43059	1.51%	0.274%
21	23.159	3377	3382	3389	rVB	41643	73328	2.56%	0.467%
22	23.347	3409	3414	3421	rBV	32872	65083	2.28%	0.415%
23	23.964	3513	3519	3528	rVB3	38812	94876	3.32%	0.605%
24	24.886	3666	3676	3695	rVB2	282183	871143	30.47%	5.551%
25	26.014	3863	3868	3877	rVB3	25574	72672	2.54%	0.463%


Sum of corrected areas: 15693880

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG092618\
Data File : BG036984.D
Acq On : 26 Sep 2018 16:35
Operator : JU/SJ
Sample : J5068-25
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
CONCRETE-WALL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG092018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

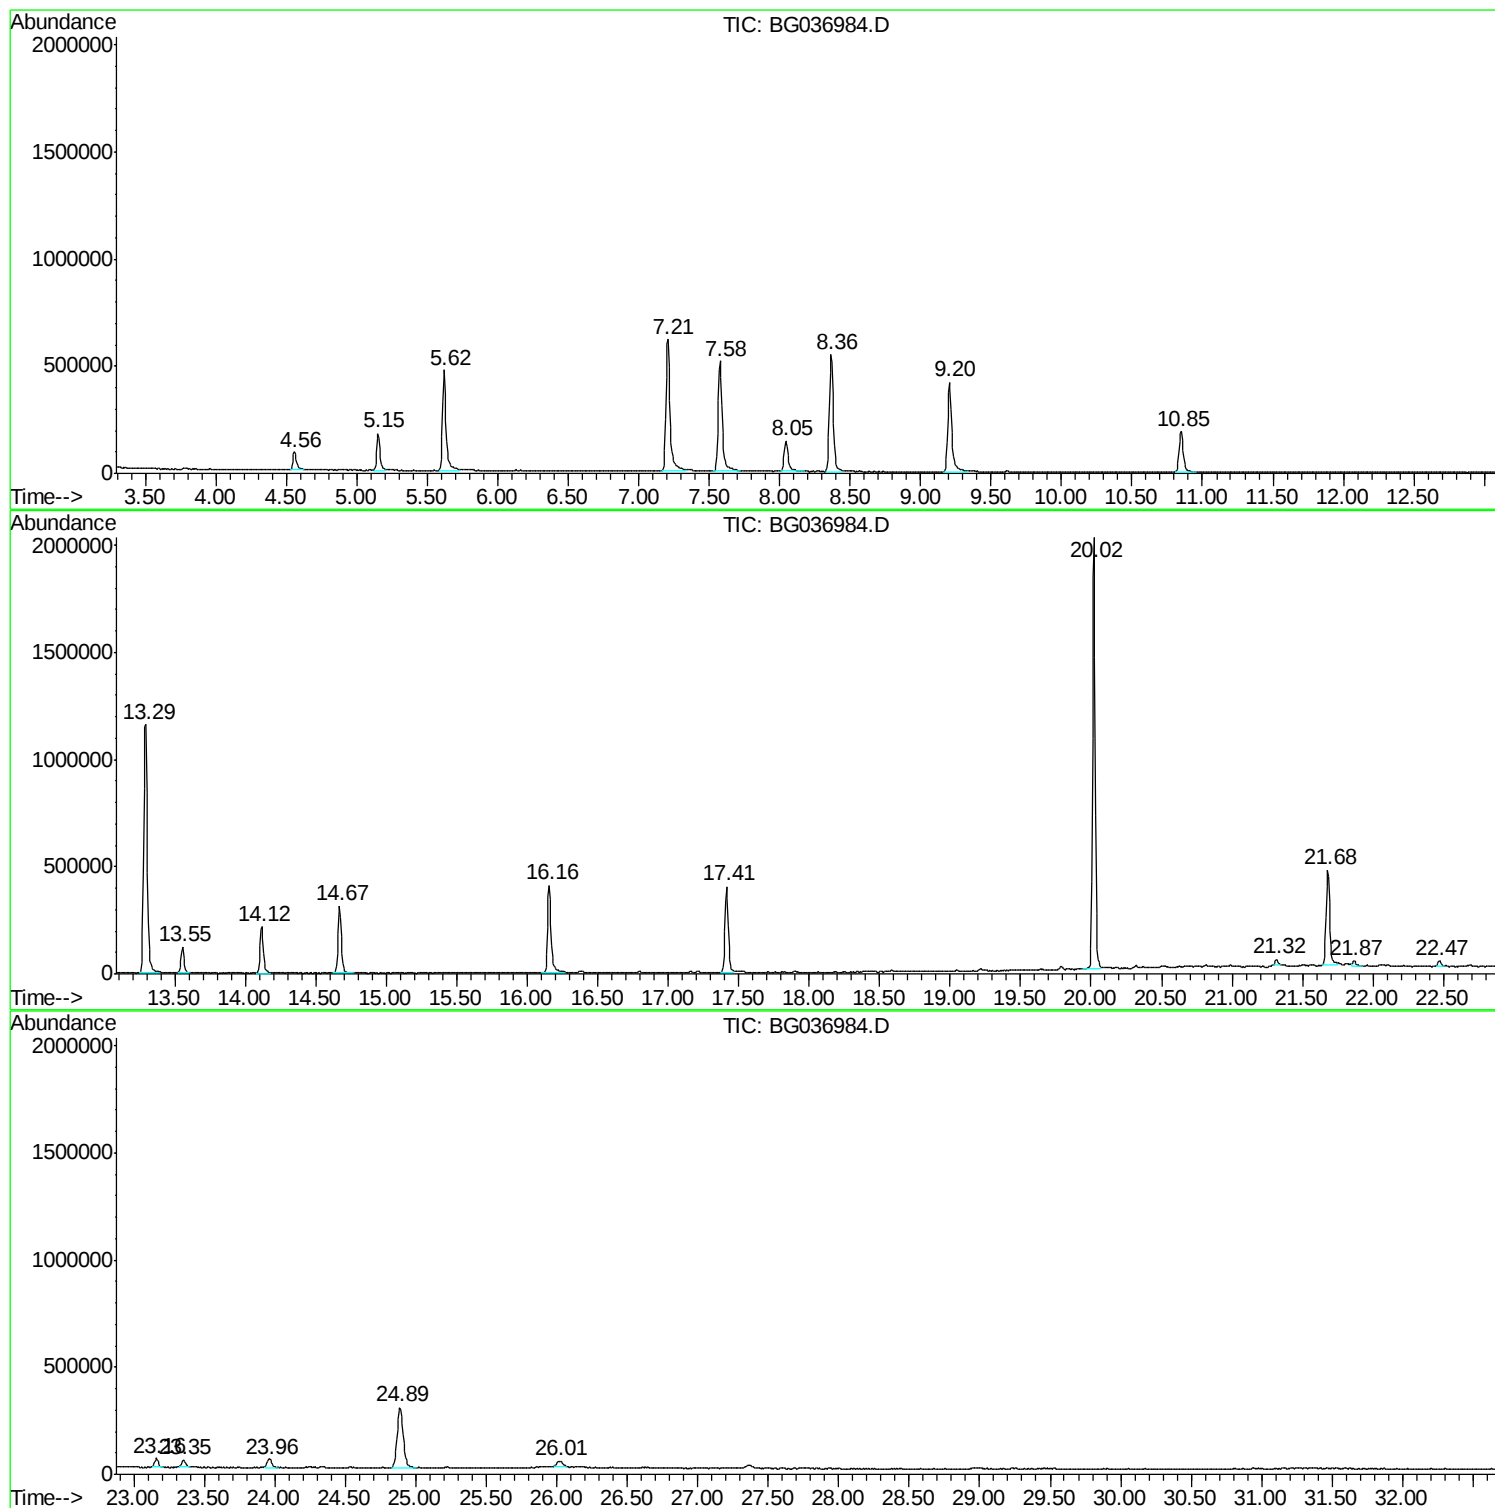

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG092618\\
Data_File : BG036984.D
Acq_On : 26-Sep-2018 16:355
Operator : JU/SJJ
Sample : J5068-255
Misc :
ALS_Vial : 5 Sample_Multiplier: 11

Instrument :
BNA_G
ClientSampleId :
CONCRETE-WALL

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092018.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\Database\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
				#	RT Resp Conc

No Library Search Compounds Detected
