


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG092618\
 Data File : BG036980.D
 Acq On : 26 Sep 2018 14:00
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092018.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Sep 24 10:41:23 2018

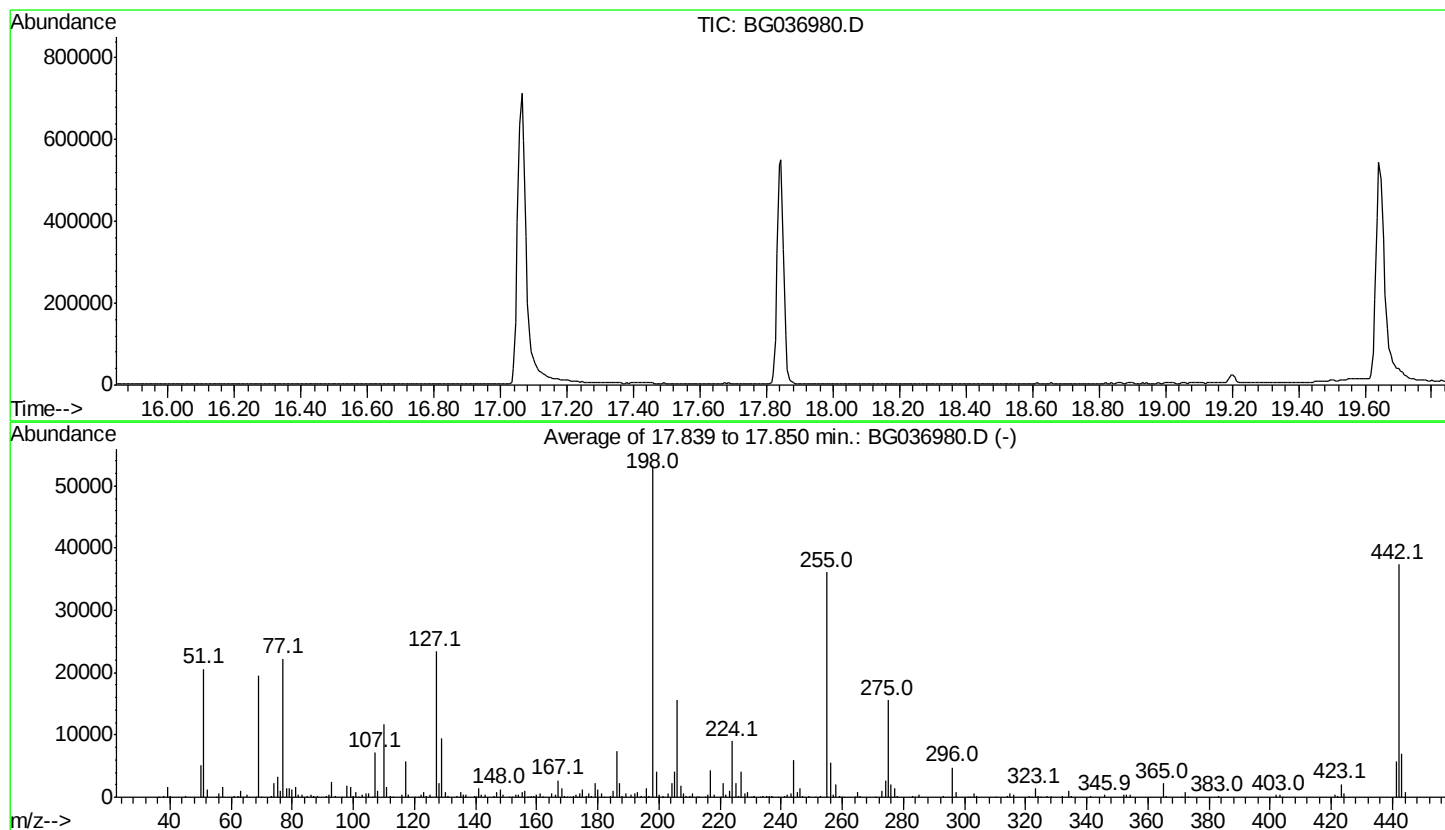

AutoFind: Scans 2476, 2477, 2478; Background Corrected with Scan 2469

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.7	20630	PASS
68	69	0.00	2	0.4	69	PASS
69	198	0.00	100	36.7	19532	PASS
70	69	0.00	2	0.3	66	PASS
127	198	10	80	43.9	23399	PASS
197	198	0.00	2	0.5	251	PASS
198	198	100	100	100.0	53258	PASS
199	198	5	9	7.6	4040	PASS
275	198	10	60	29.2	15568	PASS
365	198	1	100	4.1	2170	PASS
441	198	0.01	100	11.0	5850	PASS
442	198	50	100	70.1	37360	PASS
443	442	15	24	18.8	7015	PASS