


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG092618\
 Data File : BG036999.D
 Acq On : 27 Sep 2018 2:58
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092018.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Sep 24 10:41:23 2018

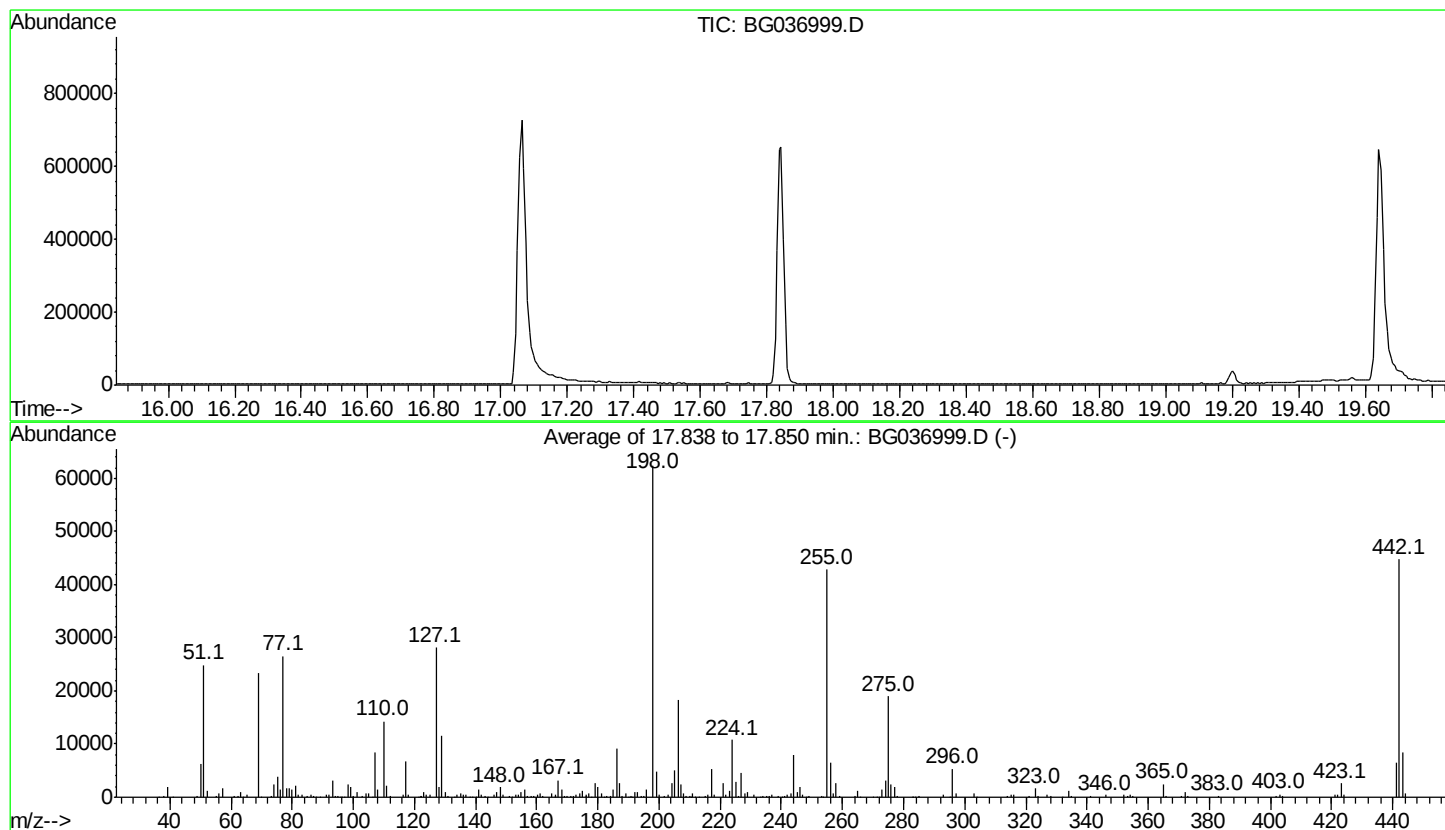

AutoFind: Scans 2476, 2477, 2478; Background Corrected with Scan 2469

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.8	24823	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	37.3	23256	PASS
70	69	0.00	2	0.3	65	PASS
127	198	10	80	45.0	28096	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	62373	PASS
199	198	5	9	7.8	4867	PASS
275	198	10	60	30.4	18941	PASS
365	198	1	100	4.0	2511	PASS
441	198	0.01	100	10.6	6626	PASS
442	198	50	100	71.7	44709	PASS
443	442	15	24	18.8	8419	PASS