

Data Path : Z:\HPCHEM1\BNA G\DATA\BG092717\
 Data File : BG028956.D
 Acq On : 27 Sep 2017 23:43
 Operator : SJ/JU
 Sample : I5444-06
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BU-03-092617

Quant Time: Sep 28 01:29:56 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG091217.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 12 16:57:11 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.28	152	29812	20.00	ng	-0.05
21) Naphthalene-d8	11.10	136	113389	20.00	ng	-0.05
38) Acenaphthene-d10	14.89	164	83943	20.00	ng	-0.05
63) Phenanthrene-d10	17.65	188	255394	20.00	ng	-0.05
75) Chrysene-d12	21.97	240	306035	20.00	ng	-0.07
86) Perylene-d12	25.42	264	305932	20.00	ng	-0.11
System Monitoring Compounds						
5) 2-Fluorophenol	5.85	112	223555	123.73	ng	-0.05
7) Phenol-d6	7.44	99	281286	103.40	ng	-0.05
23) Nitrobenzene-d5	9.45	82	202393	85.39	ng	-0.05
41) 2,4,6-Tribromophenol	16.38	330	214984	154.85	ng	-0.05
44) 2-Fluorobiphenyl	13.52	172	535483	85.06	ng	-0.05
78) Terphenyl-d14	20.23	244	1316666	91.75	ng	-0.05
Target Compounds						
40) Hexachlorocyclopentadiene	13.15	237	61	7.644	ng	# 29
53) 2,4-Dinitrophenol	15.21	184	188	8.206	ng	# 15

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG092717\
Data File : BG028956.D
Acq On : 27 Sep 2017 23:43
Operator : SJ/JU
Sample : I5444-06
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BU-03-092617

Quant Time: Sep 28 01:29:56 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG091217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 16:57:11 2017
Response via : Initial Calibration

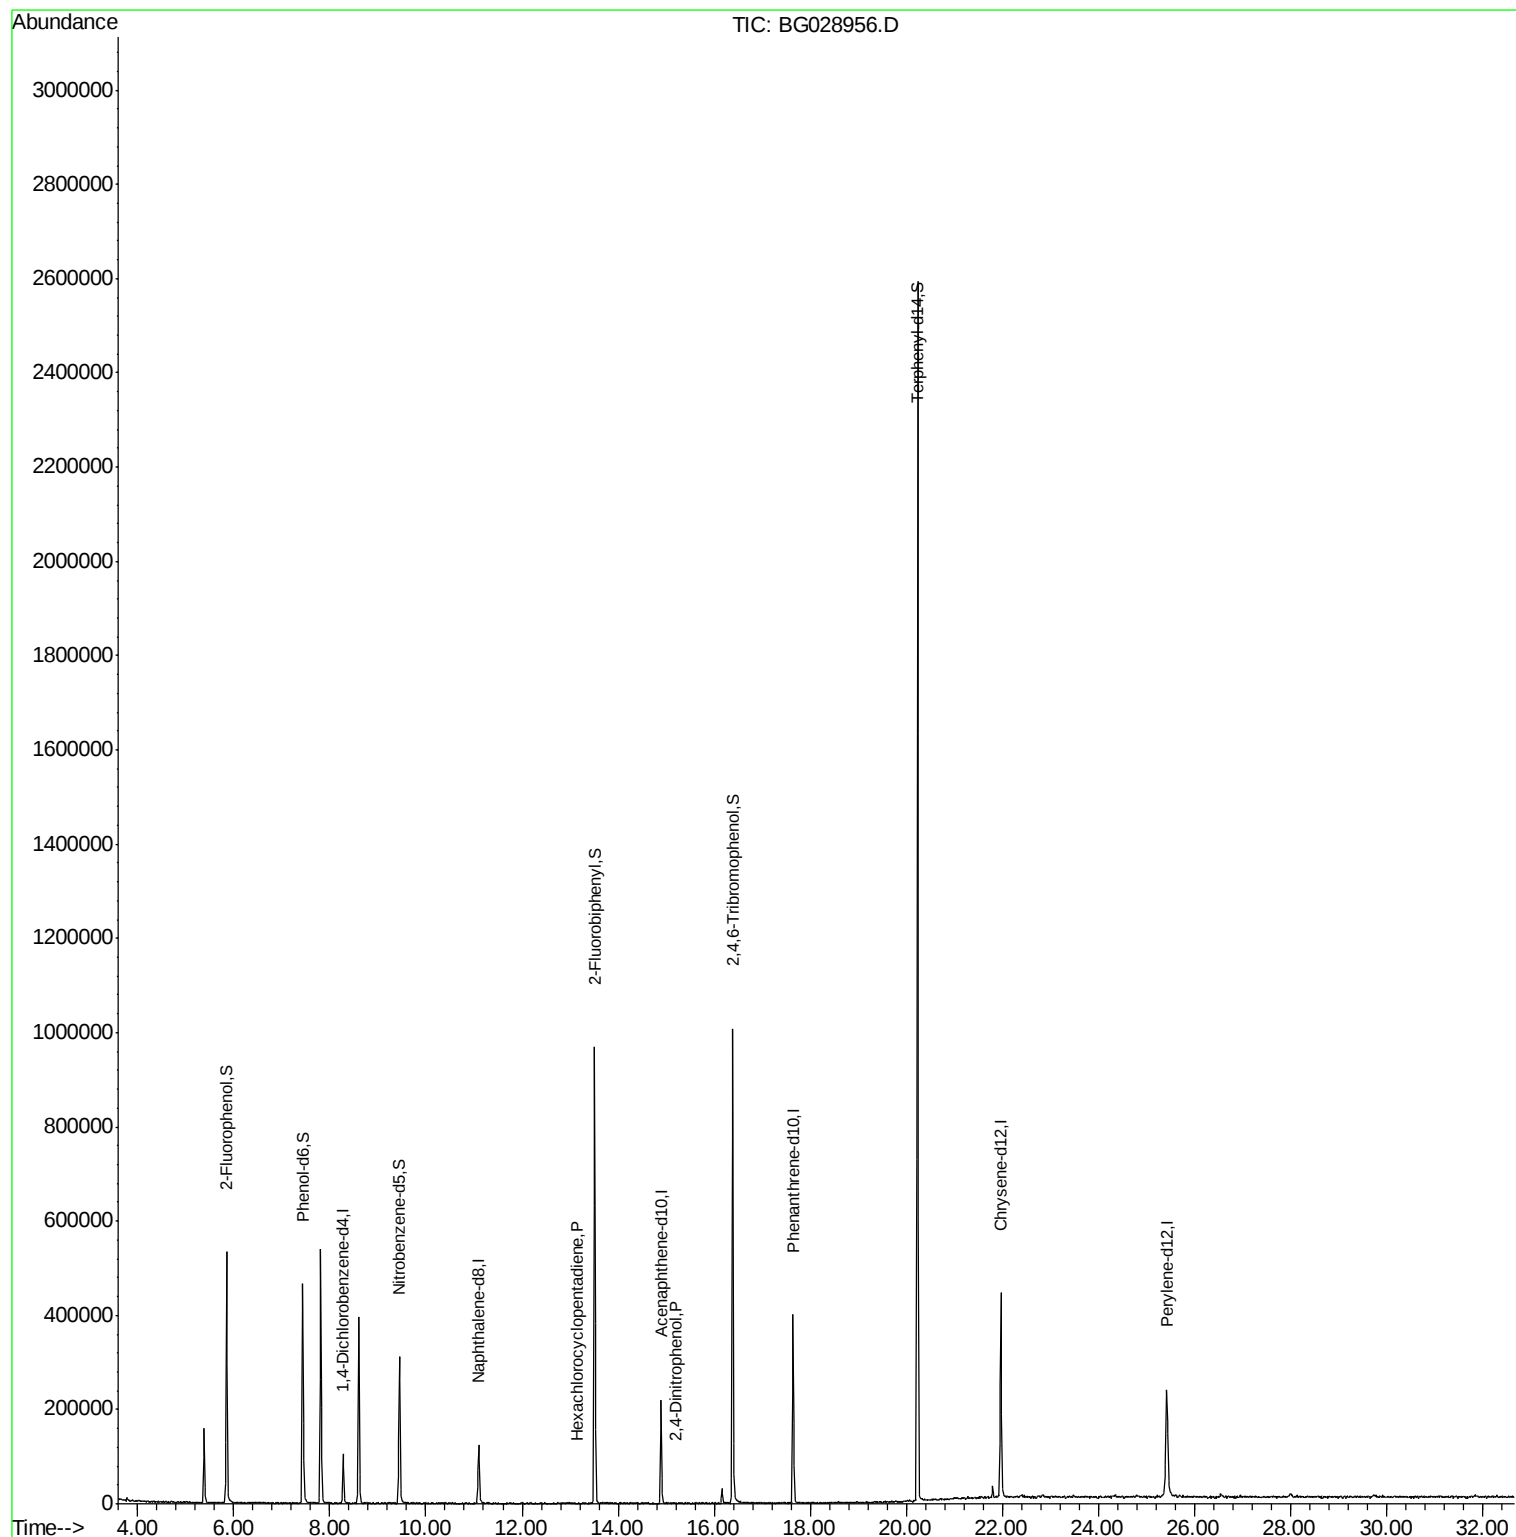



#1

1,4-Dichlorobenzene-d4

Concen: 20.000 ng

RT: 8.28 min Scan# 799

Delta R.T. -0.05 min

Lab File: BG028956.D

Acq: 27 Sep 2017 23:43

Instrument :

BNA_G

ClientSampleId :

BU-03-092617


Tot Ion:152 Resp: 29812

Ion Ratio Lower Upper

152 100

150 133.6 114.0 171.0




115 55.7 48.1 72.1

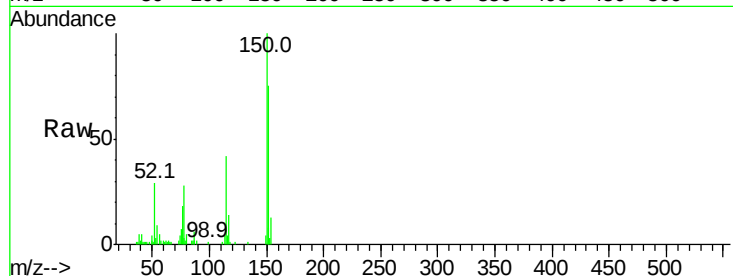

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

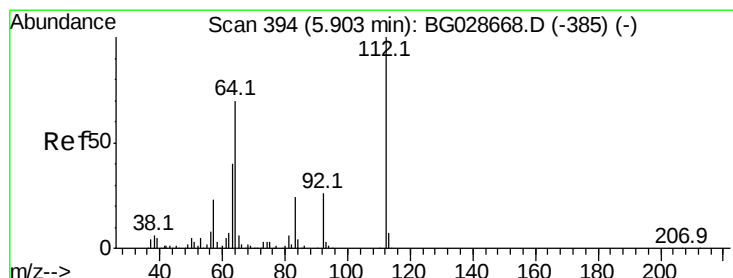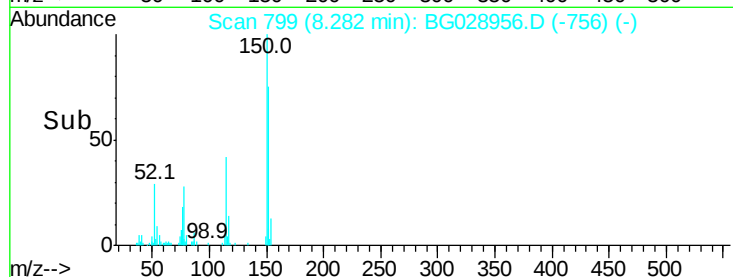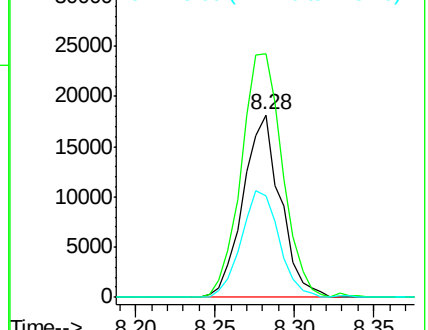

#5

2-Fluorophenol

Concen: 123.734 ng

RT: 5.85 min Scan# 385

Delta R.T. -0.05 min

Lab File: BG028956.D

Acq: 27 Sep 2017 23:43


Tgt Ion:112 Resp: 223555

Ion Ratio Lower Upper

112 100

64 73.5 61.8 92.6



63 39.0 37.2 55.8

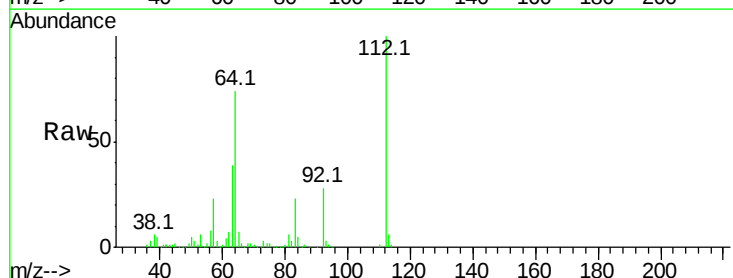


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BGC

Ion 63.00 (62.70 to 63.70): BGC

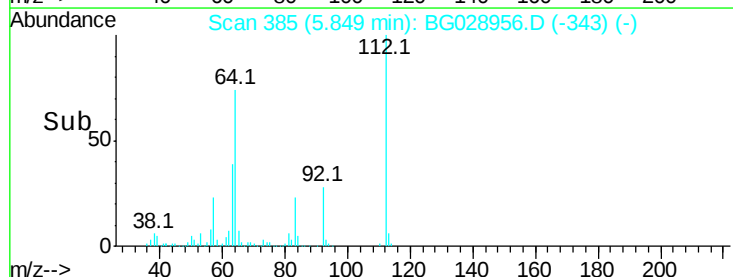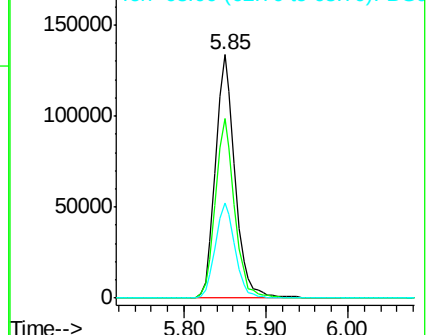

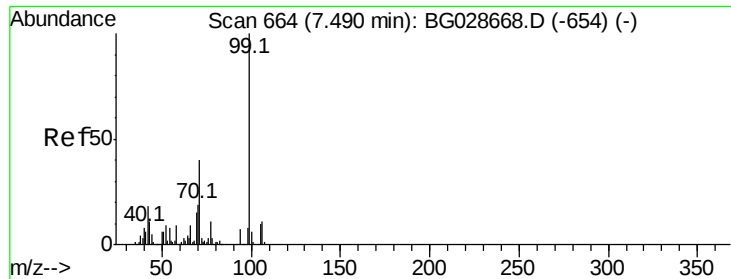

#7

Phenol-d6

Concen: 103.404 ng

RT: 7.44 min Scan# 655

Delta R.T. -0.05 min

Lab File: BG028956.D

Acq: 27 Sep 2017 23:43

Instrument :

BNA_G

ClientSampleId :

BU-03-092617


Tot Ion: 99 Resp: 281286

Ion Ratio Lower Upper

99 100

42 19.5 20.5 30.7#




71 39.3 37.6 56.4

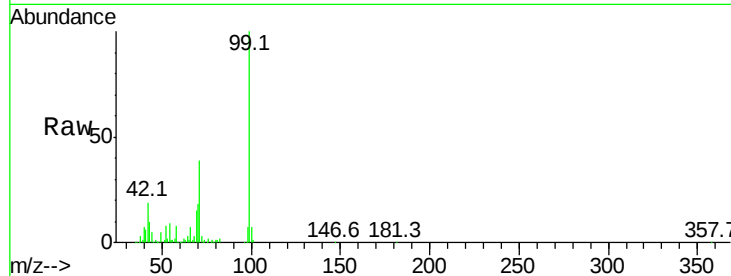

Abundance Ion 99.00 (98.70 to 99.70): BGC

Ion 42.00 (41.70 to 42.70): BGC

Ion 71.00 (70.70 to 71.70): BGC

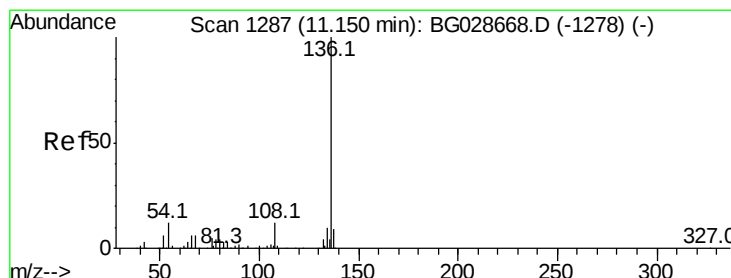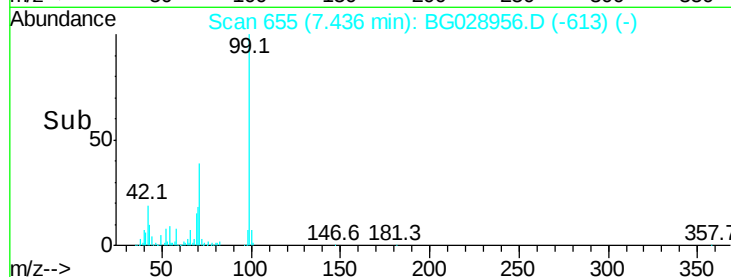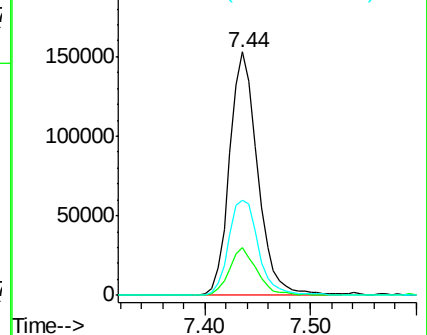

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 11.10 min Scan# 1278

Delta R.T. -0.05 min

Lab File: BG028956.D

Acq: 27 Sep 2017 23:43

Tgt Ion: 136 Resp: 113389


Ion Ratio Lower Upper

136 100

137 11.3 8.9 13.3

54 12.5 9.3 13.9

68 5.2 5.1 7.7


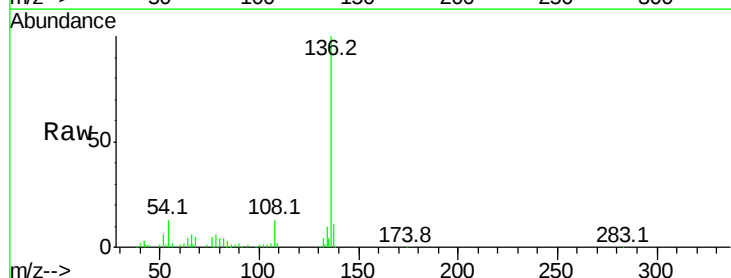



Abundance Ion 136.00 (135.70 to 136.70): BGC

Ion 137.00 (136.70 to 137.70): BGC

Ion 54.00 (53.70 to 54.70): BGC

Ion 68.00 (67.70 to 68.70): BGC



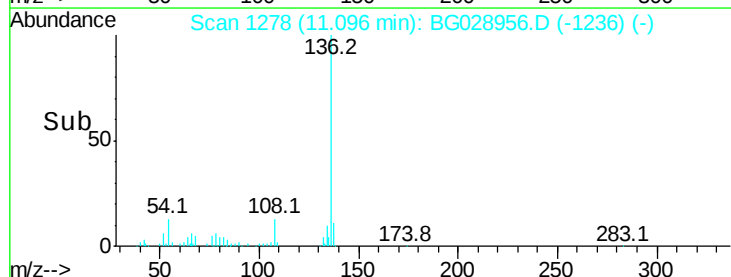
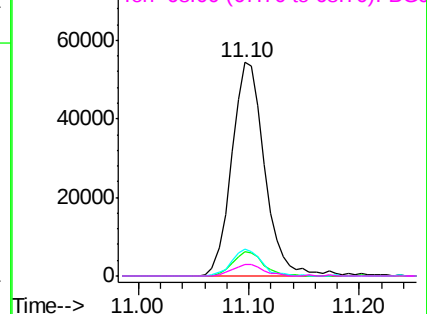


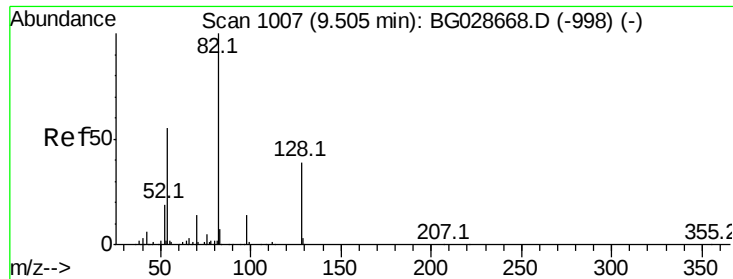

#23
 Nitrobenzene-d5
 Concen: 85.387 ng
 RT: 9.45 min Scan# 998
 Delta R.T. -0.05 min
 Lab File: BG028956.D
 Acq: 27 Sep 2017 23:43




Instrument :
 BNA_G
 ClientSampleId :
 BU-03-092617


Tot Ion	82	Resp	202393
Ion	Ratio	Lower	Upper
82	100		
128	37.7	26.4	39.6
54	58.3	49.4	74.2

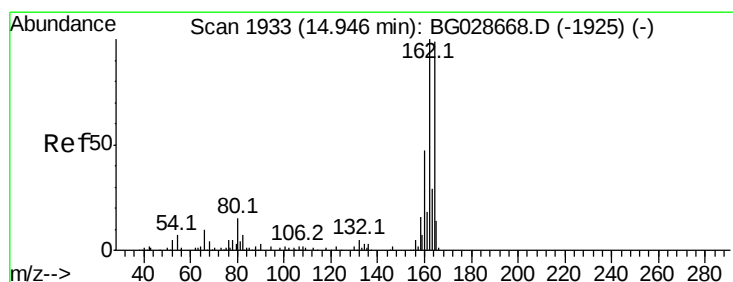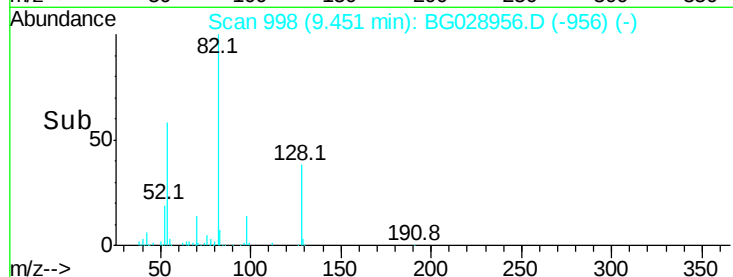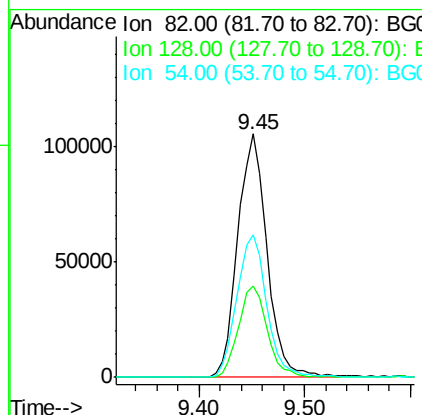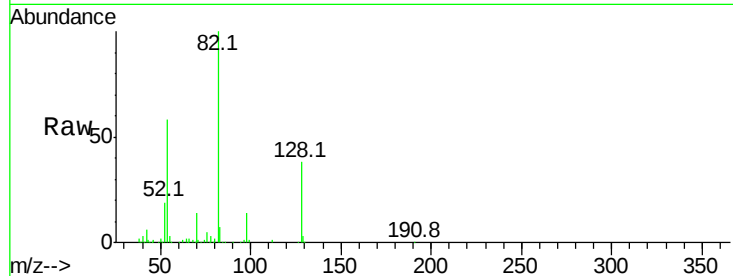

#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.89 min Scan# 1924
 Delta R.T. -0.05 min
 Lab File: BG028956.D
 Acq: 27 Sep 2017 23:43

Tgt Ion	164	Resp	83943
Ion	Ratio	Lower	Upper
164	100		
162	98.6	85.1	127.7
160	40.4	34.7	52.1

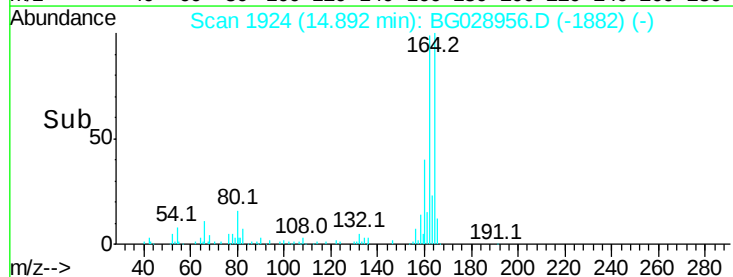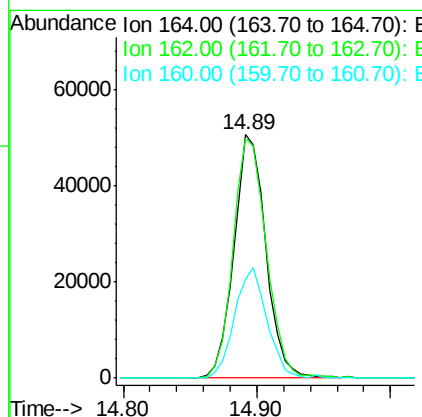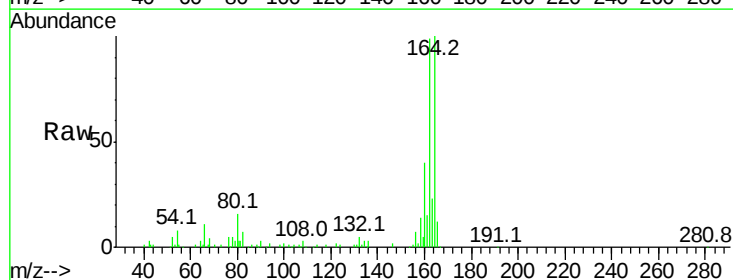


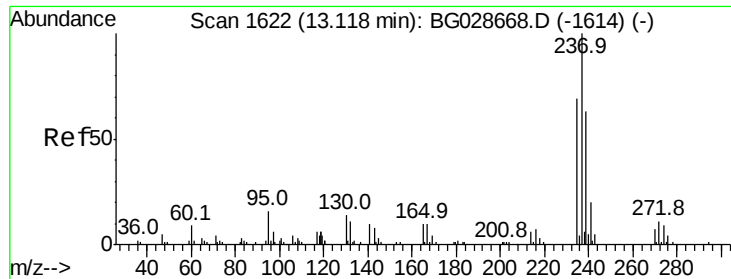




#40
Hexachlorocyclopentadiene
Concen: 7.644 ng
RT: 13.15 min Scan# 1627
Delta R.T. 0.03 min
Lab File: BG028956.D
Acq: 27 Sep 2017 23:43

Instrument :
BNA_G
ClientSampleId :
BU-03-092617

Tot Ion:237 Resp: 61
Ion Ratio Lower Upper
237 100
235 0.0 39.4 79.4#
272 0.0 0.0 32.0

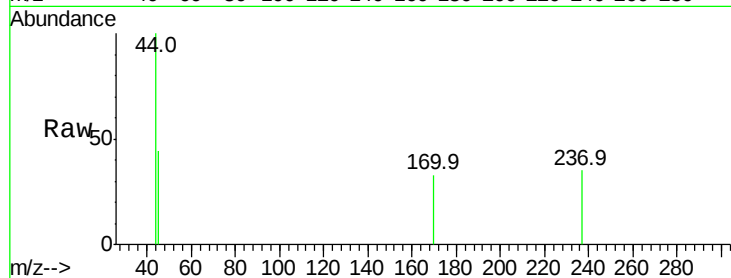


Abundance Ion 236.80 (236.50 to 237.50): E
Ion 234.90 (234.60 to 235.60): E
Ion 271.75 (271.45 to 272.45): E

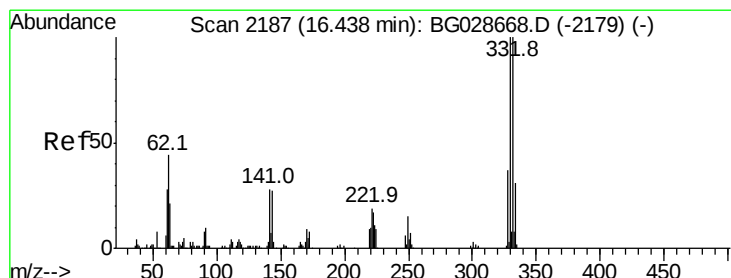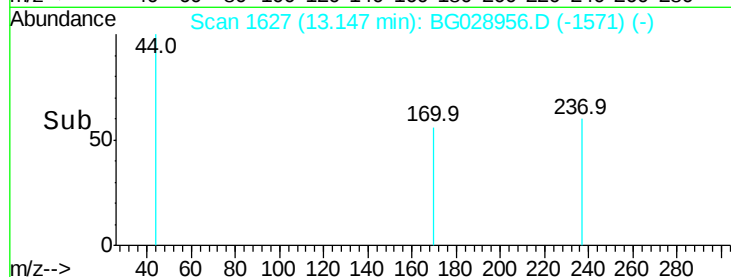
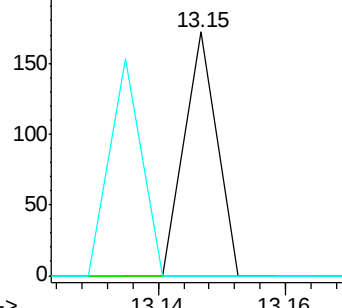



#41
2,4,6-Tribromophenol
Concen: 154.847 ng
RT: 16.38 min Scan# 2178
Delta R.T. -0.05 min
Lab File: BG028956.D
Acq: 27 Sep 2017 23:43

Tgt Ion:330 Resp: 214984
Ion Ratio Lower Upper
330 100
332 96.4 77.3 115.9
141 30.2 32.1 48.1#

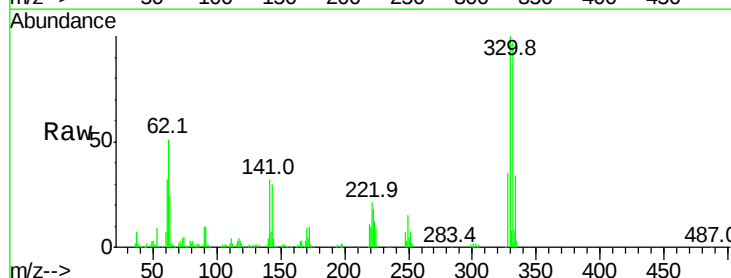

Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E



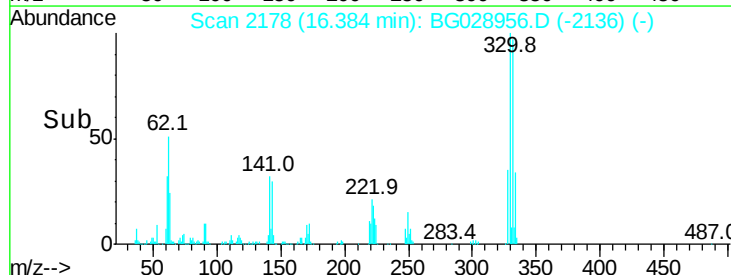
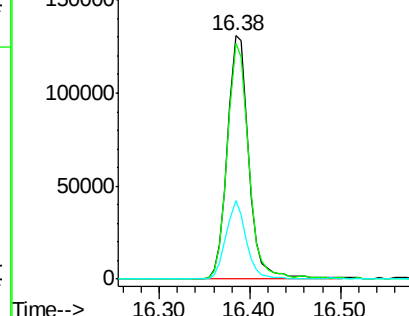


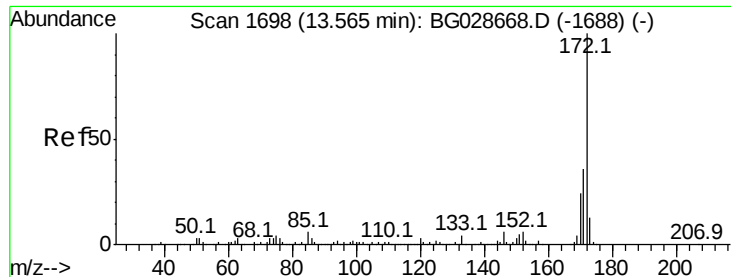

#44
2-Fluorobiphenyl
Concen: 85.061 ng
RT: 13.52 min Scan# 1690
Delta R.T. -0.05 min
Lab File: BG028956.D
Acq: 27 Sep 2017 23:43




Instrument :
BNA_G
ClientSampleId :
BU-03-092617


Tot Ion:172 Resp: 535483
Ion Ratio Lower Upper
172 100
171 35.9 32.2 48.2
170 23.1 21.8 32.6

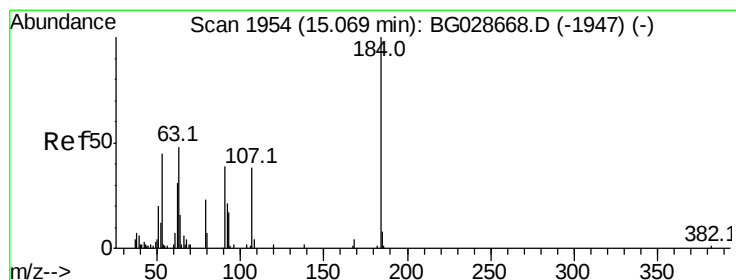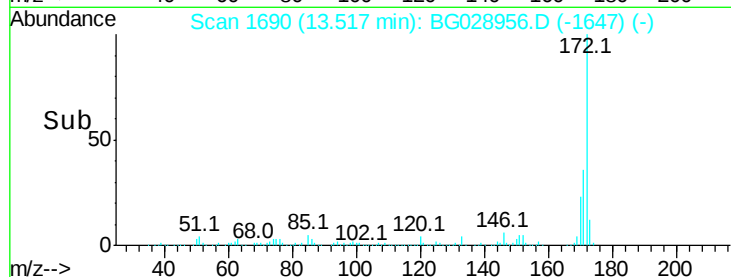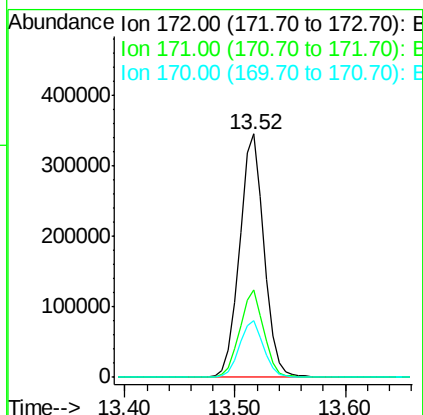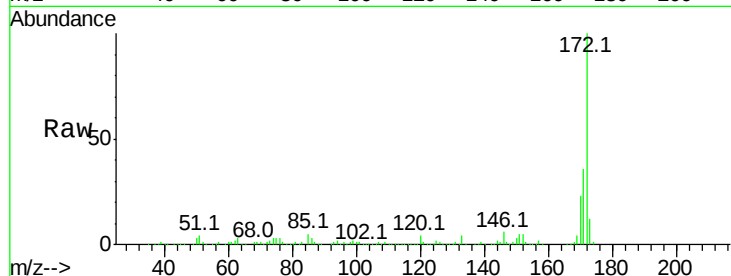

#53
2,4-Dinitrophenol
Concen: 8.206 ng
RT: 15.21 min Scan# 1978
Delta R.T. 0.14 min
Lab File: BG028956.D
Acq: 27 Sep 2017 23:43

Tgt Ion:184 Resp: 188
Ion Ratio Lower Upper
184 100
63 0.0 52.7 79.1#
154 0.0 57.3 85.9#

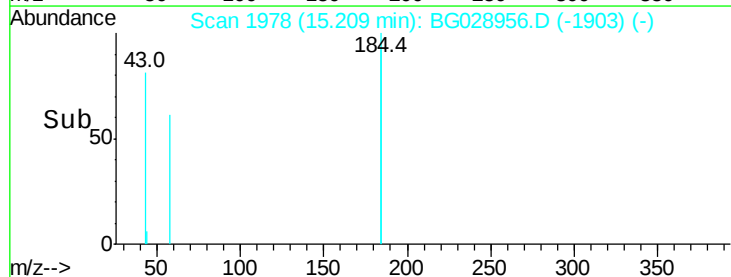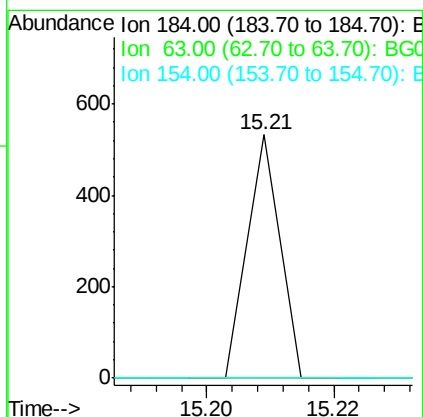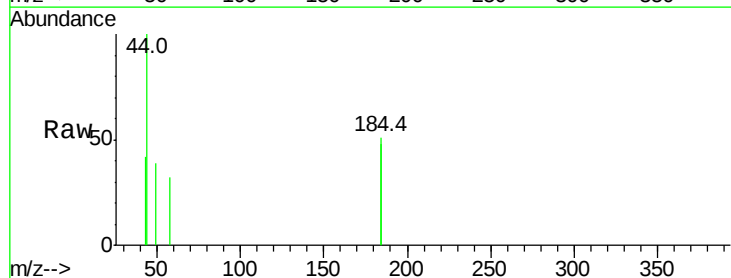

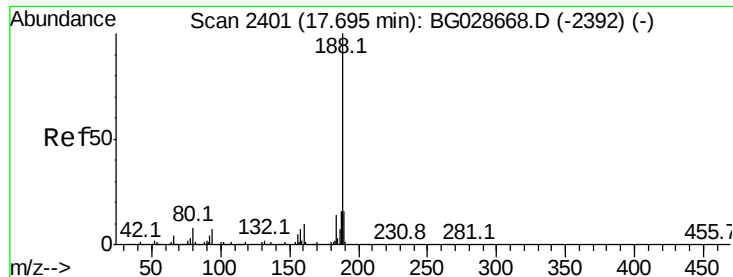

#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.65 min Scan# 2393

Delta R.T. -0.05 min

Lab File: BG028956.D

Acq: 27 Sep 2017 23:43

Instrument :

BNA_G

ClientSampleId :

BU-03-092617


Tot Ion:188 Resp: 255394

Ion Ratio Lower Upper

188 100

94 6.5 5.8 8.8




80 6.9 7.5 11.3#

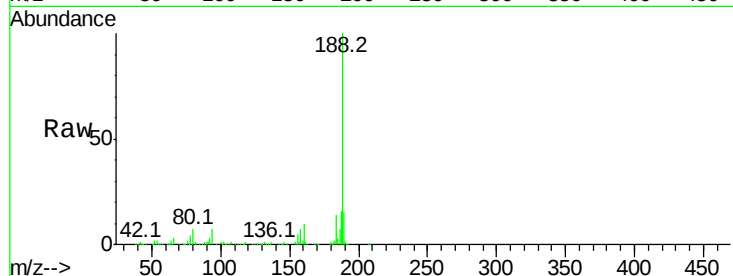

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): B

Ion 80.00 (79.70 to 80.70): B

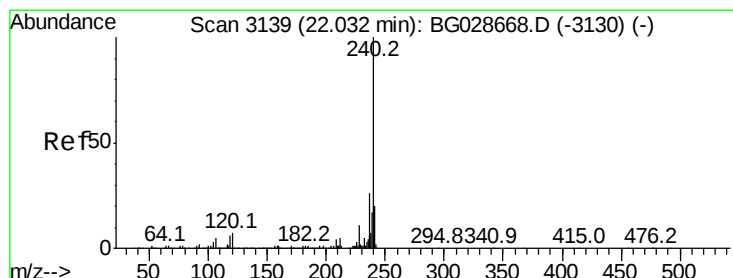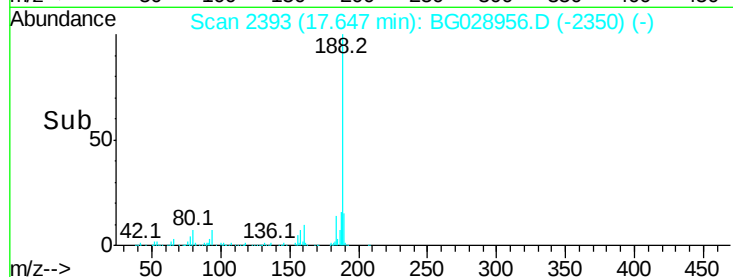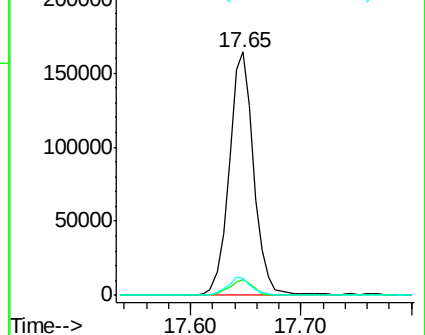

#75

Chrysene-d12

Concen: 20.000 ng

RT: 21.97 min Scan# 3128

Delta R.T. -0.07 min

Lab File: BG028956.D

Acq: 27 Sep 2017 23:43


Tgt Ion:240 Resp: 306035

Ion Ratio Lower Upper

240 100

120 7.2 5.7 8.5



236 25.9 22.2 33.4

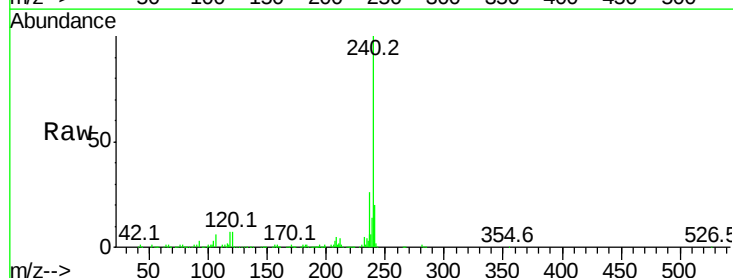


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

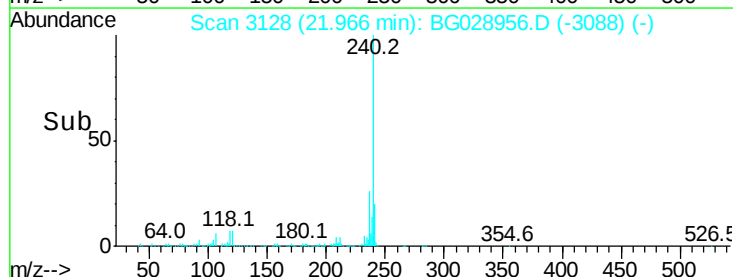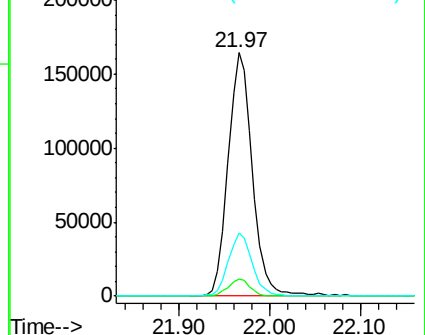

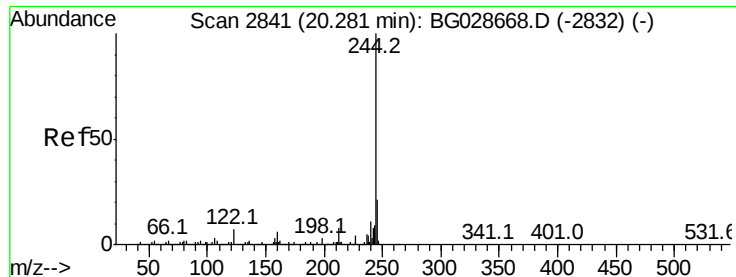

#78

Terphenyl-d14

Concen: 91.750 ng

RT: 20.23 min Scan# 2833

Delta R.T. -0.05 min

Lab File: BG028956.D

Acq: 27 Sep 2017 23:43

Instrument :


BNA_G

ClientSampleId :

BU-03-092617

Tot Ion:244 Resp: 1316666

Ion	Ratio	Lower	Upper
244	100		
212	7.8	10.0	15.0#
122	7.3	8.6	12.8#



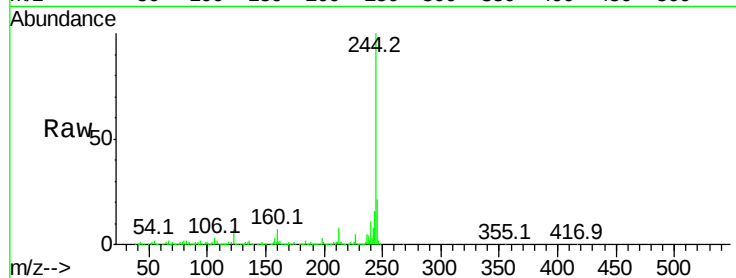


Abundance

Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

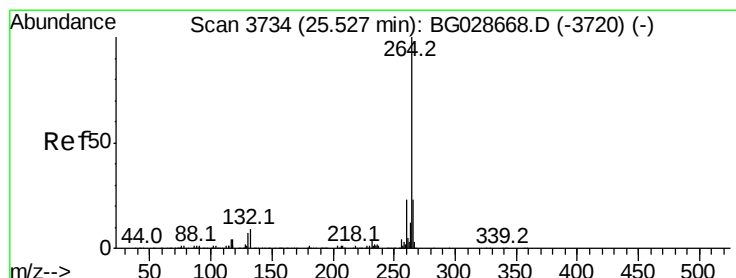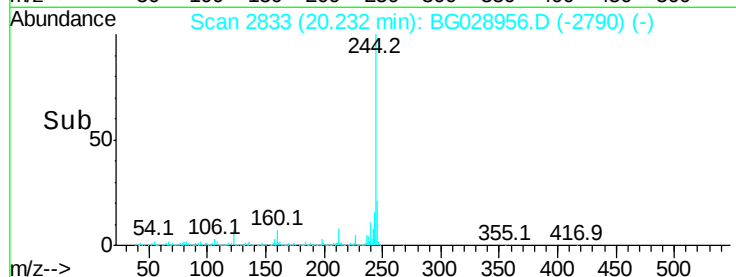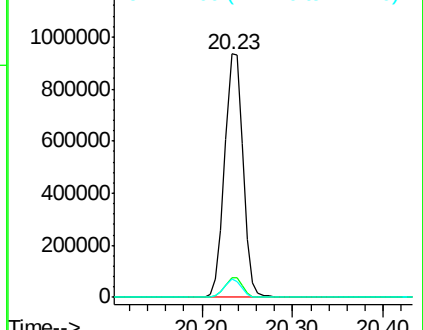

#86

Perylene-d12

Concen: 20.000 ng

RT: 25.42 min Scan# 3716


Delta R.T. -0.11 min

Lab File: BG028956.D

Acq: 27 Sep 2017 23:43

Tgt Ion:264 Resp: 305932

Ion	Ratio	Lower	Upper
264	100		
260	24.2	21.8	32.8
265	21.9	18.2	27.4

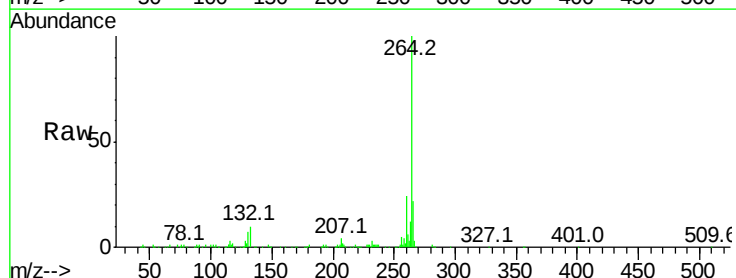

Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

