
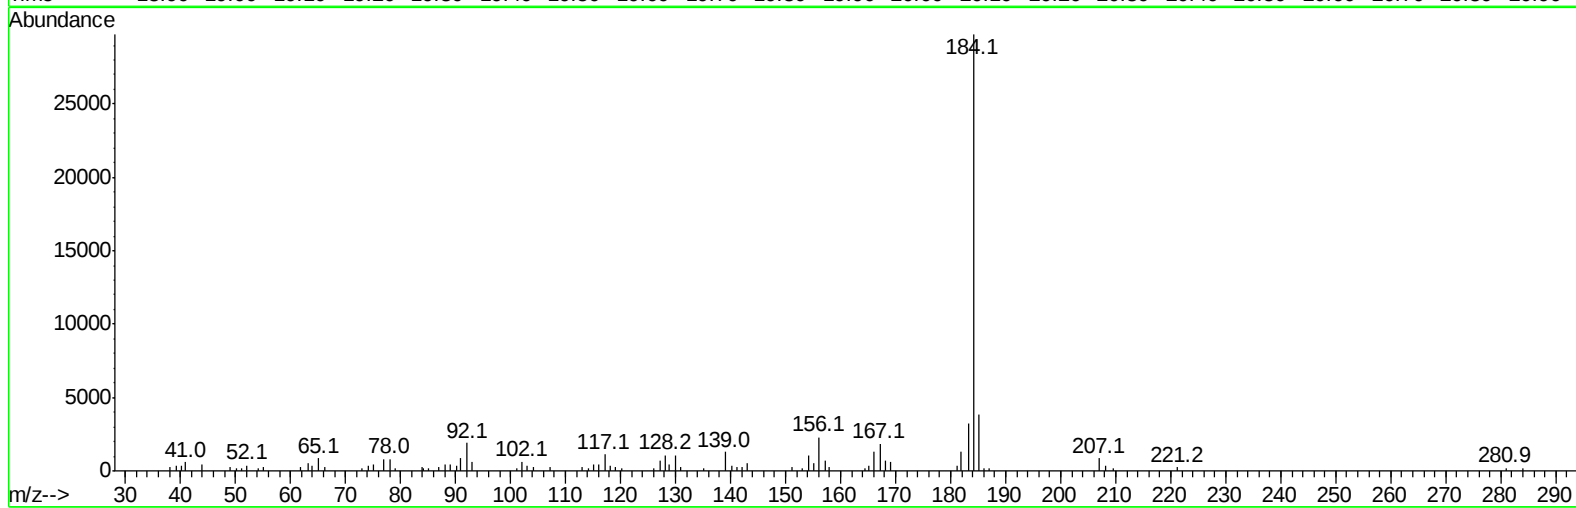


Data Path : Z:\HPCHEM1\BNA G\DATA\BG092717\
Data File : BG028943.D
Acq On : 27 Sep 2017 15:06
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 28 03:51:05 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG091217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 16:57:11 2017
Response via : Initial Calibration

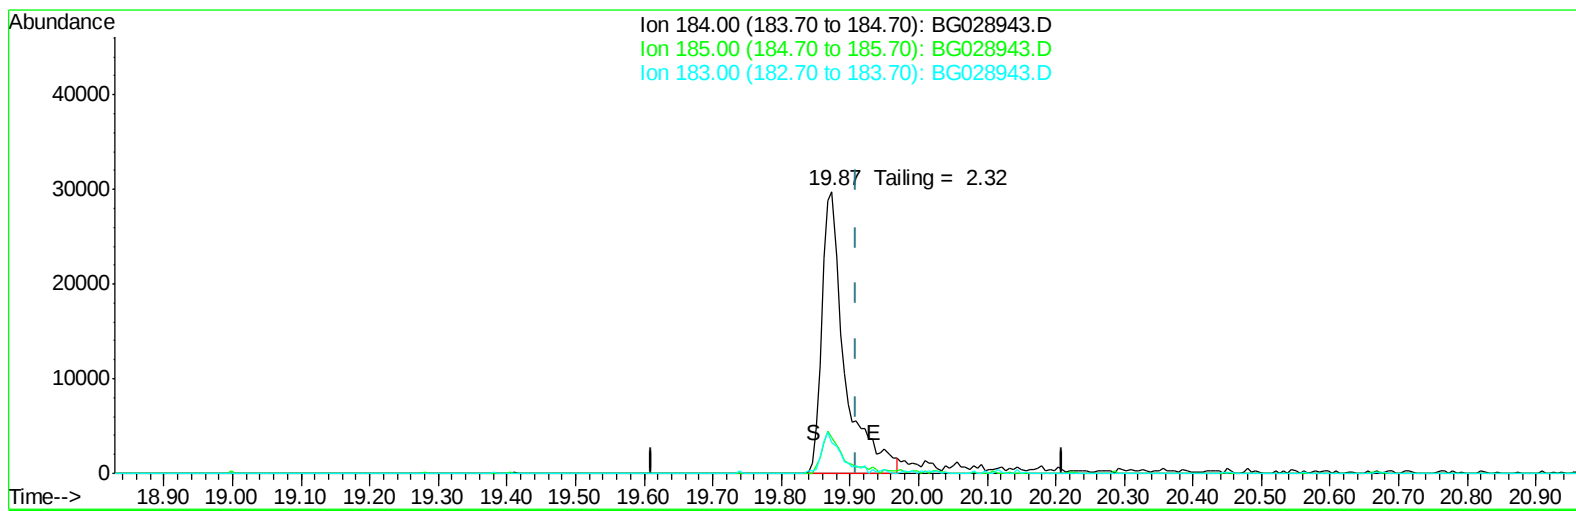

TIC: BG028943.D

(76) Benzidine



19.874min (-0.036) 36142.41ng

response 65608

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	12.81#
183.00	13.80	10.80#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG092717\
Data File : BG028943.D
Acq On : 27 Sep 2017 15:06
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 28 03:51:05 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG091217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 16:57:11 2017
Response via : Initial Calibration

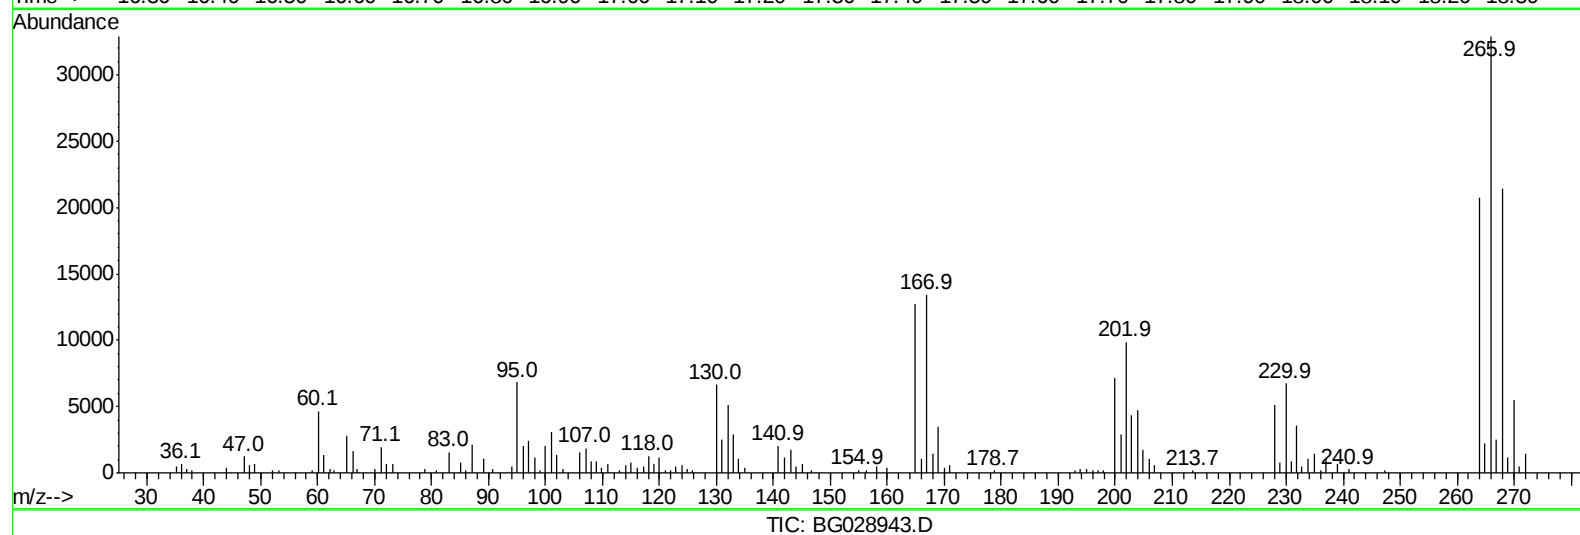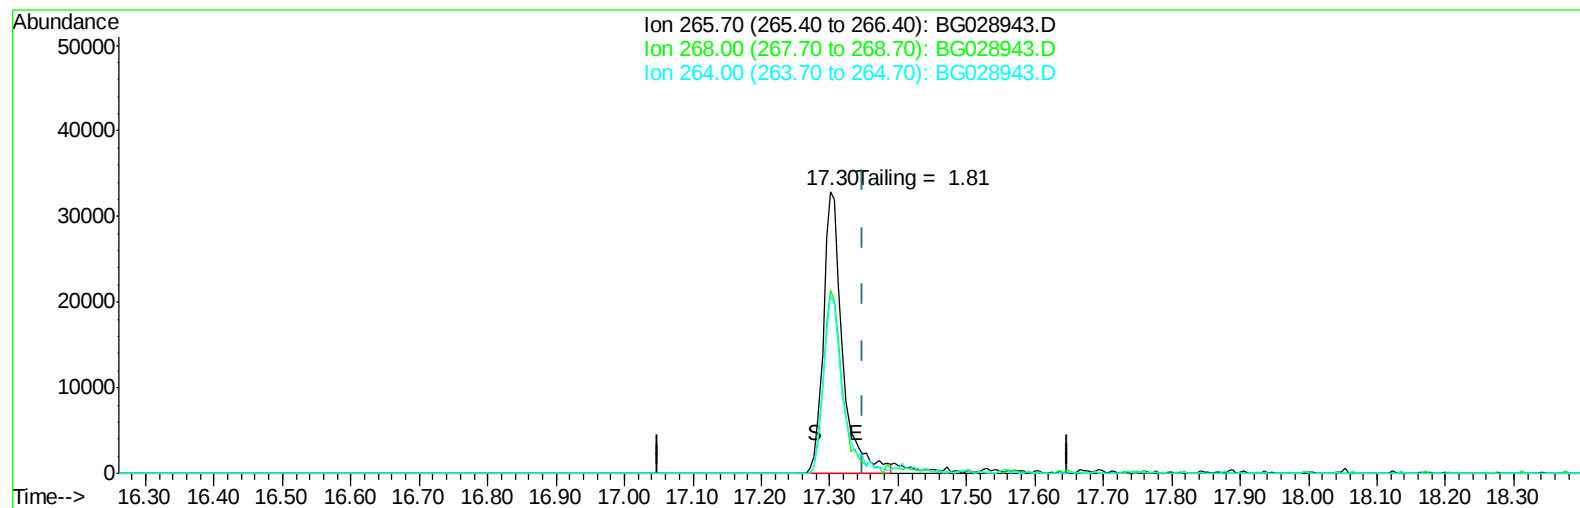

(69) Pentachlorophenol (C)

17.301min (-0.048) 122435.95ng

response 63191

Ion	Exp%	Act%
265.70	100	100
268.00	60.70	65.00
264.00	62.60	63.05
0.00	0.00	0.00