


Data Path : Z:\HPCHEM1\BNA G\Data\BG092717\
 Data File : BG028943.D
 Acq On : 27 Sep 2017 15:06
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG091217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 12 16:57:11 2017

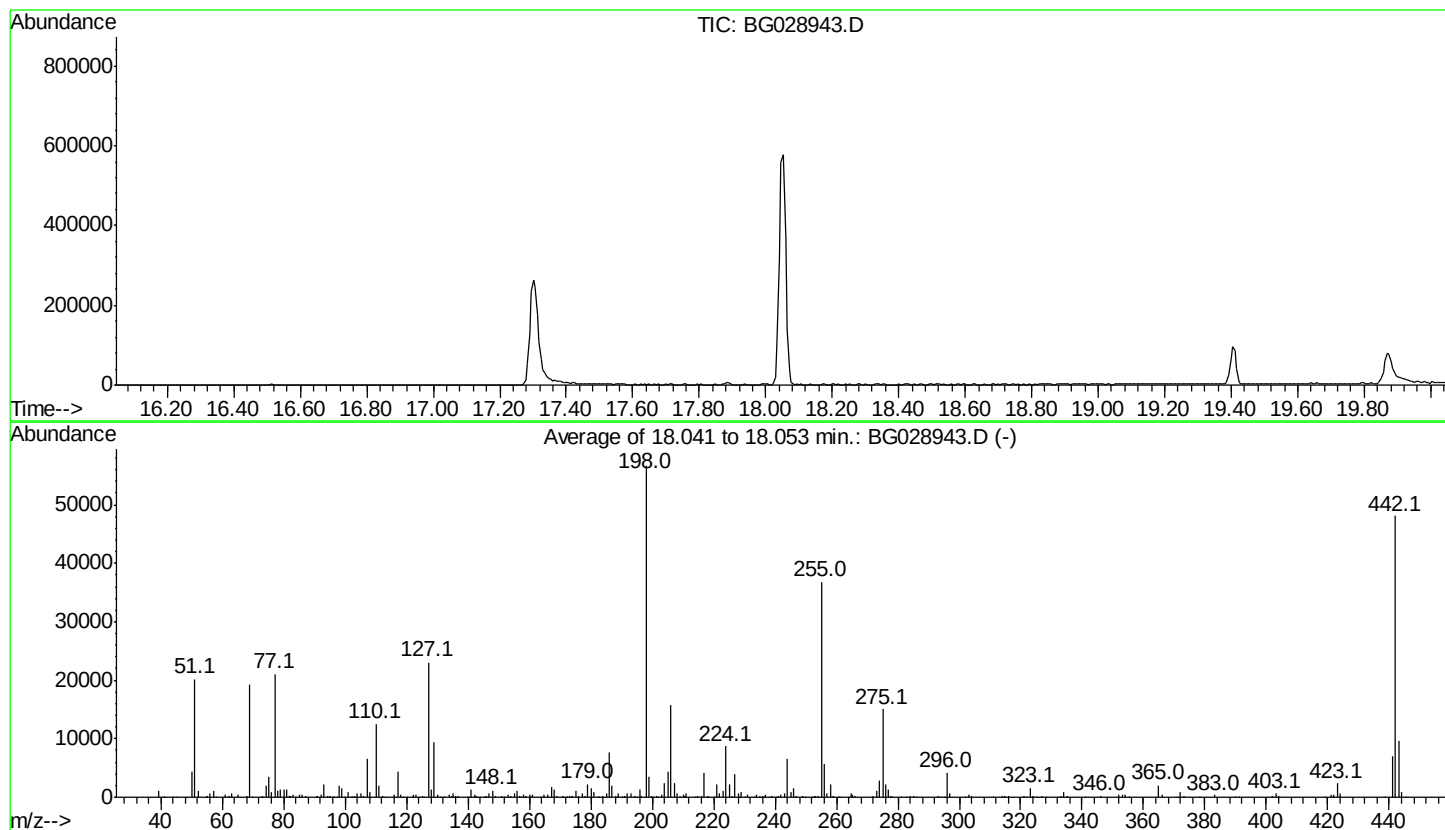

AutoFind: Scans 2460, 2461, 2462; Background Corrected with Scan 2454

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.5	20149	PASS
68	69	0.00	2	1.6	306	PASS
69	198	0.00	100	33.8	19179	PASS
70	69	0.00	2	0.4	84	PASS
127	198	10	80	40.6	23024	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	56682	PASS
199	198	5	9	6.4	3617	PASS
275	198	10	60	26.5	15033	PASS
365	198	1	100	3.6	2039	PASS
441	442	0.01	24	14.6	7029	PASS
442	198	50	100	84.9	48104	PASS
443	442	15	24	20.2	9732	PASS