
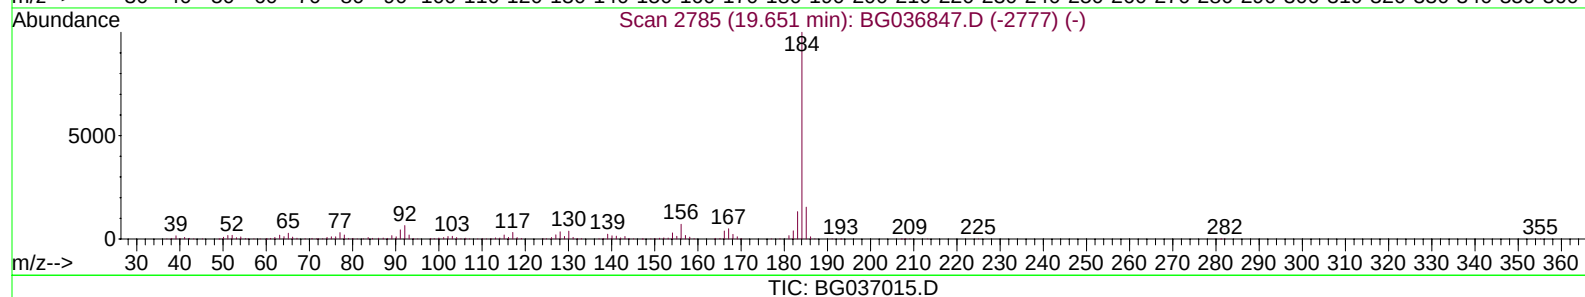
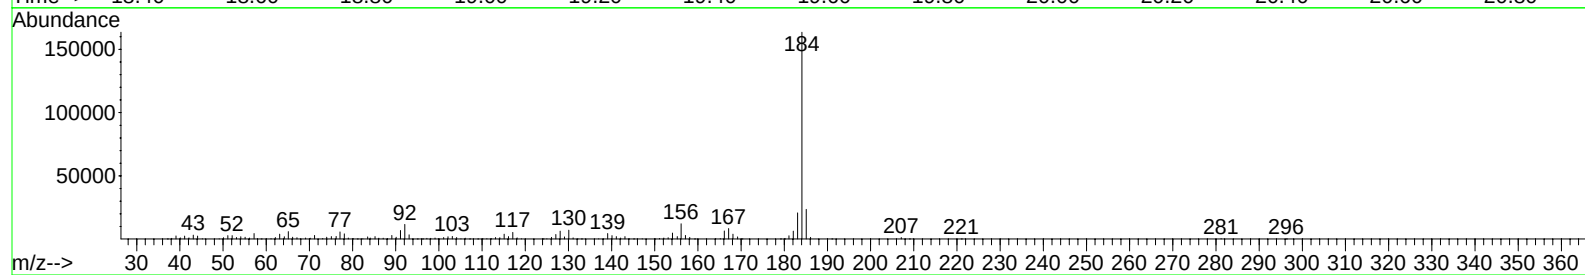


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG092718\  
Data File : BG037015.D  
Acq On : 27 Sep 2018 15:21  
Operator : JU/SJ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 27 19:21:11 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG092018.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Sep 24 10:41:23 2018  
Response via : Initial Calibration

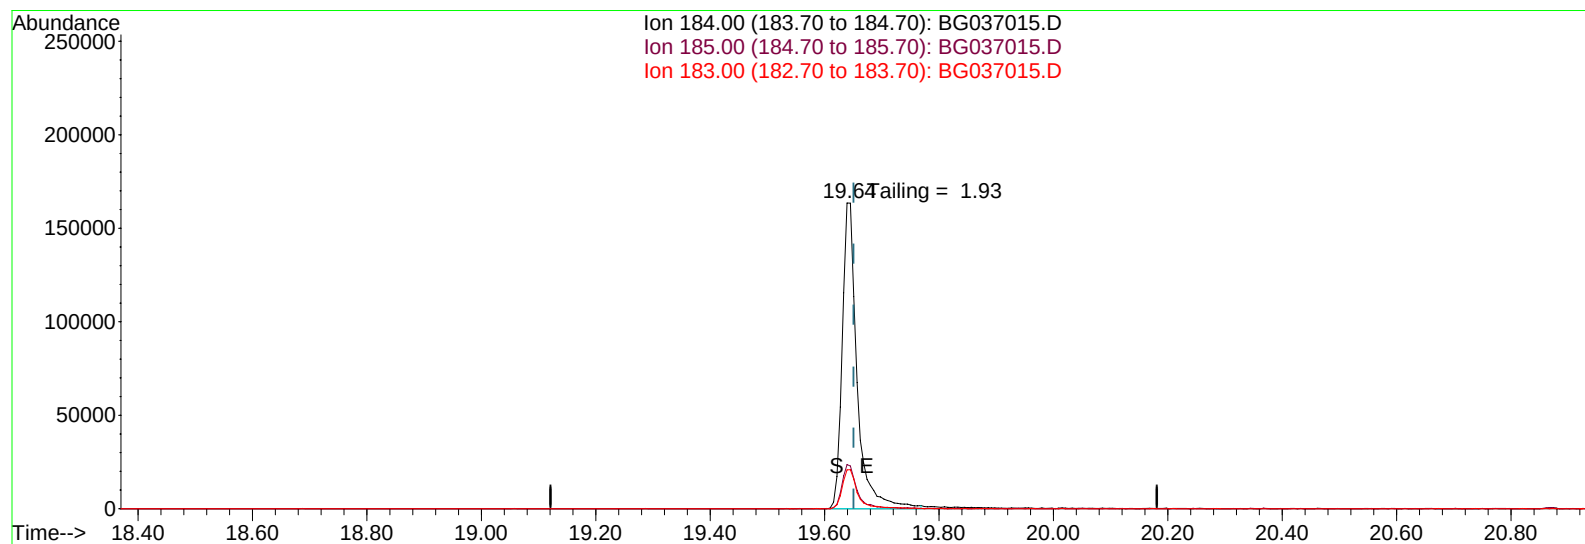

(76) Benzidine




19.639min (-0.012) 6493.74ng

response 298578

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 15.70 | 14.44 |
| 183.00 | 13.60 | 12.72 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG092718\  
Data File : BG037015.D  
Acq On : 27 Sep 2018 15:21  
Operator : JU/SJ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 27 19:21:11 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG092018.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Sep 24 10:41:23 2018  
Response via : Initial Calibration

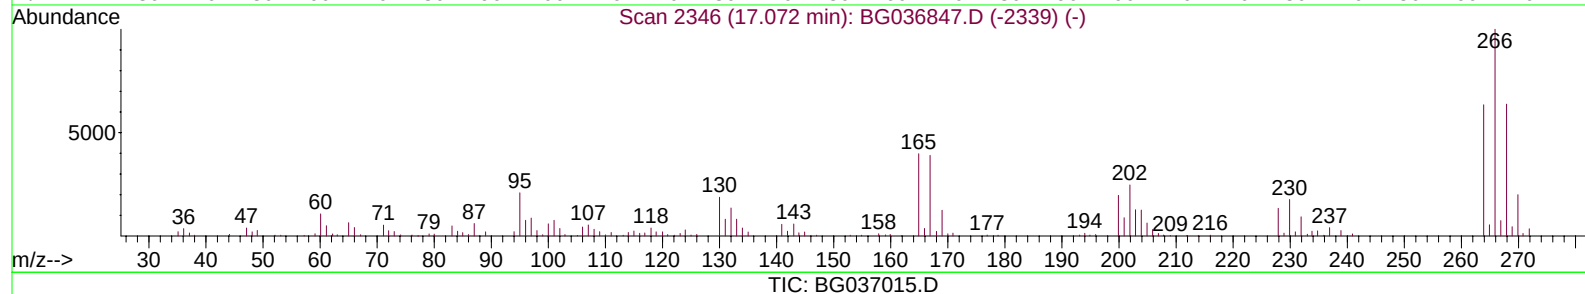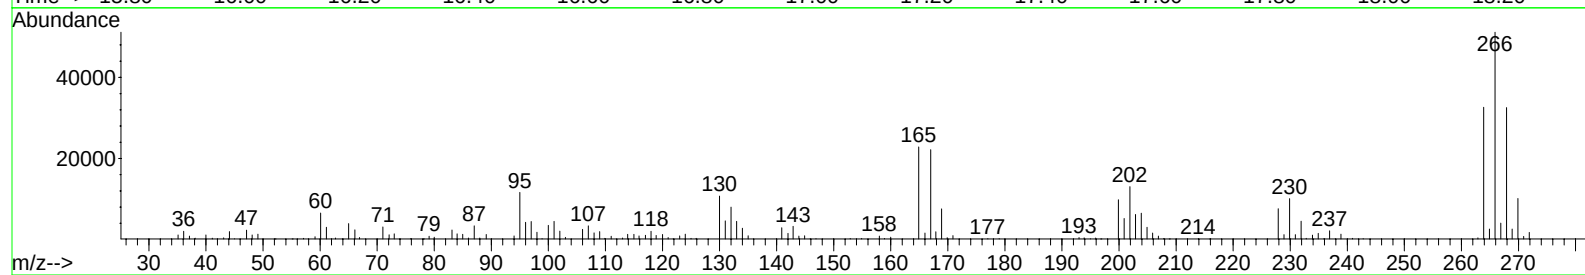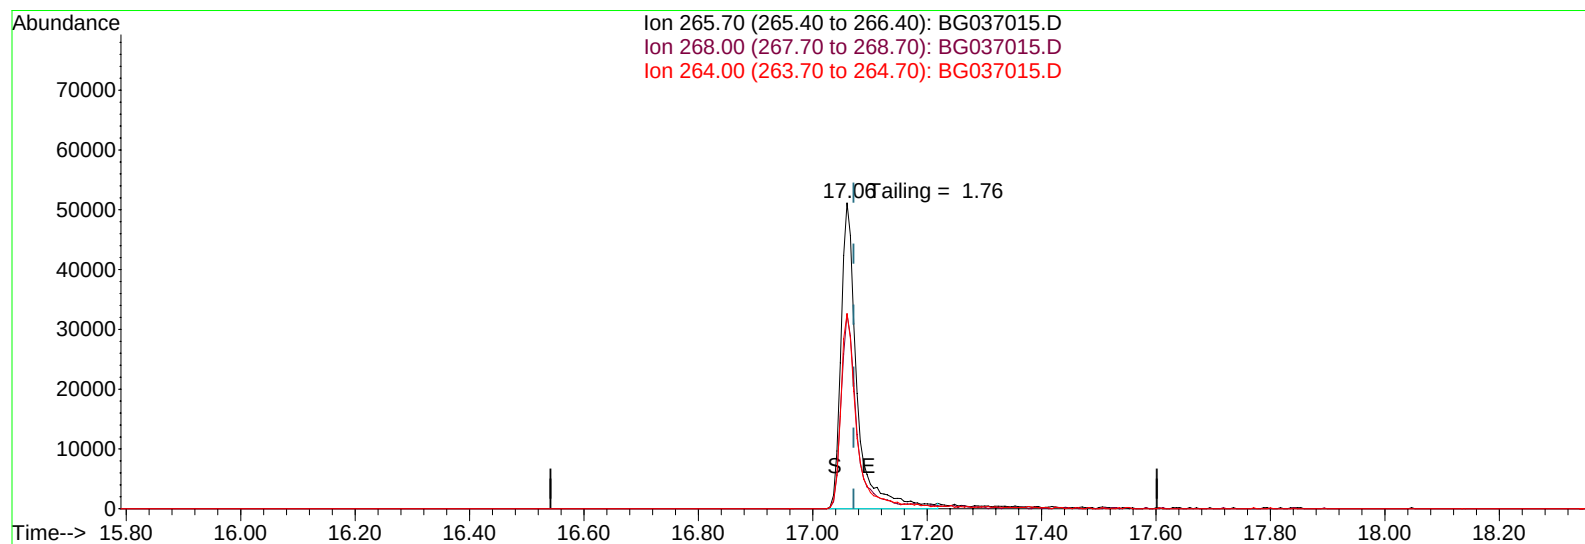

(69) Pentachlorophenol (C)

17.060min (-0.012) 12746.27ng

response 100782

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 64.30 | 63.67 |
| 264.00 | 61.10 | 63.81 |
| 0.00   | 0.00  | 0.00  |