

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG092718\
 Data File : BG037026.D
 Acq On : 27 Sep 2018 22:29
 Operator : JU/SJ
 Sample : J5096-02
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 MT-T-5-2

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092018.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.153	312	317	324	rVB	57806	91821	3.06%	0.661%
2	5.617	389	396	412	rBV	528436	969139	32.34%	6.979%
3	7.203	659	666	685	rBV	470536	940149	31.37%	6.770%
4	7.573	722	729	739	rBV	569322	1060946	35.40%	7.640%
5	8.043	802	809	822	rBV	124555	253346	8.45%	1.824%
6	8.361	856	863	880	rBV	461561	869720	29.02%	6.263%
7	9.201	998	1006	1027	rBV	355326	755107	25.20%	5.438%
8	10.846	1278	1286	1298	rBV	161650	329427	10.99%	2.372%
9	13.290	1695	1702	1719	rBV	949896	1615722	53.92%	11.635%
10	14.665	1928	1936	1951	rBV2	254444	448935	14.98%	3.233%
11	16.152	2182	2189	2212	rBV	747109	1335403	44.56%	9.616%
12	17.409	2397	2403	2425	rBV	356925	619573	20.68%	4.462%
13	20.018	2841	2847	2860	rBV	2155368	2996635	100.00%	21.579%
14	21.674	3123	3129	3144	rBV	431449	777658	25.95%	5.600%
15	23.155	3376	3381	3388	rBV3	20870	40378	1.35%	0.291%
16	23.954	3512	3517	3525	rVB4	19960	42565	1.42%	0.307%
17	24.883	3665	3675	3690	rBV2	247887	740294	24.70%	5.331%


Sum of corrected areas: 13886818

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG092718\
Data File : BG037026.D
Acq On : 27 Sep 2018 22:29
Operator : JU/SJ
Sample : J5096-02
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MT-T-5-2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG092018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

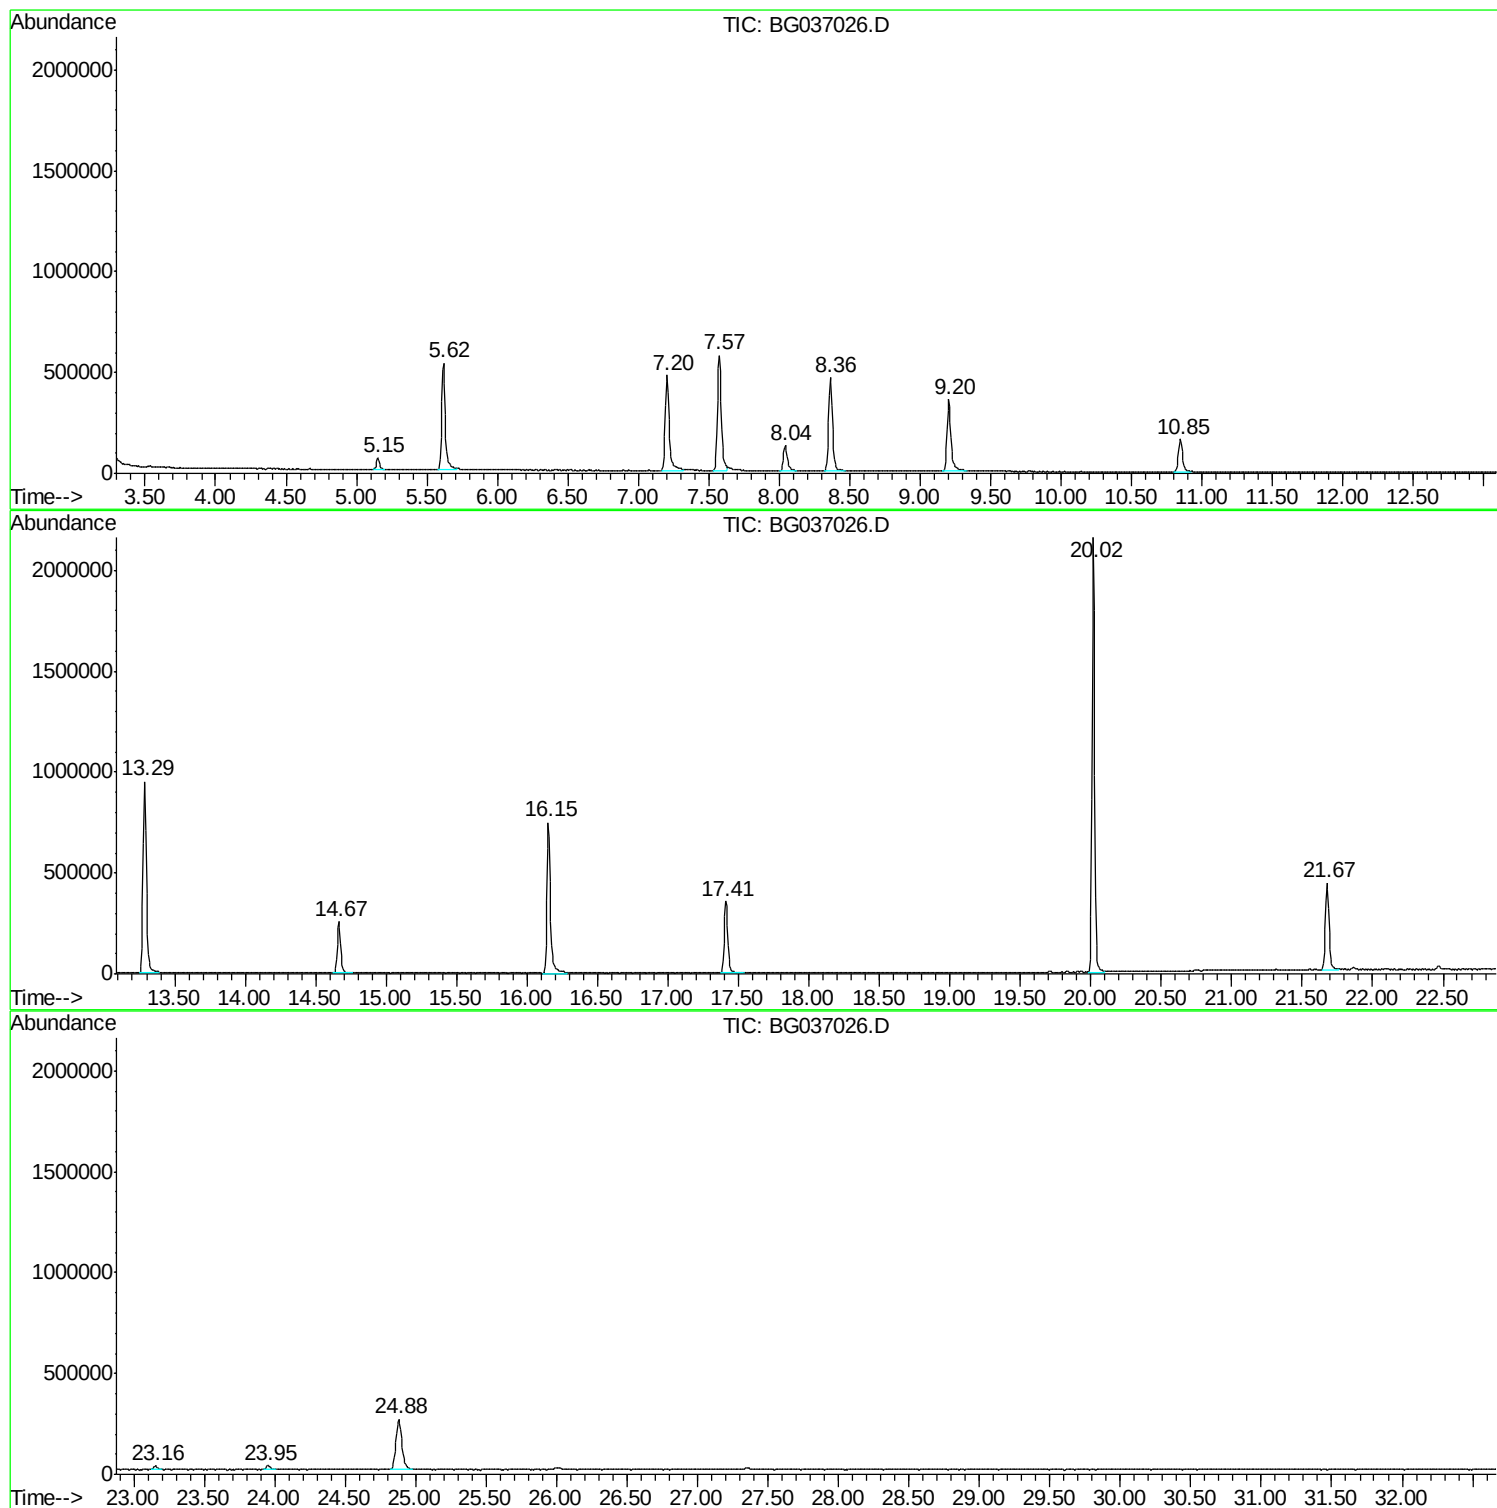

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG092718\
Data_File : BG037026.D
Acq_On : 27-Sep-2018 22:29
Operator : JU/SJJ
Sample : J5096-022
Misc :
ALS_Vial : 12 Sample_Multiplier: 11

Instrument :
BNA_G
ClientSampleId :
MT-T-5-2

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092018.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATION

TIC_Library : C:\Database\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
