

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG092718\
 Data File : BG037050.D
 Acq On : 28 Sep 2018 14:43
 Operator : JU/SJ
 Sample : J5131-04
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 FOUNDATION-CONTAINMENT-C

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092018.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.550	210	215	228	rBV	102372	179193	8.95%	1.865%
2	5.144	311	316	327	rBV	130856	219333	10.95%	2.283%
3	5.614	391	396	410	rBV	132078	261881	13.08%	2.725%
4	7.200	660	666	683	rBV	269487	586353	29.28%	6.102%
5	7.570	723	729	744	rBV	189992	389365	19.44%	4.052%
6	8.040	803	809	823	rBV	115251	232787	11.63%	2.423%
7	8.363	856	864	884	rBV	300609	610587	30.49%	6.354%
8	9.204	999	1007	1022	rBV	213627	490361	24.49%	5.103%
9	10.843	1280	1286	1302	rBV	156237	321120	16.04%	3.342%
10	13.287	1695	1702	1721	rBV	652970	1139364	56.90%	11.857%
11	14.115	1838	1843	1849	rBV2	23359	38625	1.93%	0.402%
12	14.662	1930	1936	1949	rBV2	248017	457824	22.86%	4.765%
13	16.154	2184	2190	2205	rBV	66576	144291	7.21%	1.502%
14	17.412	2396	2404	2415	rBV2	357839	630734	31.50%	6.564%
15	20.014	2841	2847	2859	rBV	1413168	2002428	100.00%	20.839%
16	21.313	3063	3068	3076	rBV2	39229	70616	3.53%	0.735%
17	21.677	3123	3130	3147	rBV2	431219	769194	38.41%	8.005%
18	21.859	3157	3161	3168	rBV3	18937	28156	1.41%	0.293%
19	22.465	3259	3264	3269	rBV3	19788	37122	1.85%	0.386%
20	23.152	3376	3381	3388	rBV6	18917	37844	1.89%	0.394%
21	23.340	3407	3413	3422	rVB	75473	145051	7.24%	1.510%
22	23.951	3510	3517	3525	rBV5	19496	45780	2.29%	0.476%
23	24.879	3665	3675	3688	rBV2	246350	741873	37.05%	7.721%
24	26.007	3860	3867	3875	rBV6	10421	29131	1.45%	0.303%


Sum of corrected areas: 9609013

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG092718\
Data File : BG037050.D
Acq On : 28 Sep 2018 14:43
Operator : JU/SJ
Sample : J5131-04
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
FOUNDATION-CONTAINMENT-C

Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG092018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

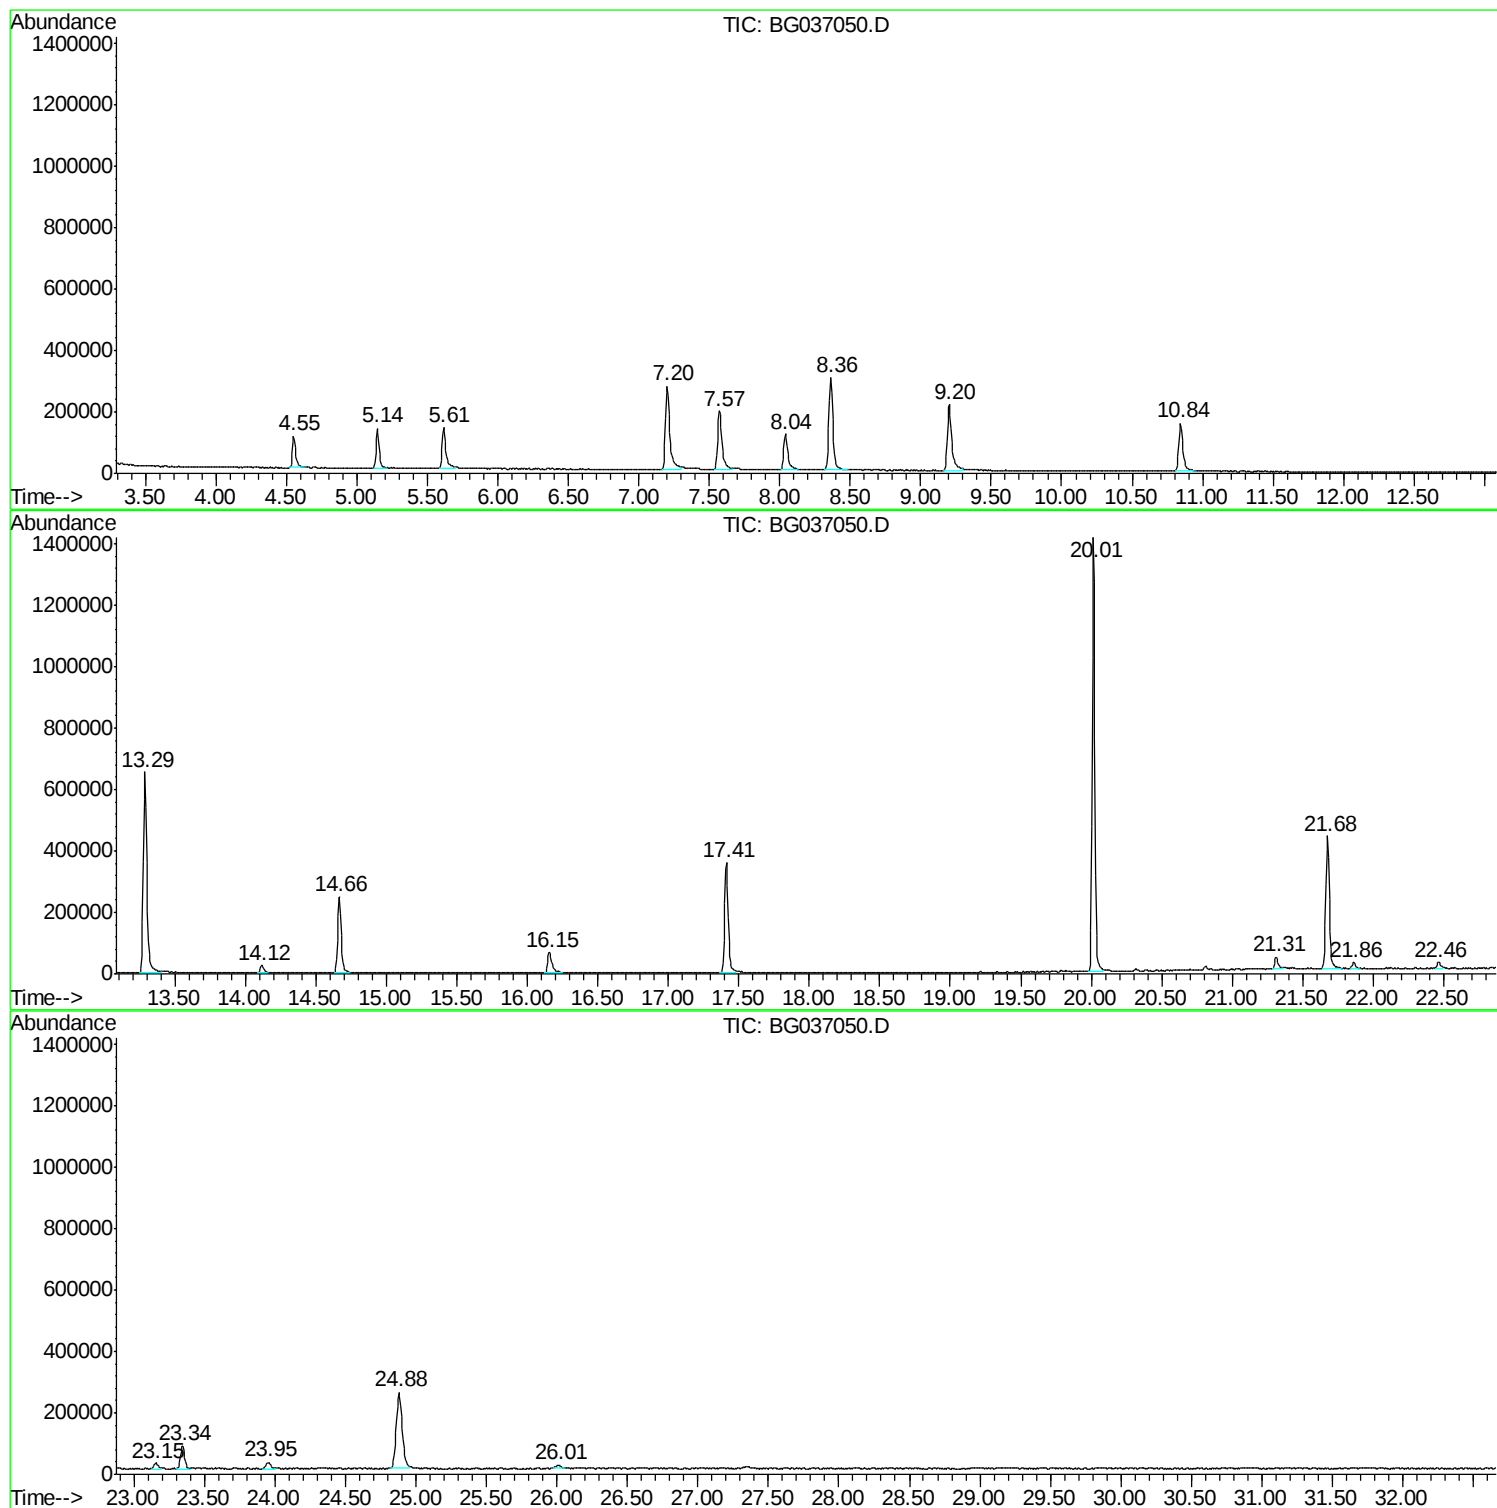

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG092718\
Data_File : BG037050.D
Acq_On : 28-Sep-2018 14:433
Operator : JU/SJJ
Sample : J5131-044
Misc :
ALS_Vial : 34 Sample_Multiplier: 11

Instrument :
BNA_G
ClientSampleId :
FOUNDATION-CONTAINMENT-C

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092018.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\Database\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
				#	RT Resp Conc

No Library Search Compounds Detected
