


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092718\
 Data File : BG037015.D
 Acq On : 27 Sep 2018 15:21
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092018.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Sep 24 10:41:23 2018

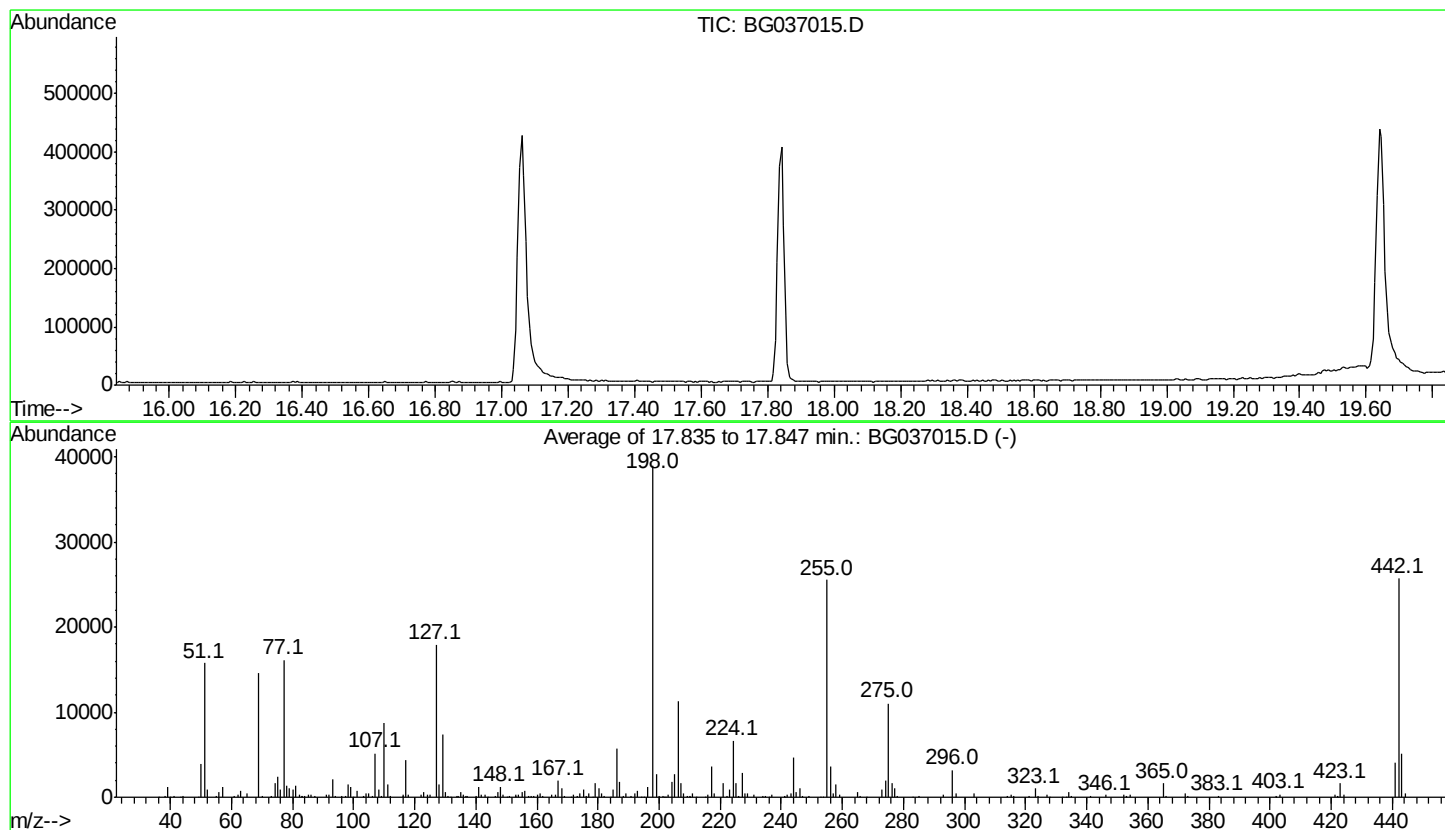

AutoFind: Scans 2476, 2477, 2478; Background Corrected with Scan 2469

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.5	15764	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	37.6	14659	PASS
70	69	0.00	2	1.4	202	PASS
127	198	10	80	46.0	17905	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	38960	PASS
199	198	5	9	6.8	2659	PASS
275	198	10	60	28.3	11027	PASS
365	198	1	100	4.2	1619	PASS
441	198	0.01	100	10.6	4125	PASS
442	198	50	100	65.9	25688	PASS
443	442	15	24	20.2	5177	PASS