


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG092718\  
 Data File : BG037034.D  
 Acq On : 28 Sep 2018 4:20  
 Operator : JU/SJ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG092018.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Mon Sep 24 10:41:23 2018

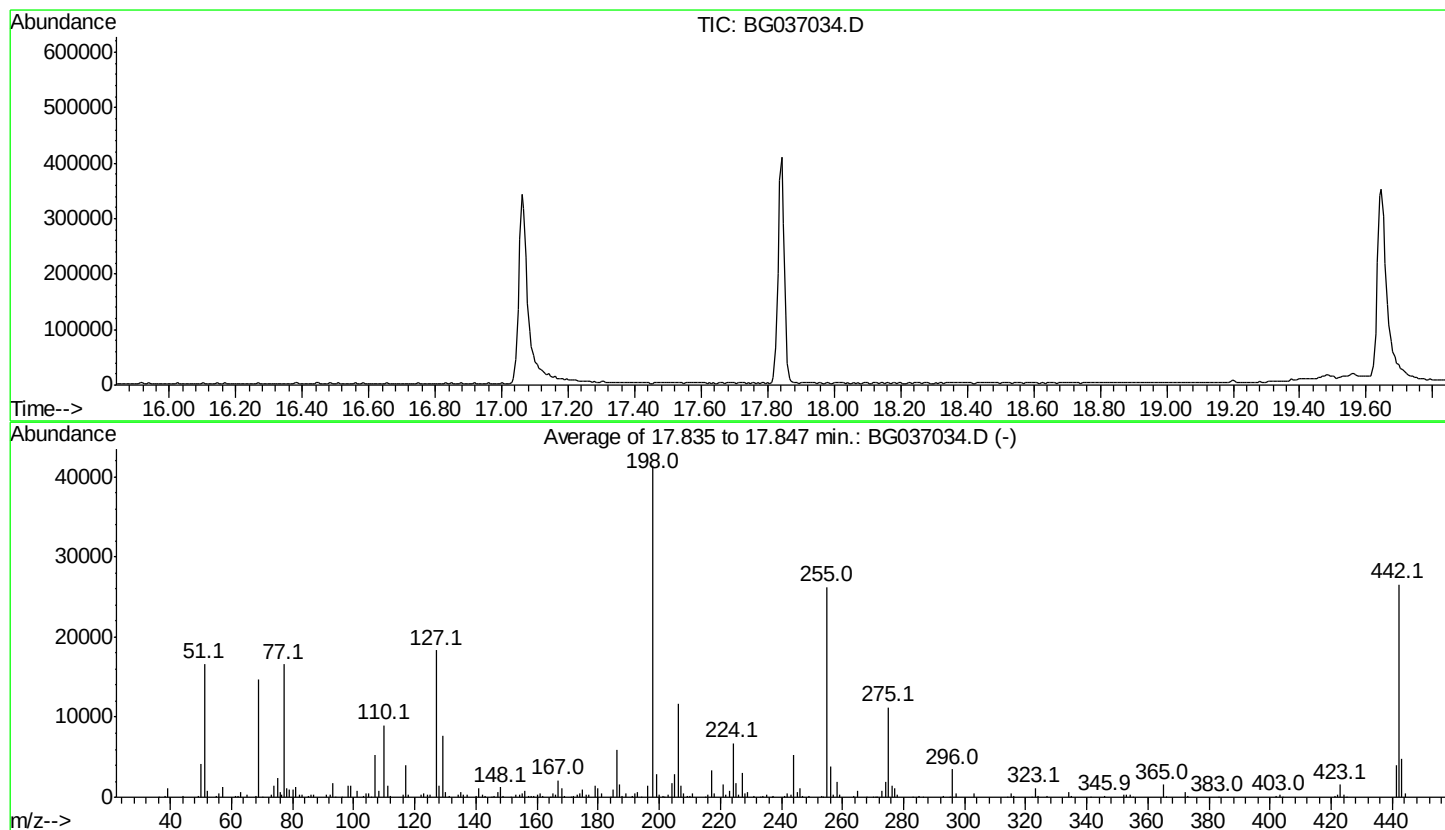

AutoFind: Scans 2476, 2477, 2478; Background Corrected with Scan 2469

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 40.3      | 16681   | PASS             |
| 68          | 69           | 0.00         | 2            | 1.4       | 204     | PASS             |
| 69          | 198          | 0.00         | 100          | 35.7      | 14766   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.4       | 54      | PASS             |
| 127         | 198          | 10           | 80           | 44.3      | 18362   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 41413   | PASS             |
| 199         | 198          | 5            | 9            | 7.0       | 2891    | PASS             |
| 275         | 198          | 10           | 60           | 27.0      | 11202   | PASS             |
| 365         | 198          | 1            | 100          | 3.7       | 1545    | PASS             |
| 441         | 198          | 0.01         | 100          | 9.8       | 4061    | PASS             |
| 442         | 198          | 50           | 100          | 64.1      | 26562   | PASS             |
| 443         | 442          | 15           | 24           | 18.4      | 4878    | PASS             |