

Data Path : Z:\HPCHEM1\BNA G\DATA\BG092815\
 Data File : BG018949.D
 Acq On : 28 Sep 2015 23:28
 Operator : UM/NP
 Sample : G3803-06
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 E43J6

Quant Time: Sep 29 01:01:45 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG091015.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 29 00:58:09 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.98	152	53488	20.00	ng/ul	0.00
18) Naphthalene-d8	10.79	136	227712	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.61	164	155991	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.36	188	412100	20.00	ng/ul	0.00
78) Chrysene-d12	21.61	240	477381	20.00	ng/ul	0.00
86) Perylene-d12	24.78	264	486803	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.42	96	1227	1.10	ng/uL	0.00
5) Phenol-d5	7.16	99	26801	6.10	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.31	67	68876	27.06	ng/ul	0.00
9) 2-Chlorophenol-d4	7.52	132	79873	24.01	ng/ul	0.00
13) 4-Methylphenol-d8	8.69	113	53956	15.14	ng/ul	0.00
19) Nitrobenzene-d5	9.15	128	50609	29.34	ng/ul	0.00
22) 2-Nitrophenol-d4	9.87	143	57759	33.29	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.41	165	102630	28.10	ng/ul	0.00
29) 4-Chloroaniline-d4	10.93	131	3244	0.76	ng/ul	0.00
44) Dimethylphthalate-d6	14.01	166	385472	30.71	ng/ul	0.00
47) Acenaphthylene-d8	14.31	160	365158	24.55	ng/ul	0.00
52) 4-Nitrophenol-d4	14.82	143	12852	5.33	ng/ul	0.00
58) Fluorene-d10	15.60	176	234166	21.33	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.72	200	42773	21.93	ng/ul	0.00
71) Anthracene-d10	17.45	188	177734	9.80	ng/ul	0.00
79) Pyrene-d10	19.73	212	384338	17.50	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.56	264	325969	13.76	ng/ul	0.00


Target Compounds					Ovalue
45) Dimethylphthalate	14.06	163	62958	5.17 ng/ul#	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG092815\
Data File : BG018949.D
Acq On : 28 Sep 2015 23:28
Operator : UM/NP
Sample : G3803-06
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
E43J6

Quant Time: Sep 29 01:01:45 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG091015.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 29 00:58:09 2015
Response via : Initial Calibration

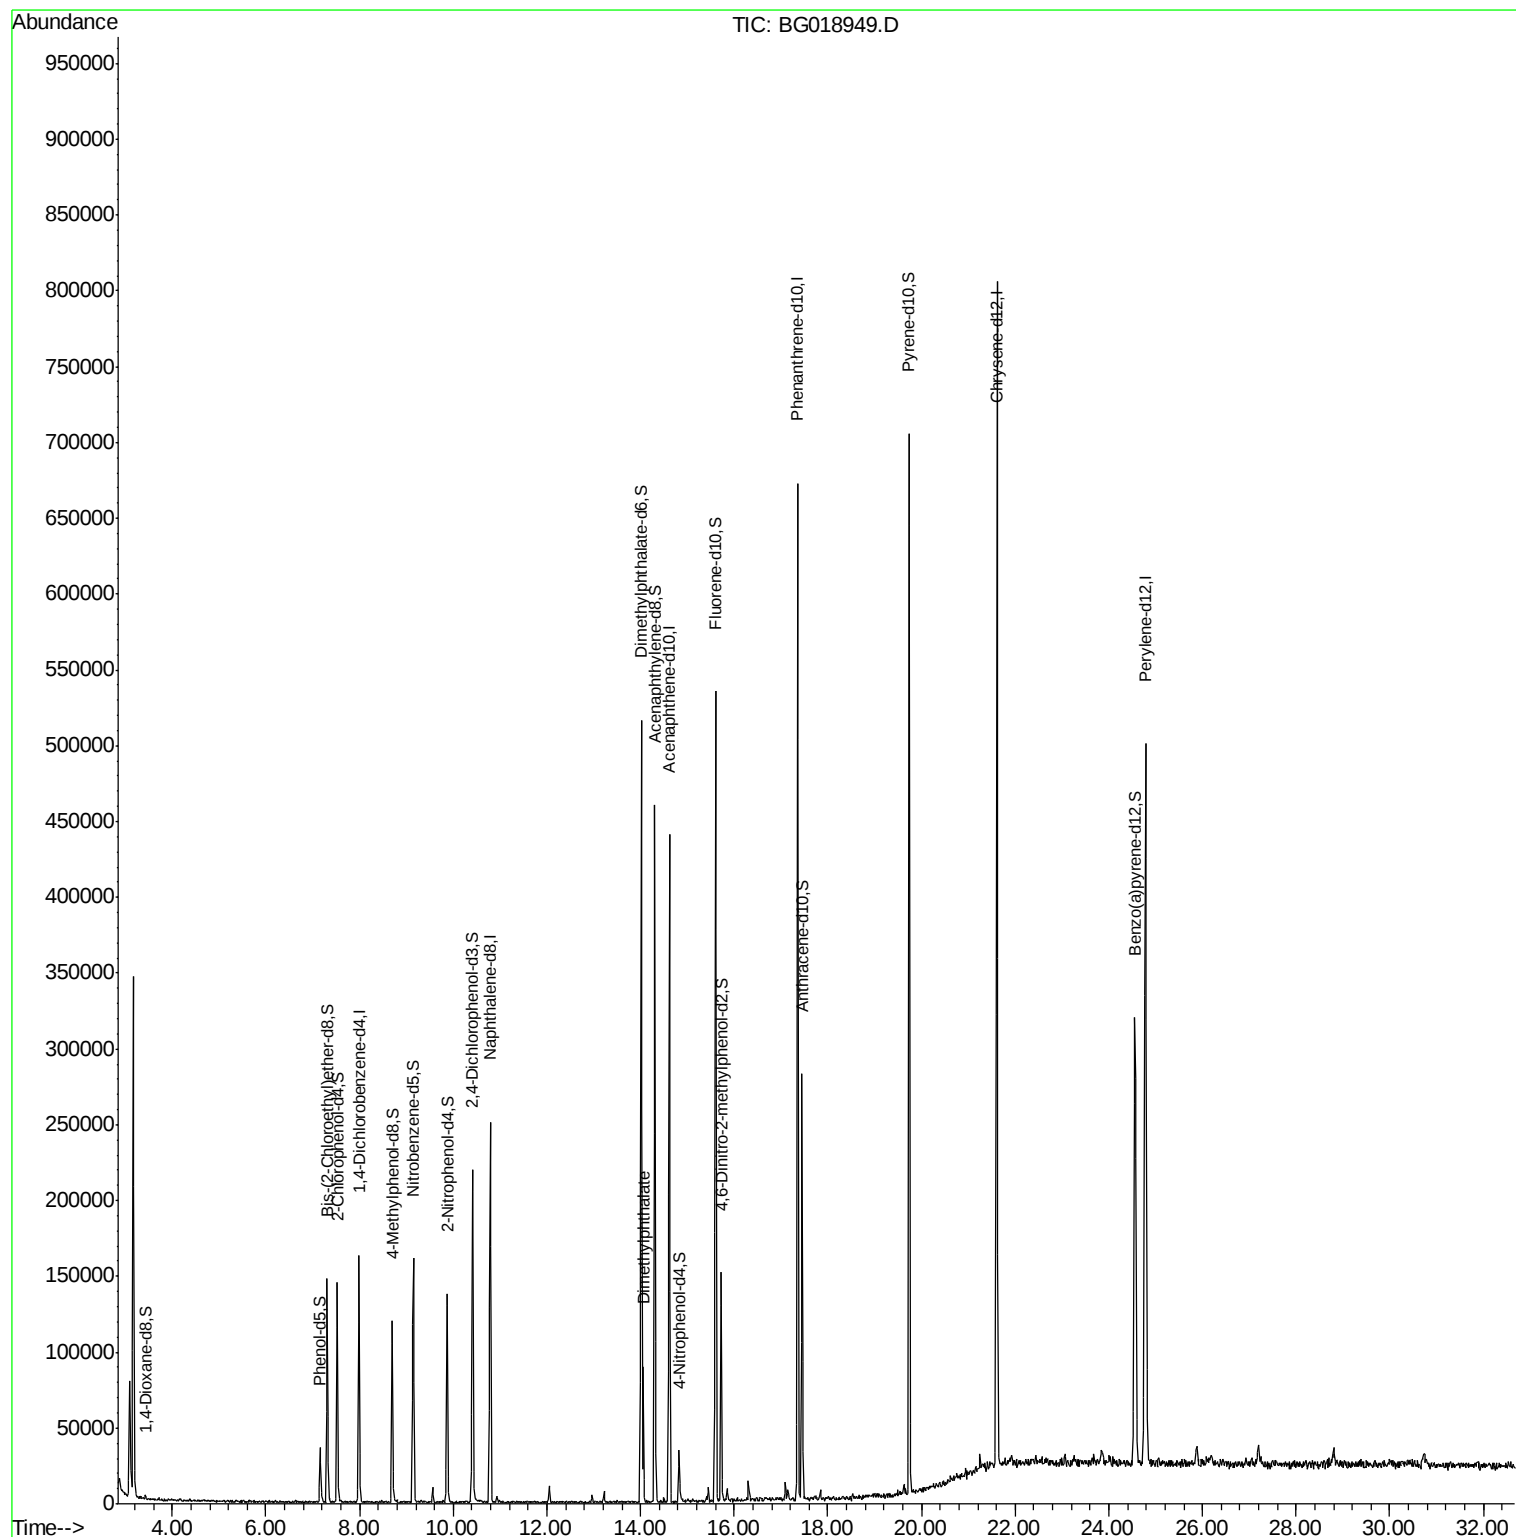

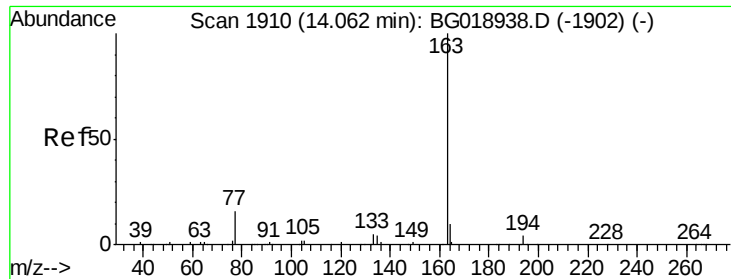

#45

Dimethylphthalate

Concen: 5.17 ng/ul

RT: 14.06 min Scan# 1910

Delta R.T. -0.00 min

Lab File: BG018949.D

Acq: 28 Sep 2015 23:28

Instrument :

BNA_G

ClientSampleId :

E43J6


Tot Ion:163 Resp: 62958

Ion Ratio Lower Upper

163 100

194 4.5 2.9 4.3#

164 10.3 7.7 11.5

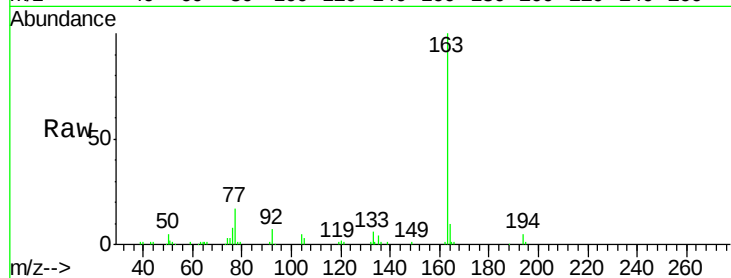

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

