


Data Path : Z:\HPCHEM1\BNA G\DATA\BG092816\
 Data File : BG024147.D
 Acq On : 28 Sep 2016 15:19
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG092316.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 23 15:35:28 2016

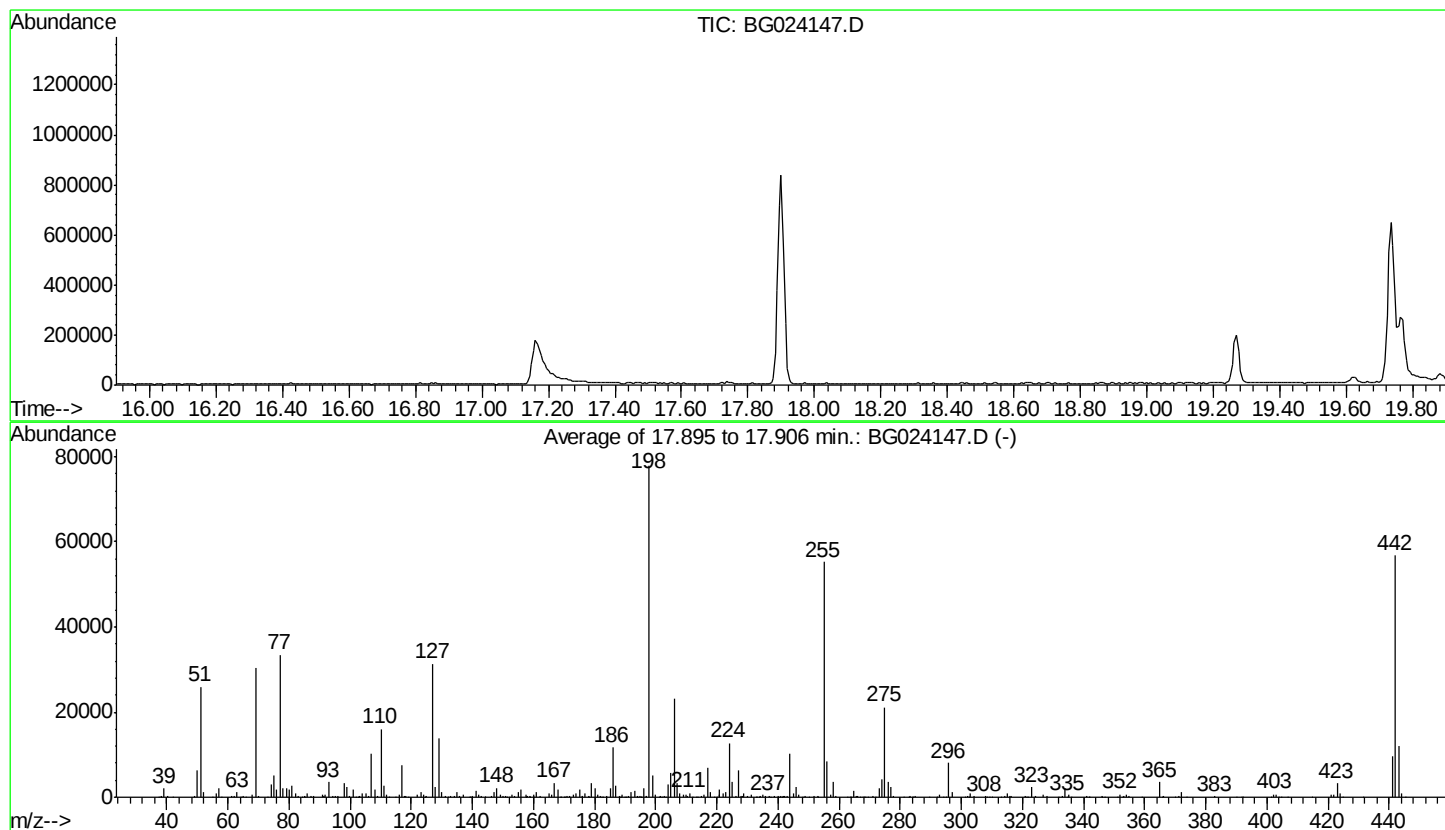

AutoFind: Scans 2563, 2564, 2565; Background Corrected with Scan 2556

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.3	25957	PASS
68	69	0.00	2	1.5	468	PASS
69	198	0.00	100	39.0	30410	PASS
70	69	0.00	2	0.8	230	PASS
127	198	10	80	40.2	31293	PASS
197	198	0.00	2	0.5	355	PASS
198	198	100	100	100.0	77893	PASS
199	198	5	9	6.7	5222	PASS
275	198	10	60	27.1	21130	PASS
365	198	1	100	4.5	3519	PASS
441	442	0.01	24	16.9	9598	PASS
442	198	50	100	72.9	56821	PASS
443	442	15	24	20.9	11892	PASS