
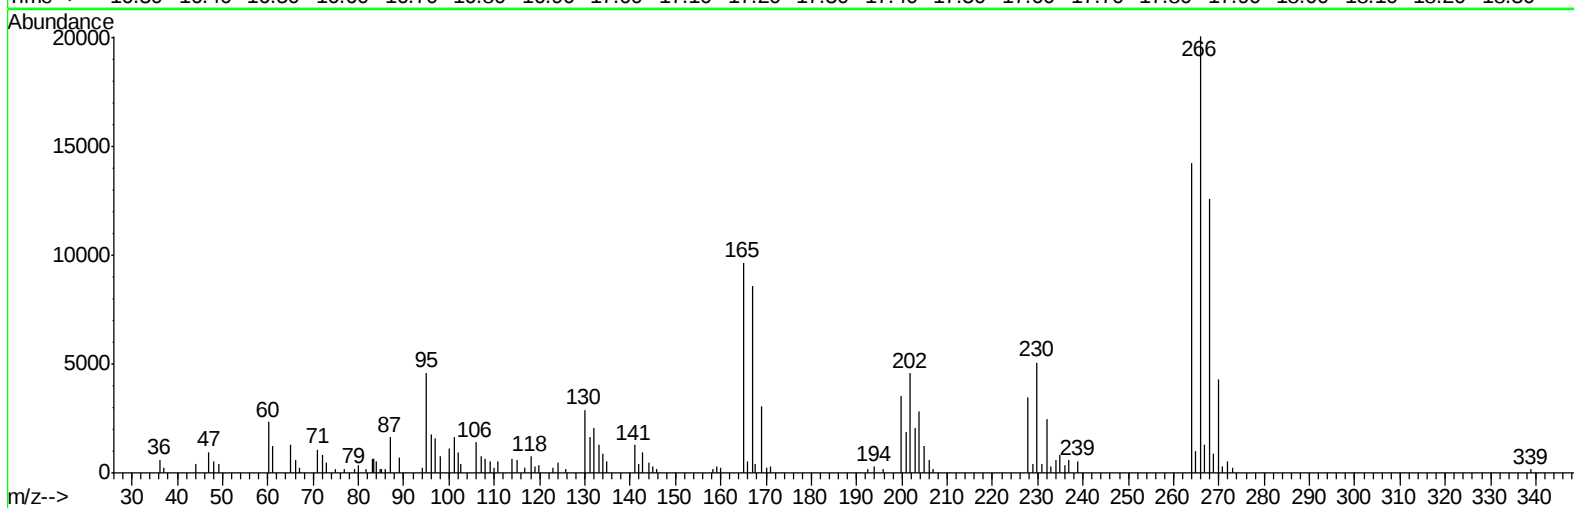


Data Path : Z:\HPCHEM1\BNA G\DATA\BG092817\
Data File : BG028959.D
Acq On : 28 Sep 2017 14:20
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Sep 29 06:44:33 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG091217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 16:57:11 2017
Response via : Initial Calibration

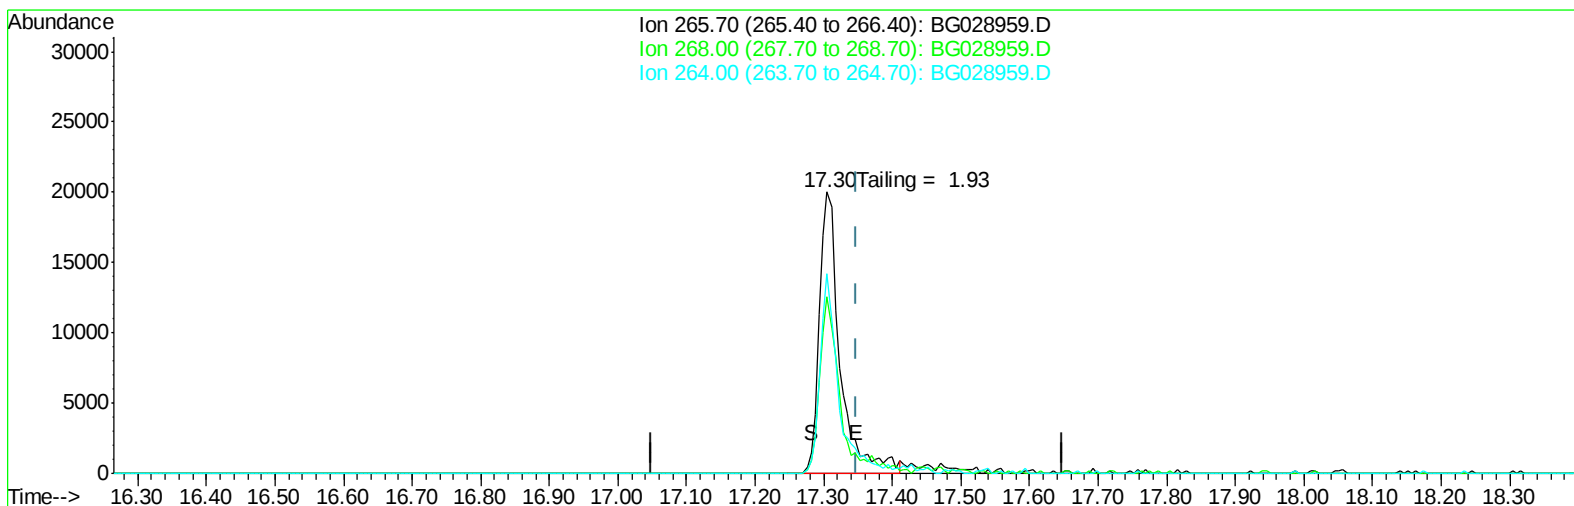

TIC: BG028959.D

(69) Pentachlorophenol (C)

17.305min (-0.044) 0.00ng



response 39754

Ion	Exp%	Act%
265.70	100	100
268.00	60.70	62.84
264.00	62.60	71.10
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG092817\
Data File : BG028959.D
Acq On : 28 Sep 2017 14:20
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Sep 29 06:44:33 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG091217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 16:57:11 2017
Response via : Initial Calibration

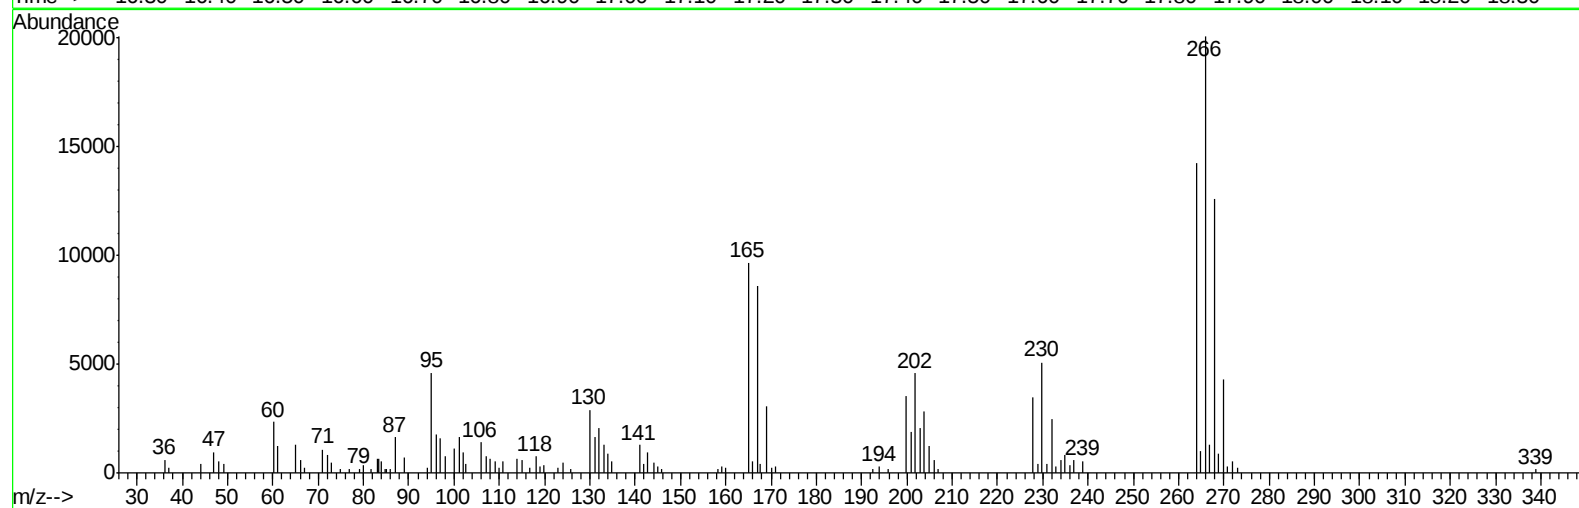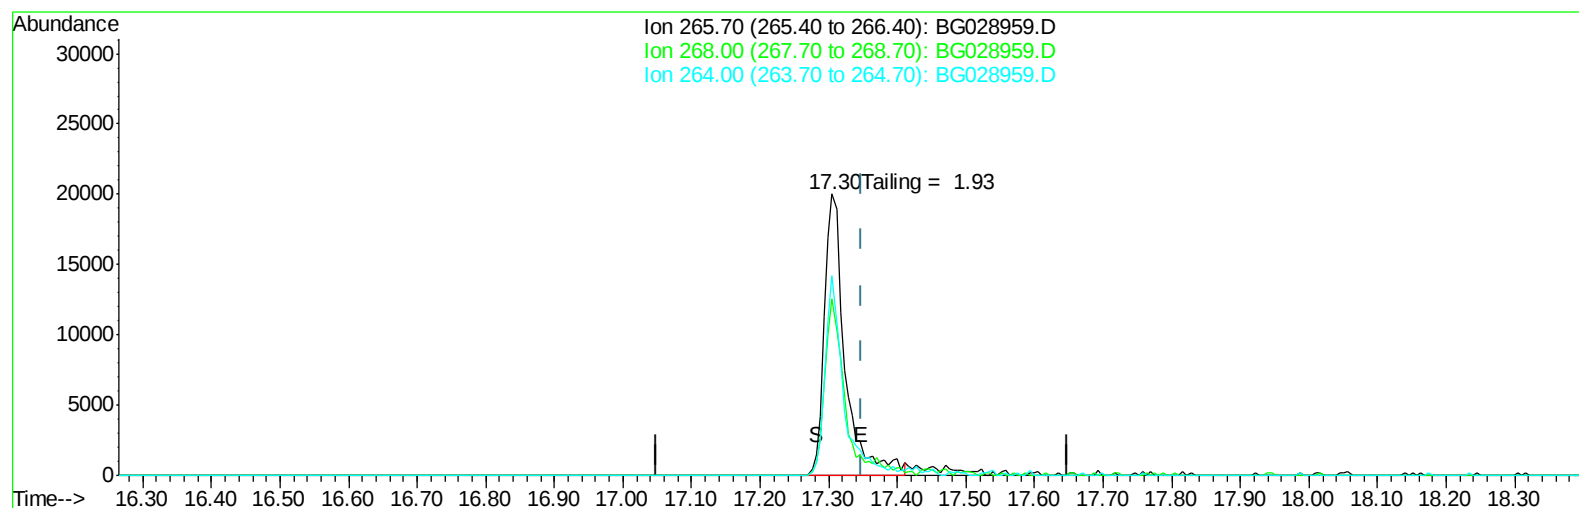

TIC: BG028959.D

(69) Pentachlorophenol (C)

17.305min (-0.044) 0.00ng

response 39754

Ion	Exp%	Act%
265.70	100	100
268.00	60.70	62.84
264.00	62.60	71.10
0.00	0.00	0.00