


Data Path : Z:\HPCHEM1\BNA G\Data\BG092817\
 Data File : BG028959.D
 Acq On : 28 Sep 2017 14:20
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG091217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 12 16:57:11 2017

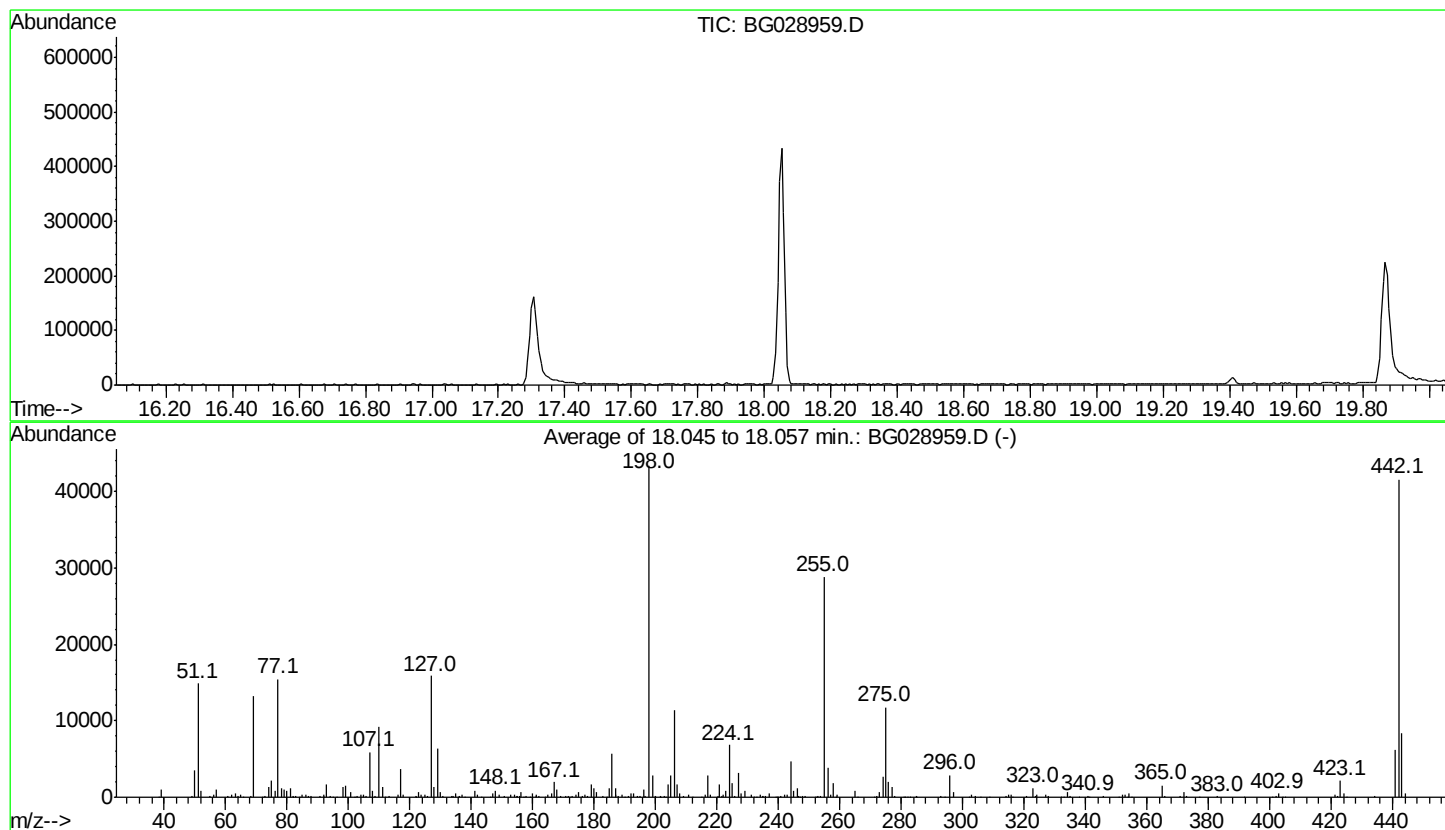

AutoFind: Scans 2460, 2461, 2462; Background Corrected with Scan 2454

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.2	14852	PASS
68	69	0.00	2	1.1	141	PASS
69	198	0.00	100	30.6	13277	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	36.6	15887	PASS
197	198	0.00	2	0.5	220	PASS
198	198	100	100	100.0	43368	PASS
199	198	5	9	6.4	2781	PASS
275	198	10	60	27.1	11750	PASS
365	198	1	100	3.5	1508	PASS
441	442	0.01	24	14.8	6146	PASS
442	198	50	100	95.9	41581	PASS
443	442	15	24	20.0	8319	PASS