
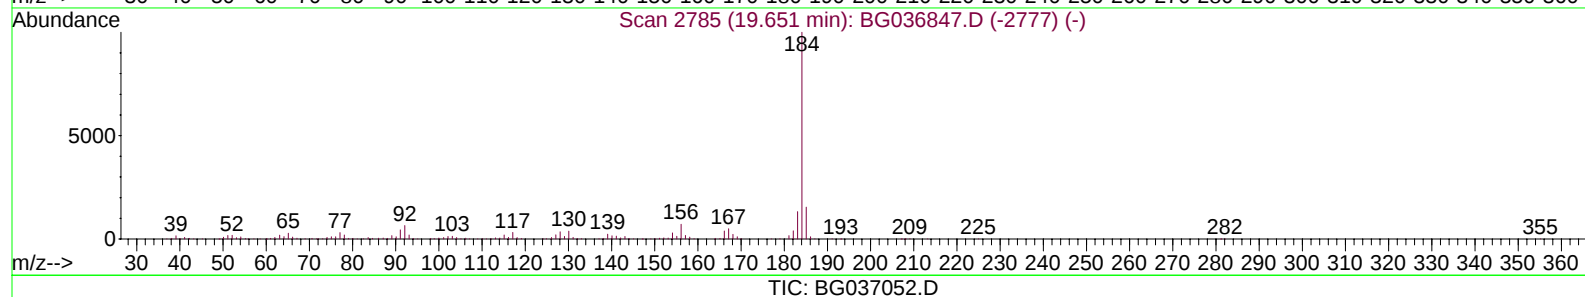
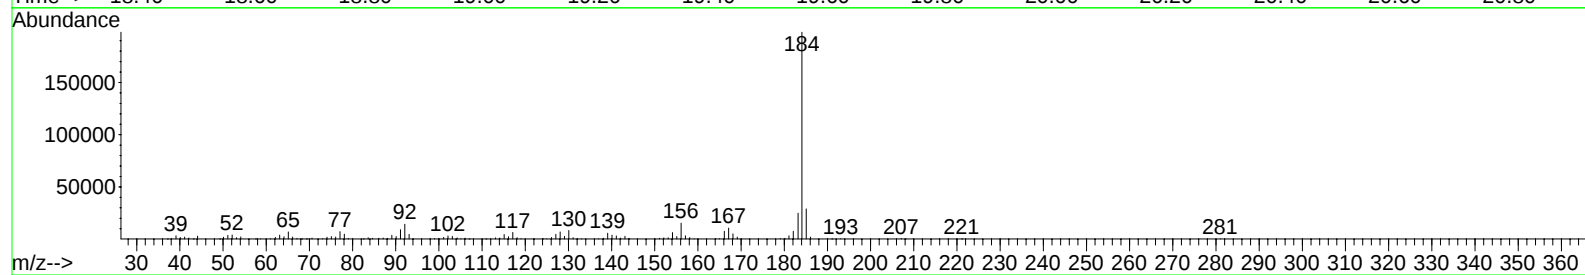


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG092818\
Data File : BG037052.D
Acq On : 28 Sep 2018 16:29
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 28 17:09:45 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG092018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 24 10:41:23 2018
Response via : Initial Calibration

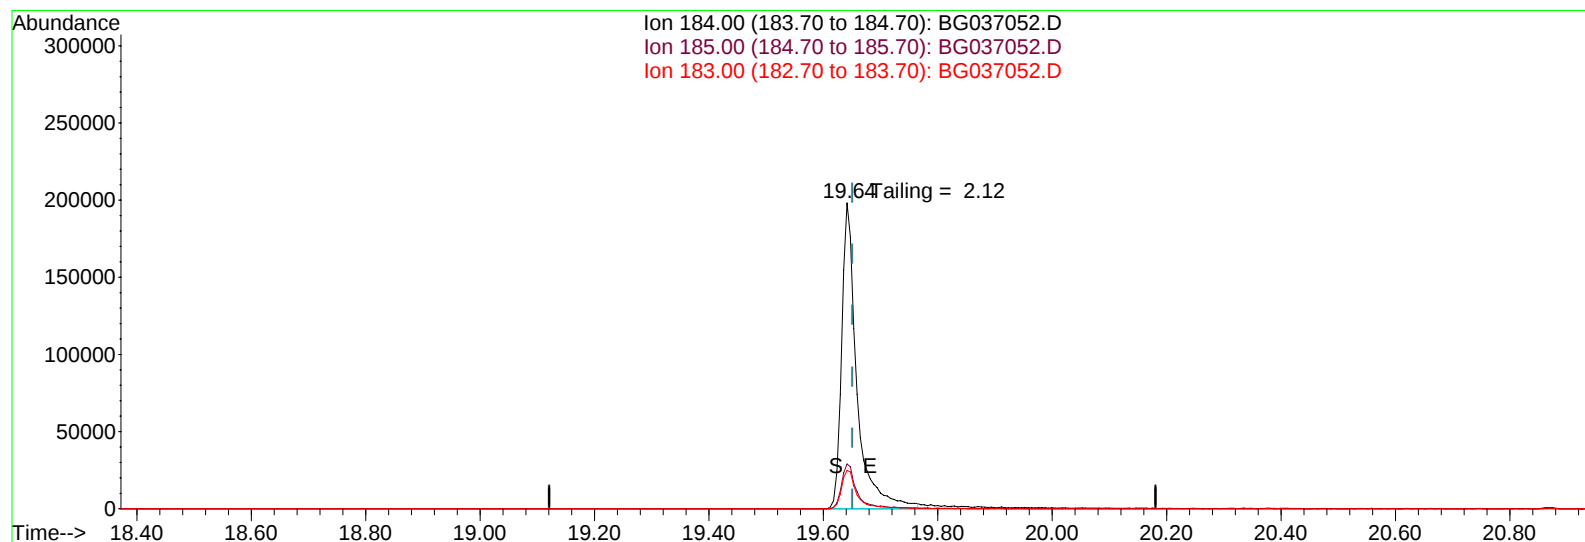

(76) Benzidine




19.641min (-0.010) 11947.97ng

response 375992

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.64
183.00	13.60	12.54
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG092818\
Data File : BG037052.D
Acq On : 28 Sep 2018 16:29
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 28 17:09:45 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG092018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 24 10:41:23 2018
Response via : Initial Calibration

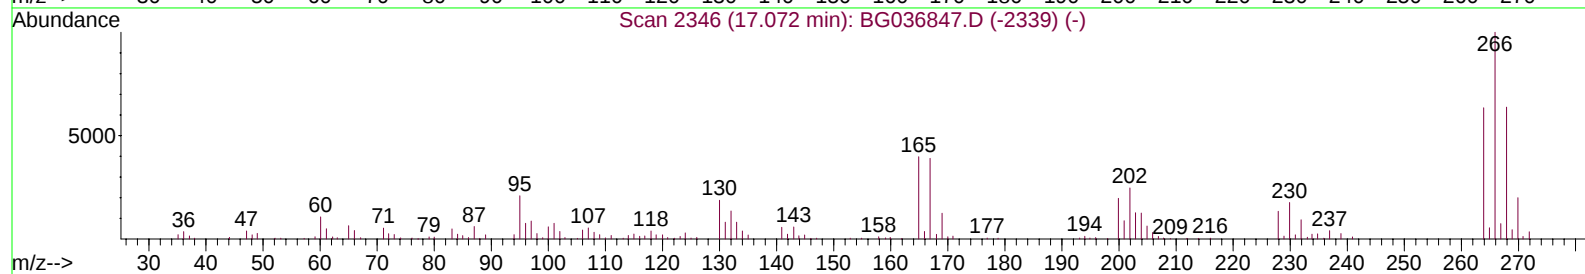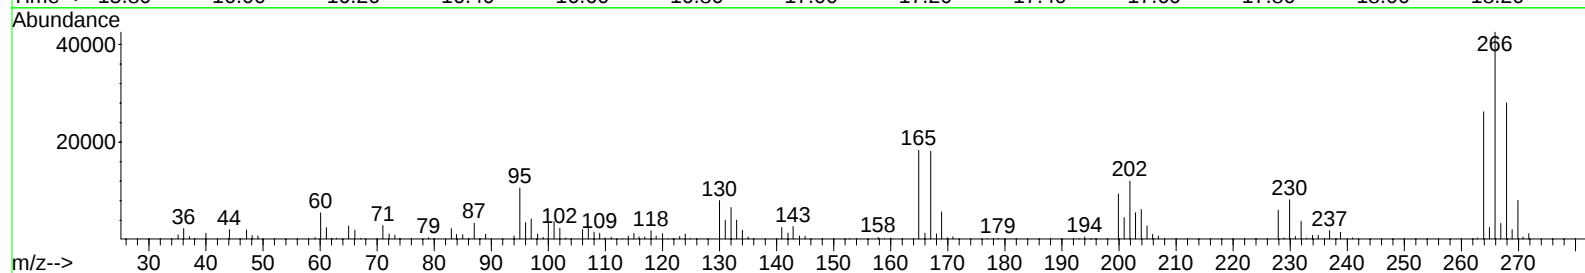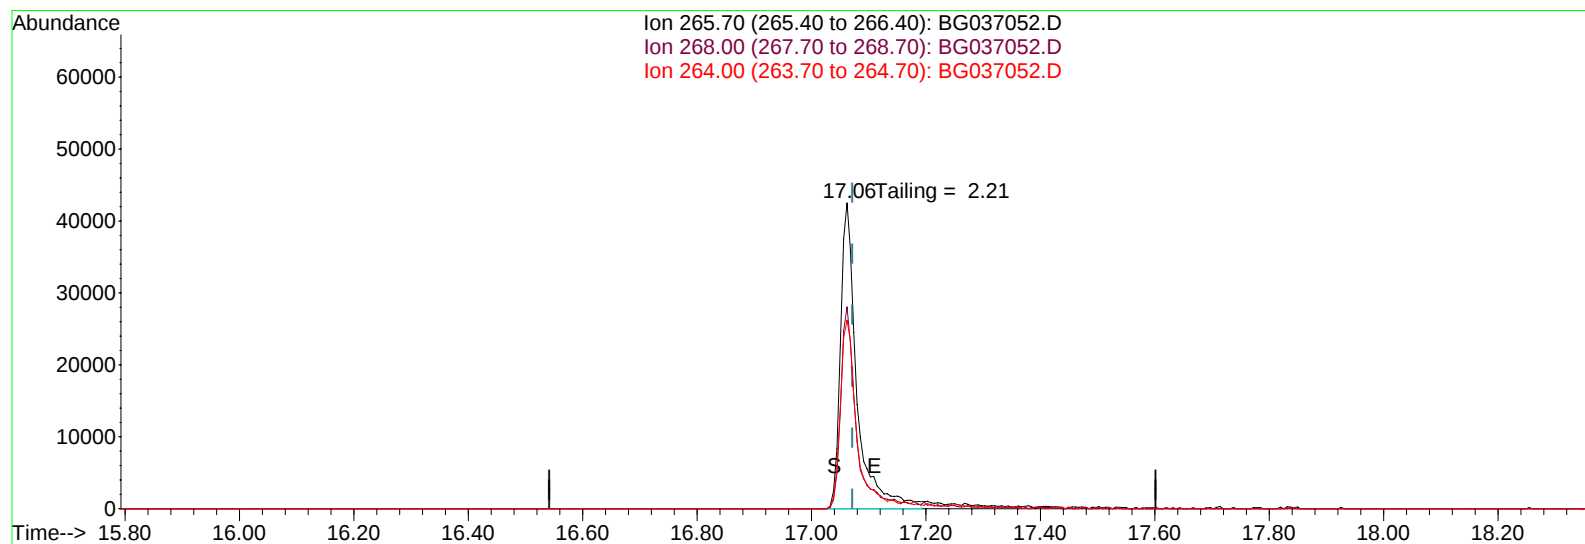

TIC: BG037052.D

(69) Pentachlorophenol (C)

17.062min (-0.010) 15670.20ng

response 85413

Ion	Exp%	Act%
265.70	100	100
268.00	64.30	65.97
264.00	61.10	61.68
0.00	0.00	0.00