
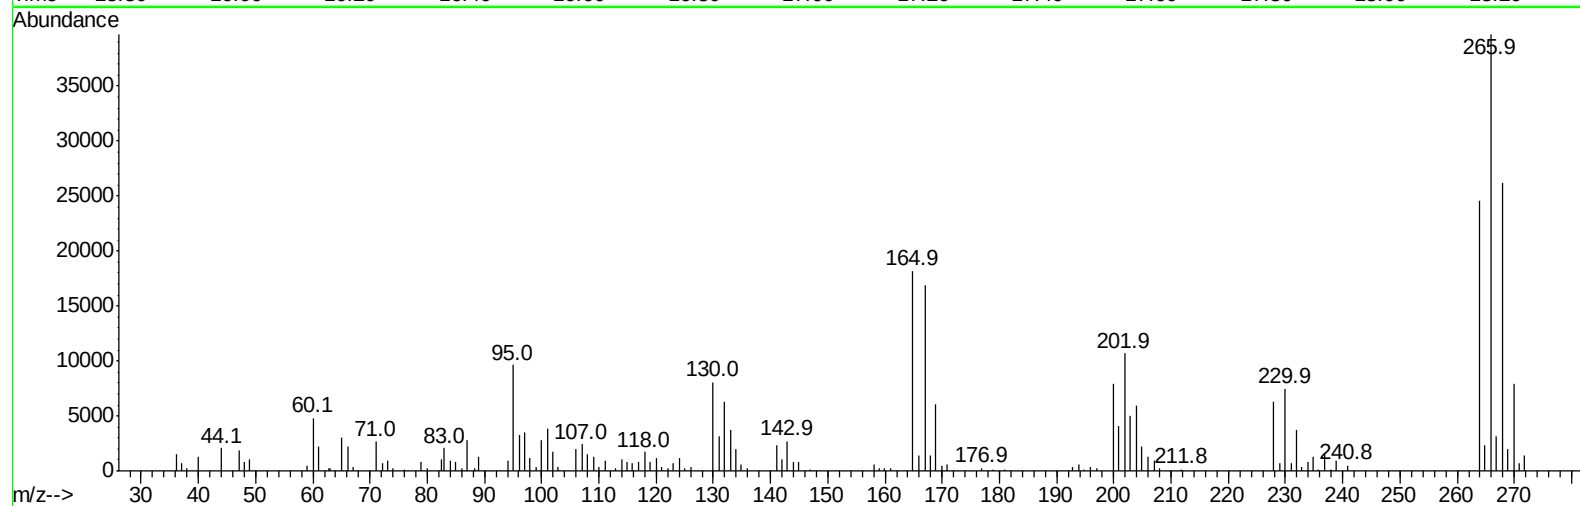


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG092818\
Data File : BG037071.D
Acq On : 29 Sep 2018 5:27
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 01 08:39:48 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG092018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 24 10:41:23 2018
Response via : Initial Calibration

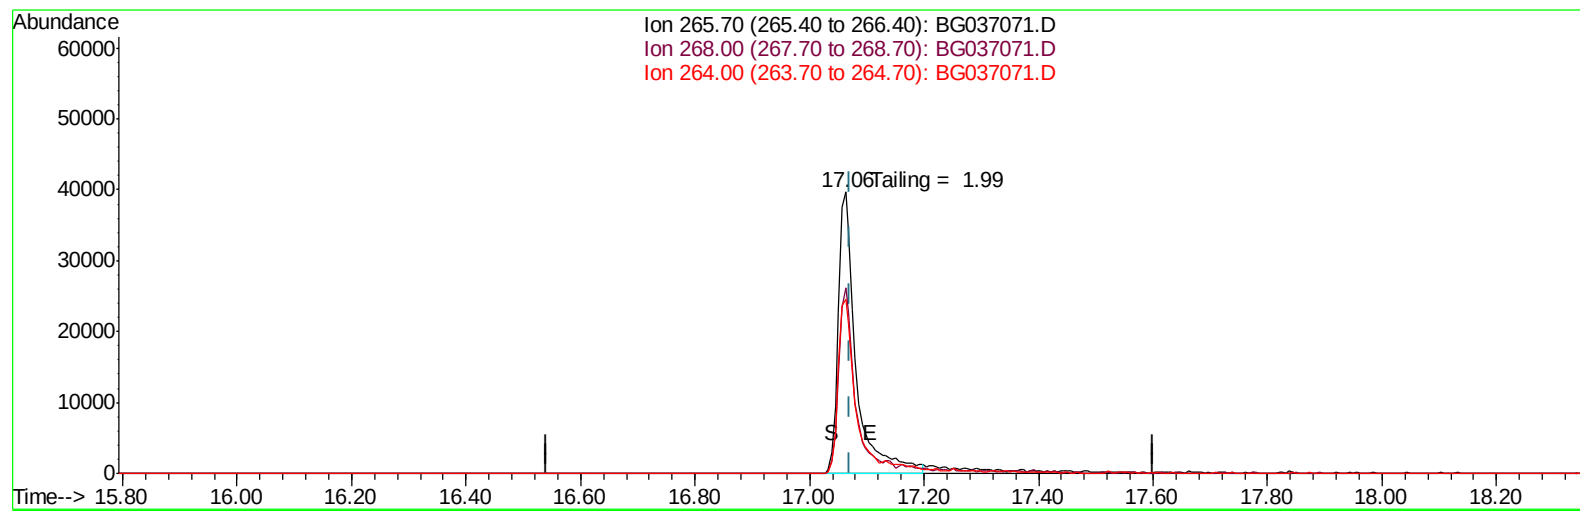

TIC: BG037071.D

(69) Pentachlorophenol (C)



17.062min (-0.009) 18074.54ng

response 86920

Ion	Exp%	Act%
265.70	100	100
268.00	64.30	65.85
264.00	61.10	61.83
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG092818\
Data File : BG037071.D
Acq On : 29 Sep 2018 5:27
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 01 08:39:48 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG092018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 24 10:41:23 2018
Response via : Initial Calibration

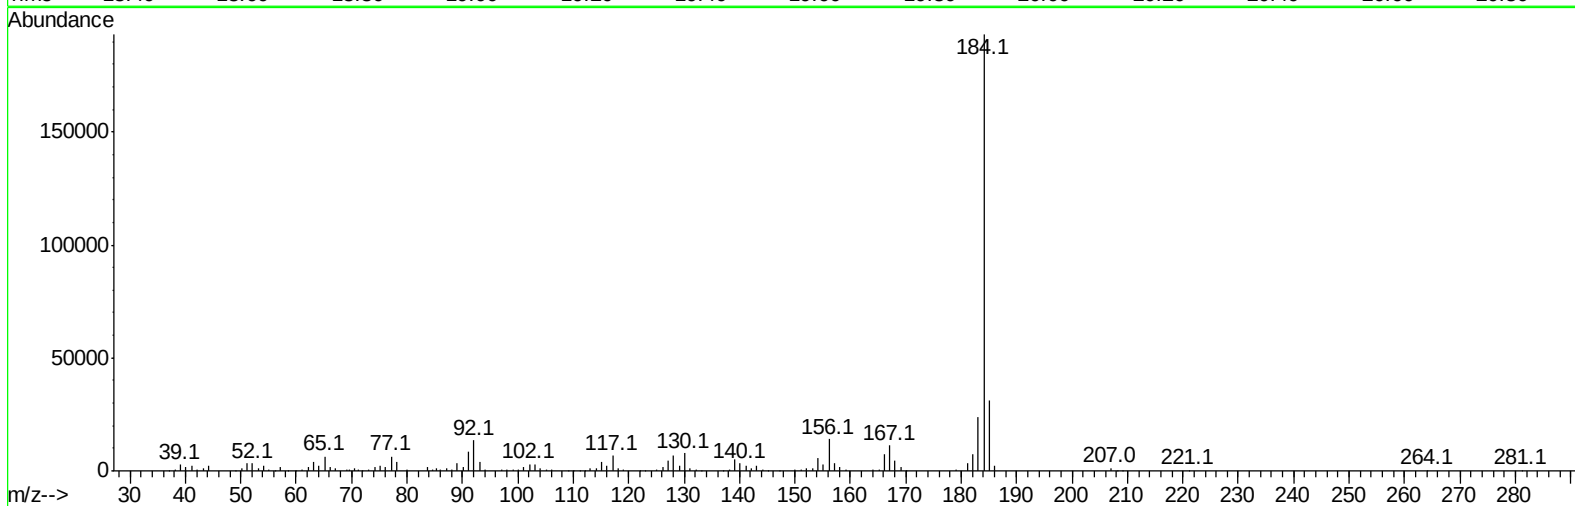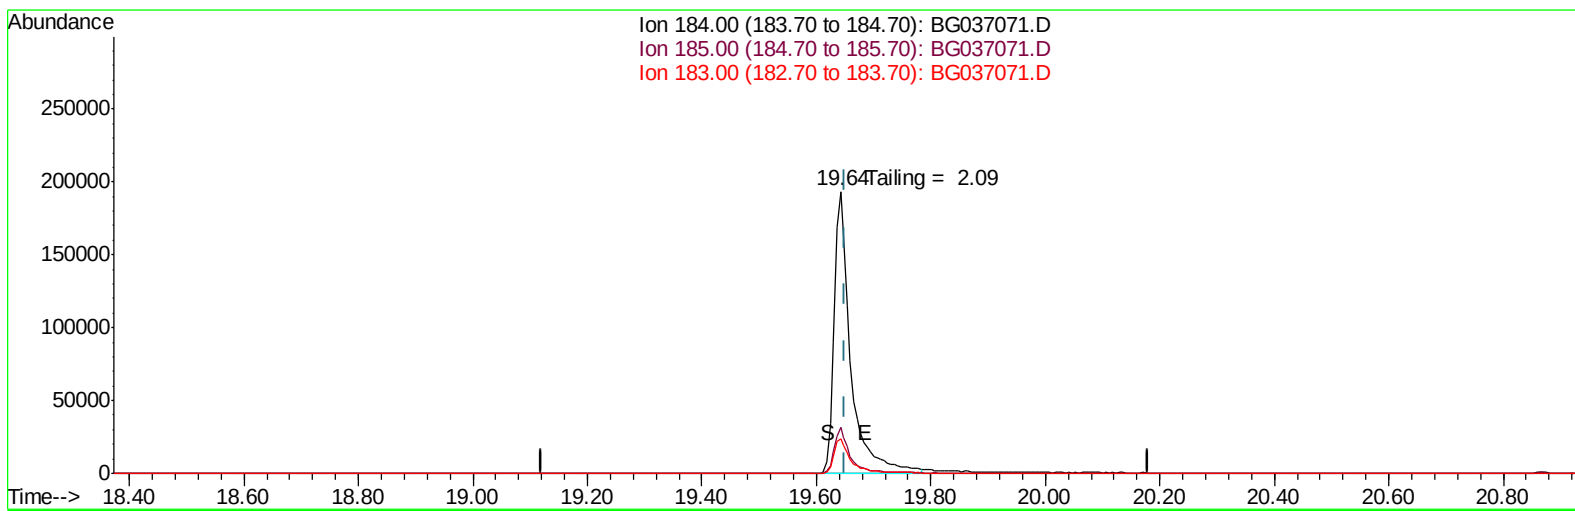

TIC: BG037071.D

(76) Benzidine

19.642min (-0.009) 10486.19ng

response 397511

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	16.18
183.00	13.60	12.39
0.00	0.00	0.00