

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG092818\
 Data File : BG037054.D
 Acq On : 28 Sep 2018 17:46
 Operator : JU/SJ
 Sample : J4777-38
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PL-01-092718-C

Quant Time: Sep 28 19:07:58 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG092018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Sep 24 10:41:23 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.04	152	42243	20.00	ng	0.00
21) Naphthalene-d8	10.84	136	174240	20.00	ng	-0.01
38) Acenaphthene-d10	14.66	164	111520	20.00	ng	-0.01
63) Phenanthrene-d10	17.41	188	284051	20.00	ng	0.00
75) Chrysene-d12	21.67	240	314522	20.00	ng	-0.02
86) Perylene-d12	24.88	264	308284	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.61	112	237941	108.02	ng	0.00
7) Phenol-d6	7.20	99	283032	83.05	ng	-0.01
23) Nitrobenzene-d5	9.20	82	263001	80.83	ng	-0.01
41) 2,4,6-Tribromophenol	16.15	330	148708	111.45	ng	-0.02
44) 2-Fluorobiphenyl	13.29	172	561585	75.00	ng	-0.01
78) Terphenyl-d14	20.01	244	1030441	86.15	ng	-0.01


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG092818\
Data File : BG037054.D
Acq On : 28 Sep 2018 17:46
Operator : JU/SJ
Sample : J4777-38
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PL-01-092718-C

Quant Time: Sep 28 19:07:58 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG092018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 24 10:41:23 2018
Response via : Initial Calibration

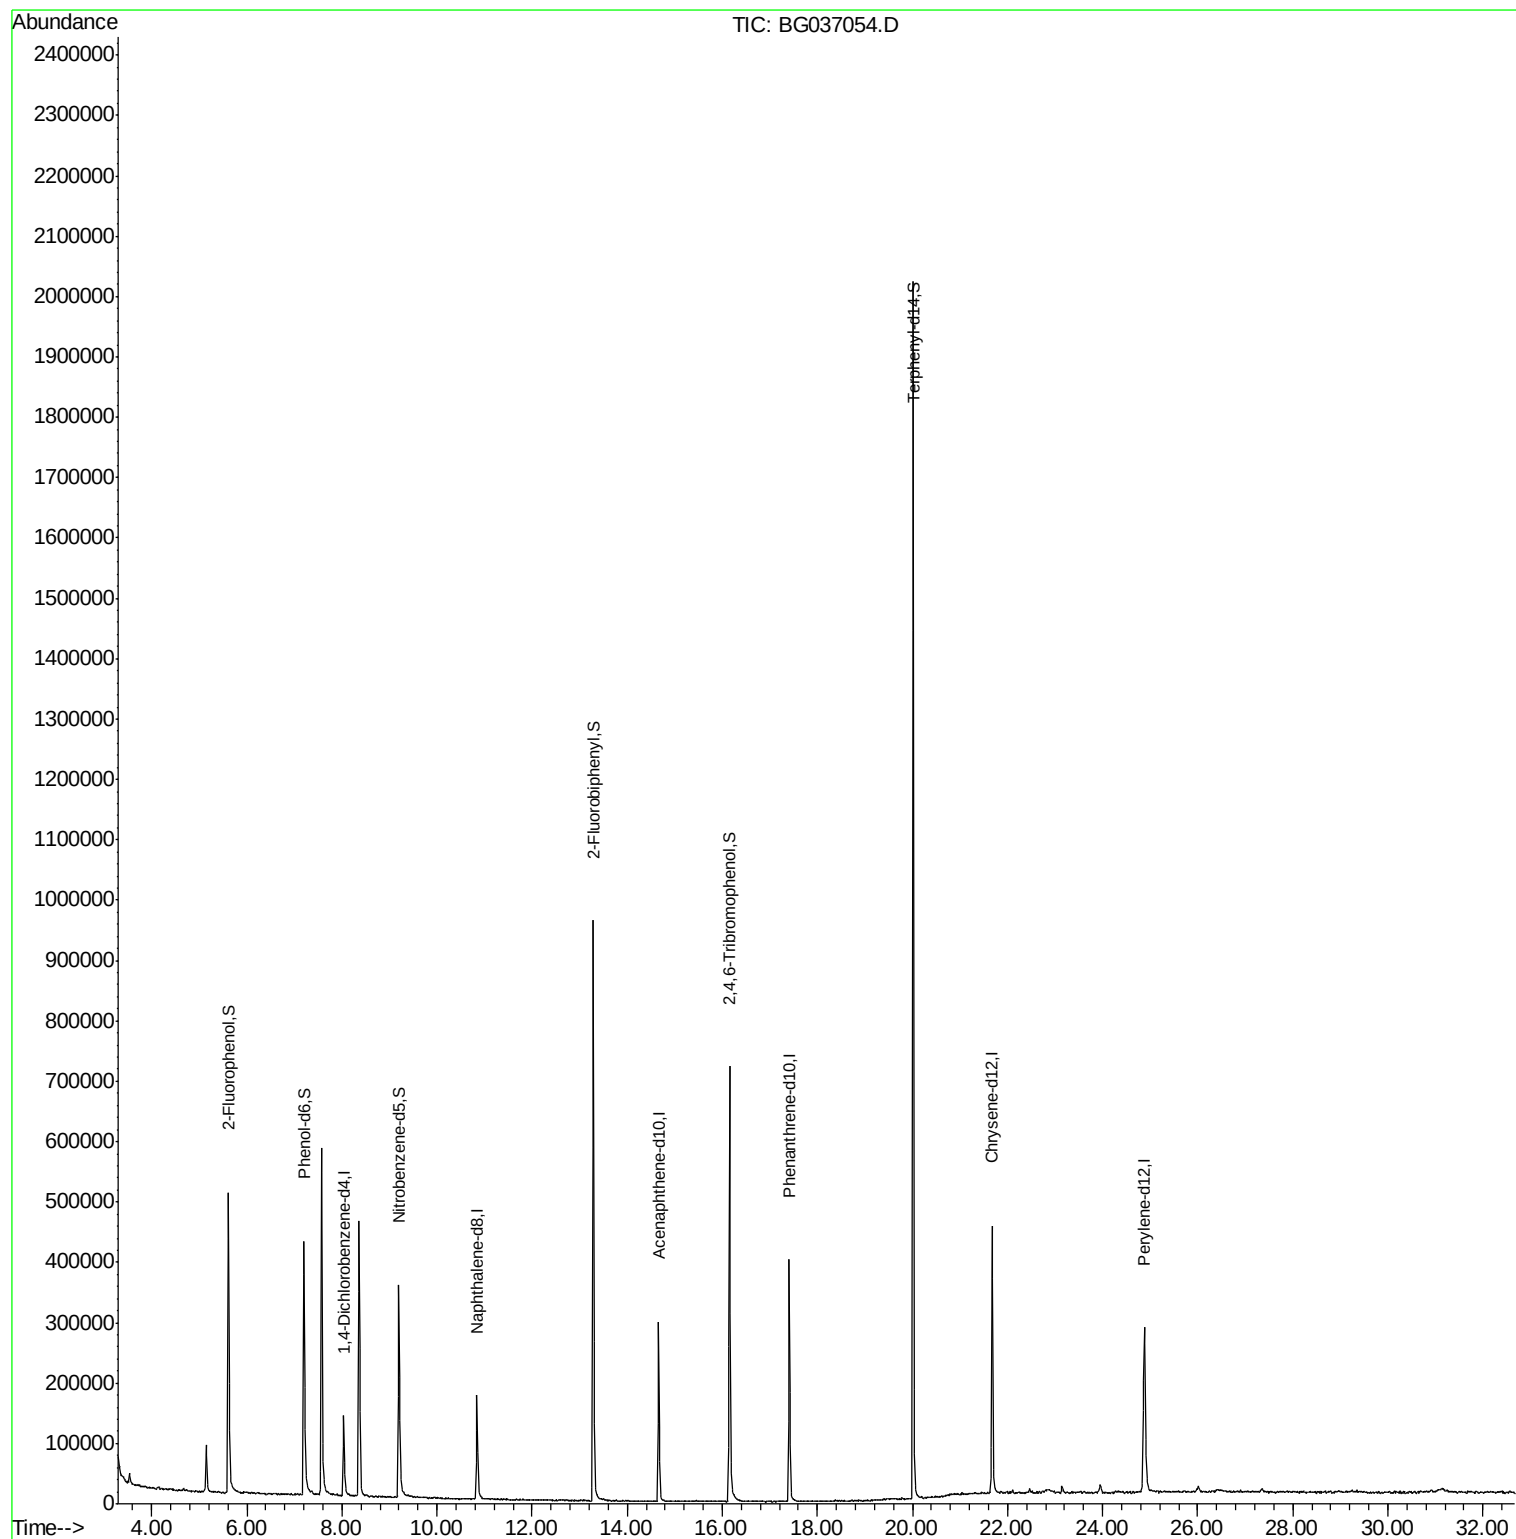

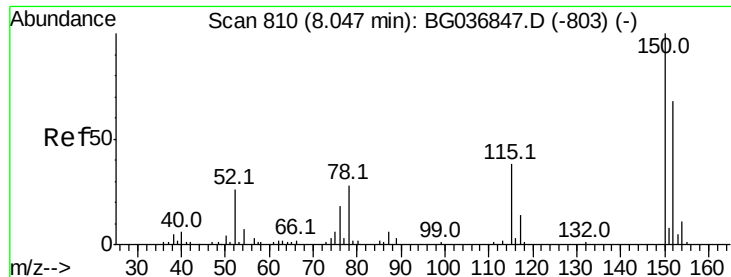


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.04 min Scan# 809
Delta R.T. -0.01 min
Lab File: BG037054.D
Acq: 28 Sep 2018 17:46

Instrument :
BNA_G
ClientSampleId :
PL-01-092718-C

Tot Ion:152 Resp: 42243
Ion Ratio Lower Upper
152 100
150 157.4 119.5 179.3
115 61.3 44.5 66.7

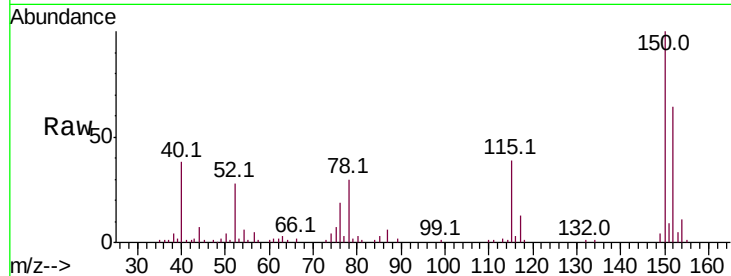


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

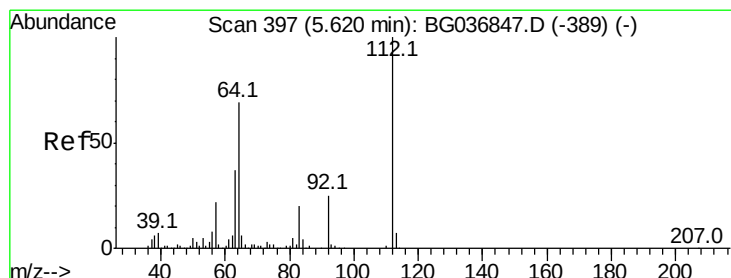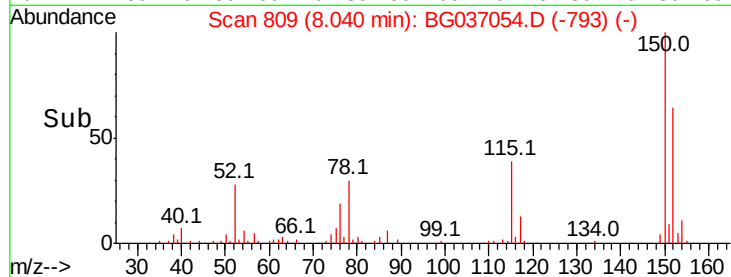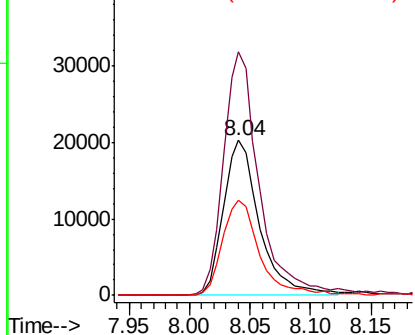



#5


2-Fluorophenol
Concen: 108.022 ng
RT: 5.61 min Scan# 396
Delta R.T. -0.01 min
Lab File: BG037054.D
Acq: 28 Sep 2018 17:46

Tgt Ion:112 Resp: 237941
Ion Ratio Lower Upper
112 100
64 72.6 57.2 85.8
63 38.2 30.8 46.2

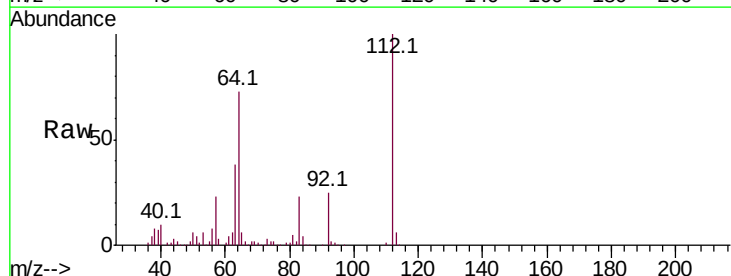

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG
Ion 63.00 (62.70 to 63.70): BG

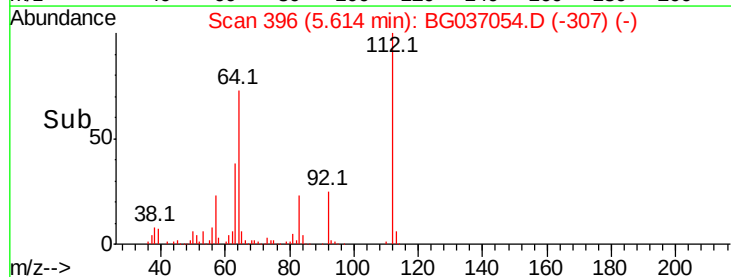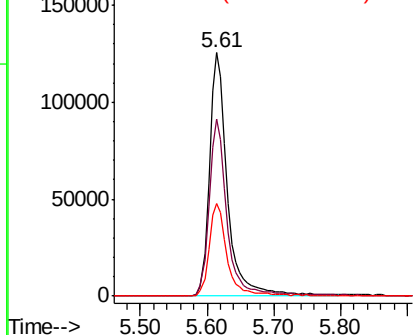

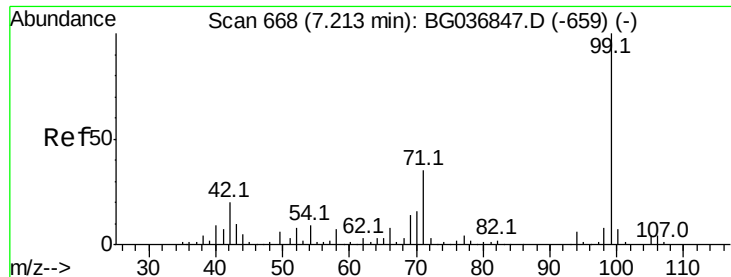

#7

Phenol-d6

Concen: 83.050 ng

RT: 7.20 min Scan# 666

Delta R.T. -0.01 min

Lab File: BG037054.D

Acq: 28 Sep 2018 17:46

Instrument :

BNA_G

ClientSampleId :

PL-01-092718-C


Tot Ion: 99 Resp: 283032

Ion Ratio Lower Upper




99 100

42 23.6 16.5 24.7

71 36.7 29.4 44.2

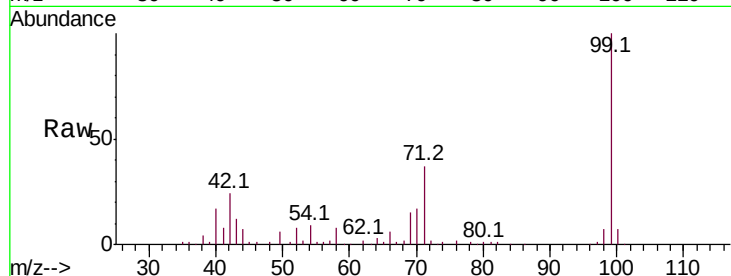

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

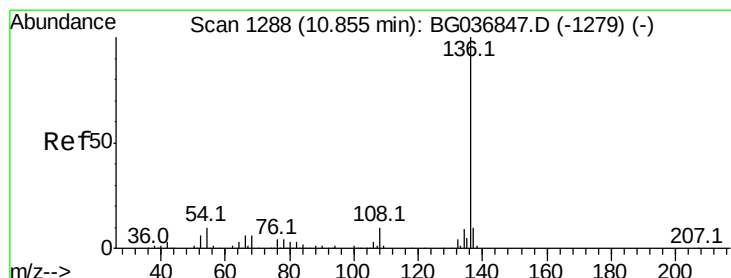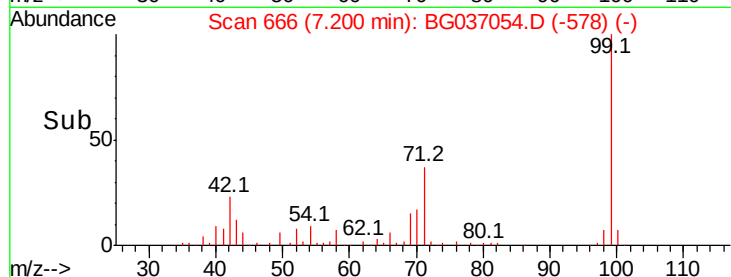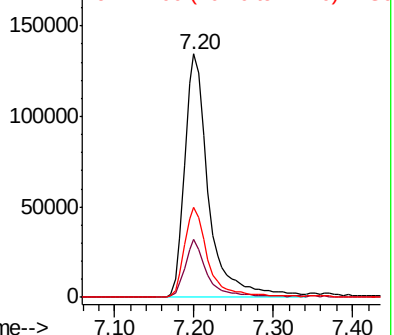

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.84 min Scan# 1286

Delta R.T. -0.01 min

Lab File: BG037054.D

Acq: 28 Sep 2018 17:46

Tgt Ion: 136 Resp: 174240


Ion Ratio Lower Upper

136 100



137 9.7 8.8 13.2


54 11.6 9.2 13.8

68 6.9 5.8 8.6

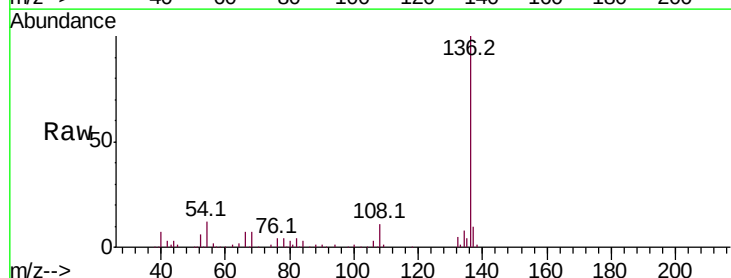

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



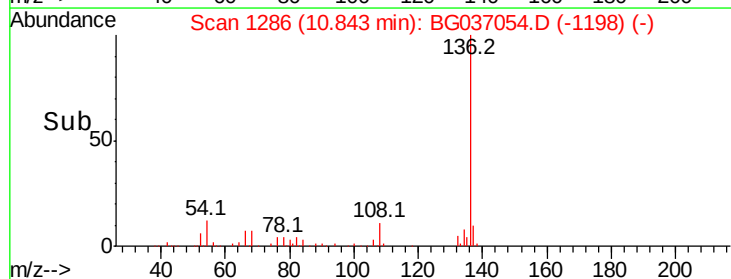
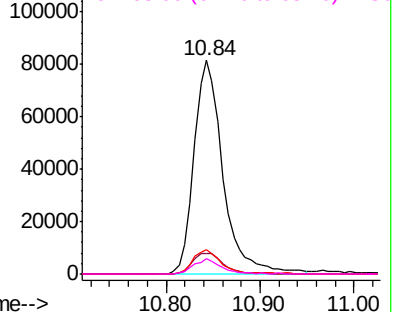


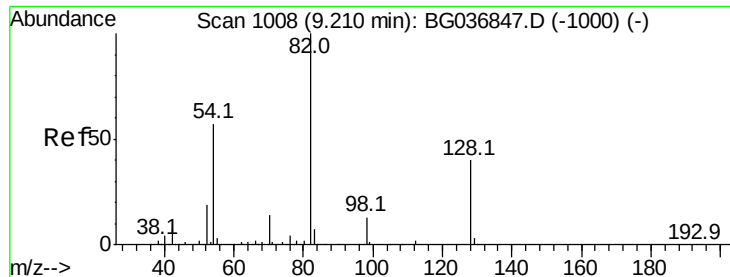

#23
 Nitrobenzene-d5
 Concen: 80.831 ng
 RT: 9.20 min Scan# 1006
 Delta R.T. -0.01 min
 Lab File: BG037054.D
 Acq: 28 Sep 2018 17:46




Instrument :
 BNA_G
 ClientSampleId :
 PL-01-092718-C


Tot Ion	82	Resp	263001
Ion Ratio	Lower	Upper	
82	100		
128	39.1	33.3	49.9
54	56.7	45.1	67.7

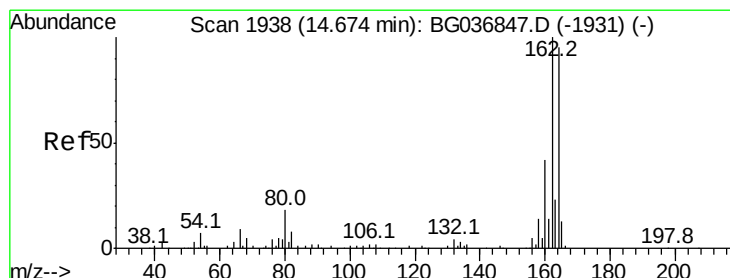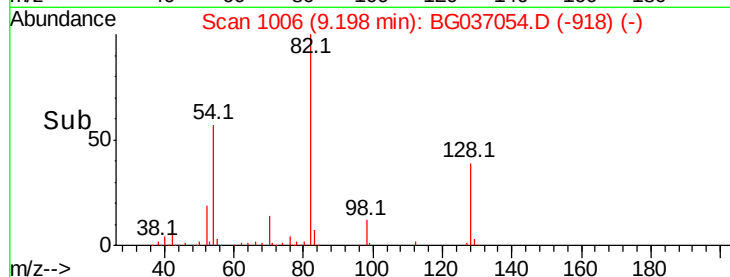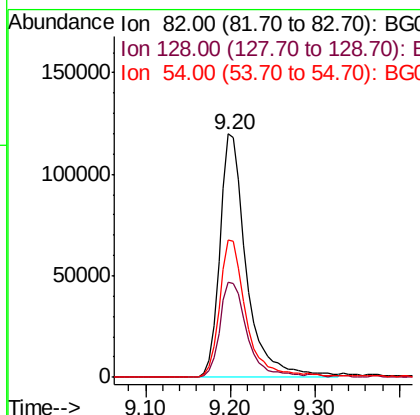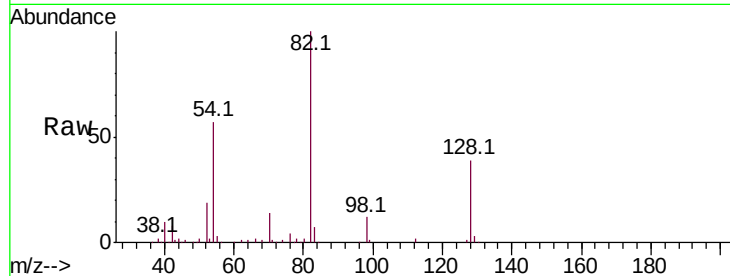

#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.66 min Scan# 1936
 Delta R.T. -0.01 min
 Lab File: BG037054.D
 Acq: 28 Sep 2018 17:46

Tgt Ion	164	Resp	111520
Ion Ratio	Lower	Upper	
164	100		
162	101.2	80.7	121.1
160	43.9	35.3	52.9

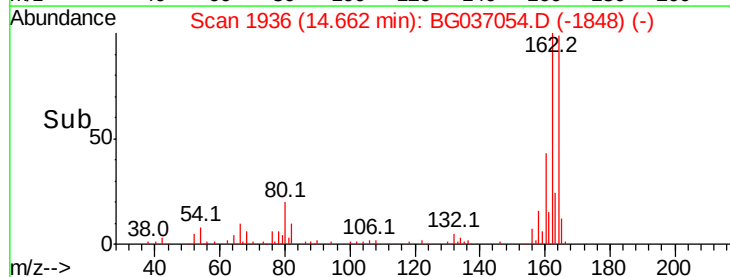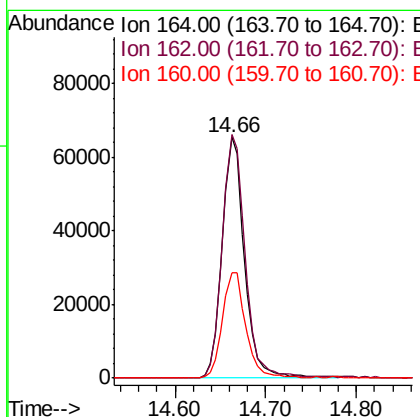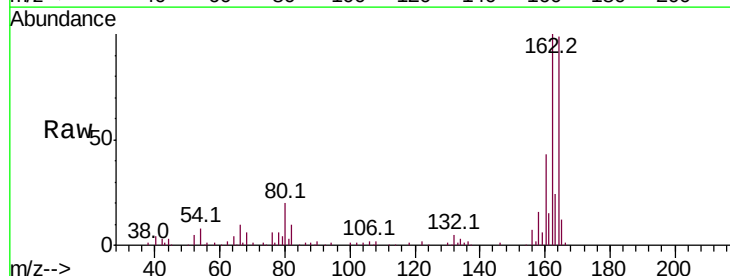


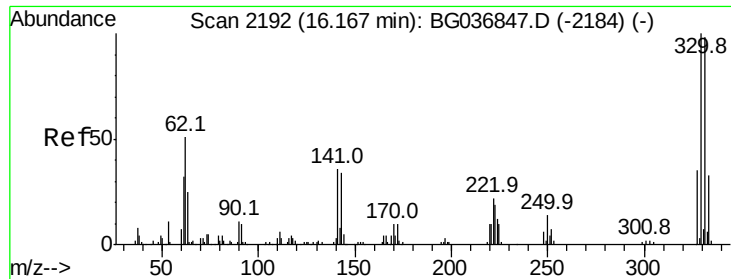




#41
 2,4,6-Tribromophenol
 Concen: 111.453 ng
 RT: 16.15 min Scan# 2189
 Delta R.T. -0.02 min
 Lab File: BG037054.D
 Acq: 28 Sep 2018 17:46

Instrument :
 BNA_G
 ClientSampleId :
 PL-01-092718-C

Tot Ion:330 Resp: 148708
 Ion Ratio Lower Upper
 330 100
 332 95.4 75.4 113.2
 141 39.9 30.7 46.1

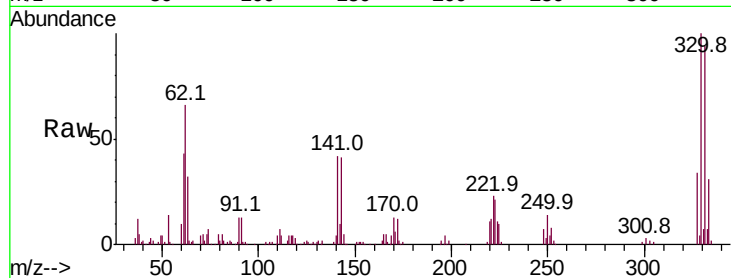


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

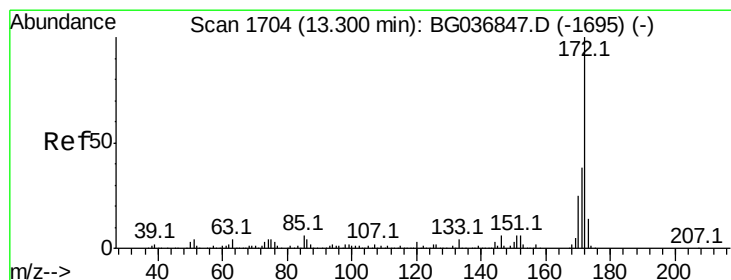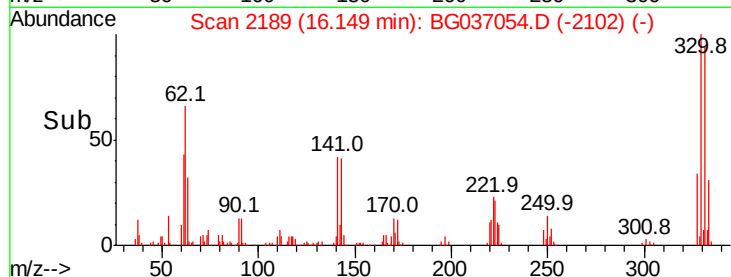
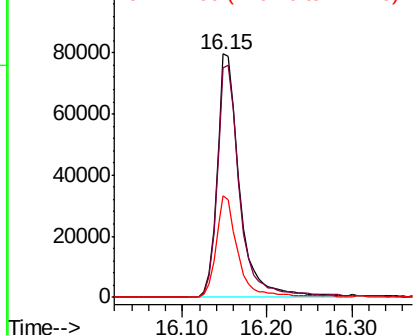



#44
 2-Fluorobiphenyl
 Concen: 75.002 ng
 RT: 13.29 min Scan# 1702
 Delta R.T. -0.01 min
 Lab File: BG037054.D
 Acq: 28 Sep 2018 17:46

Tgt Ion:172 Resp: 561585
 Ion Ratio Lower Upper
 172 100
 171 38.4 31.3 46.9
 170 24.6 21.0 31.6

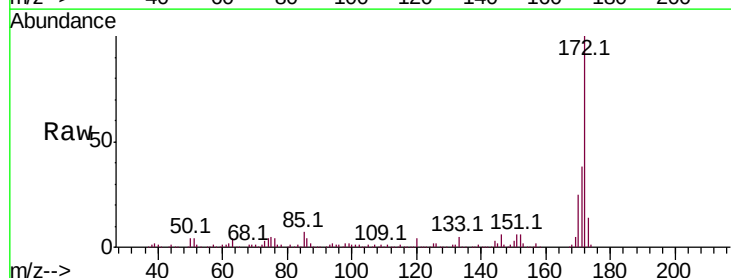

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



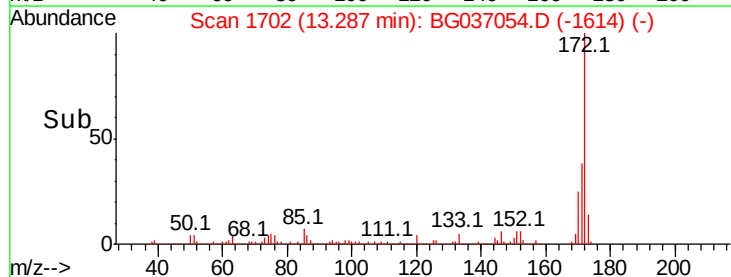
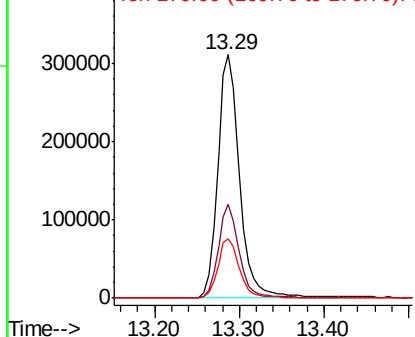


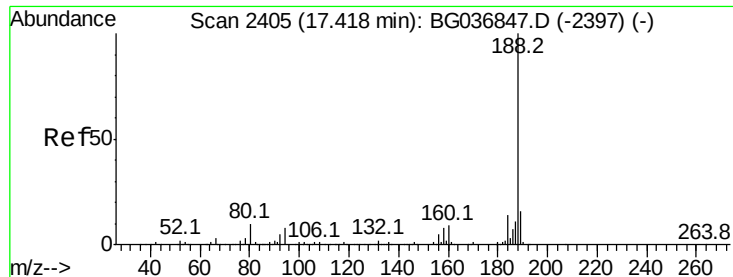

#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.41 min Scan# 2404
Delta R.T. -0.01 min
Lab File: BG037054.D
Acq: 28 Sep 2018 17:46




Instrument :
BNA_G
ClientSampleId :
PL-01-092718-C


Tot Ion:188 Resp: 284051
Ion Ratio Lower Upper
188 100
94 7.7 6.7 10.1
80 10.0 8.1 12.1

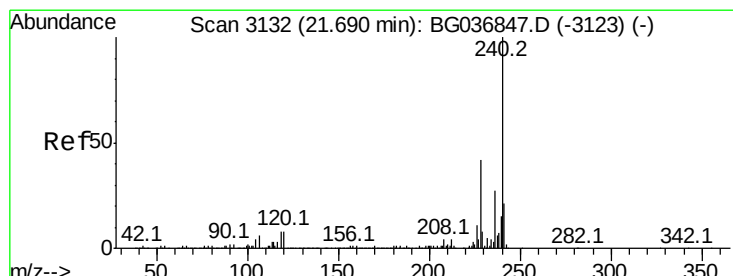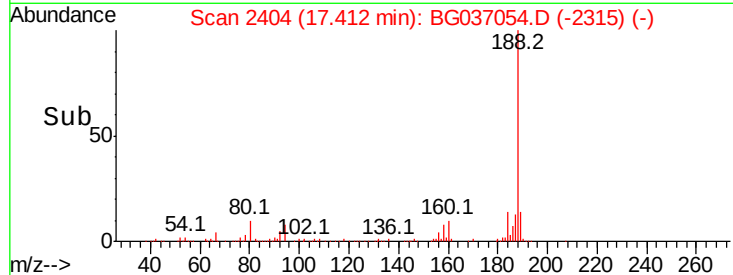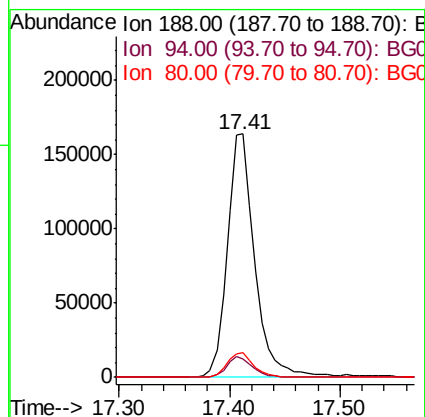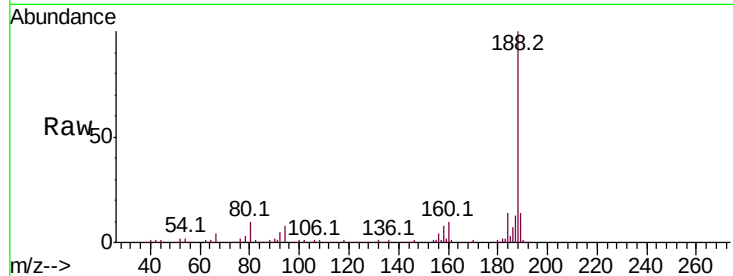

#75
Chrysene-d12
Concen: 20.000 ng
RT: 21.67 min Scan# 3129
Delta R.T. -0.02 min
Lab File: BG037054.D
Acq: 28 Sep 2018 17:46

Tgt Ion:240 Resp: 314522
Ion Ratio Lower Upper
240 100
120 8.8 6.9 10.3
236 25.8 21.2 31.8


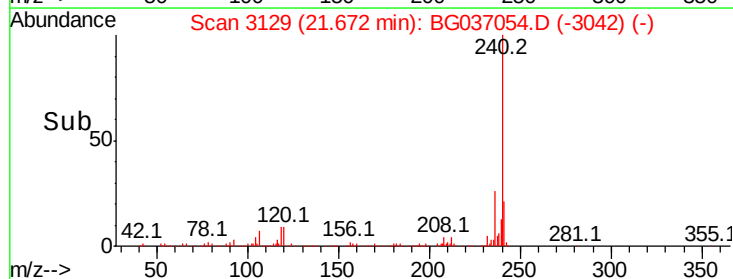
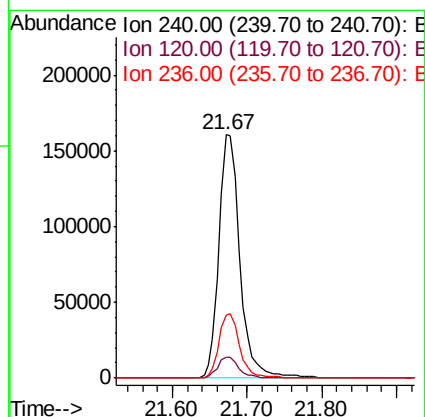
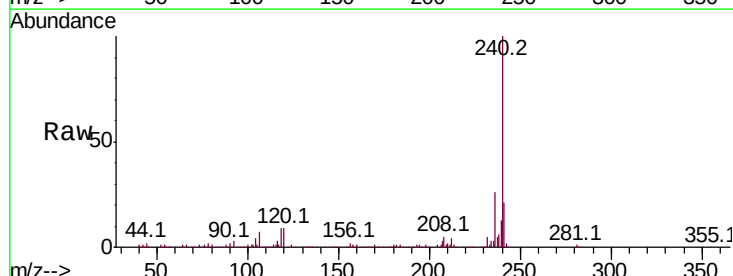


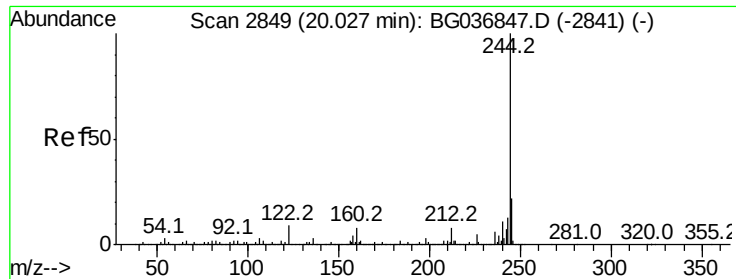

#78
 Terphenyl-d14
 Concen: 86.148 ng
 RT: 20.01 min Scan# 2847
 Delta R.T. -0.01 min
 Lab File: BG037054.D
 Acq: 28 Sep 2018 17:46

Instrument :
 BNA_G
 ClientSampleId :
 PL-01-092718-C

Tot Ion:244 Resp: 1030441
 Ion Ratio Lower Upper
 244 100
 212 8.3 7.0 10.6
 122 9.8 7.1 10.7

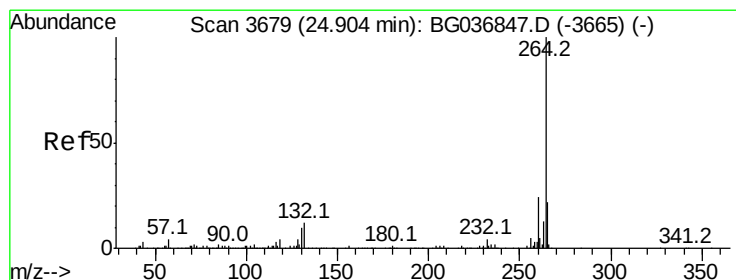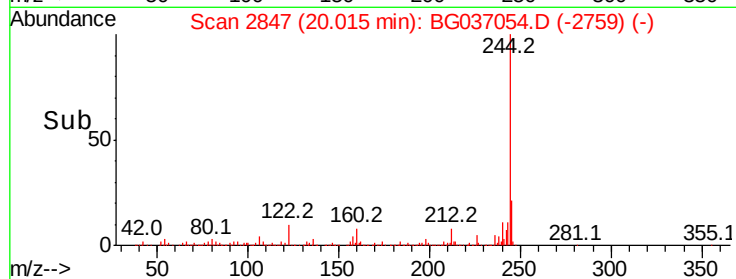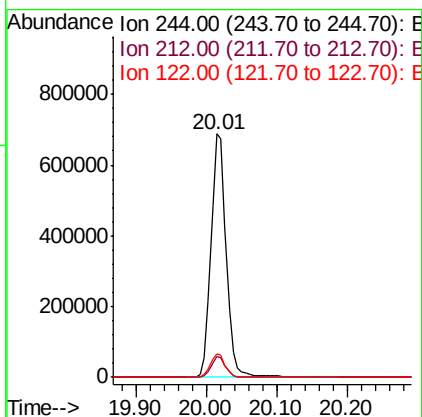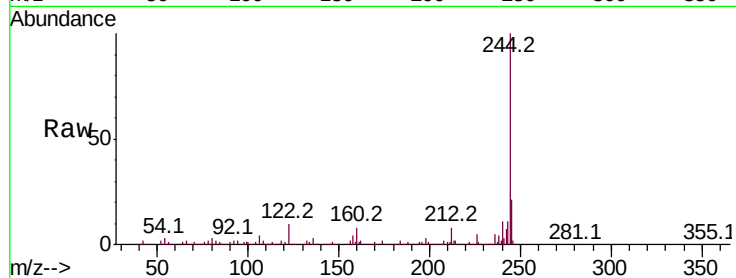

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 24.88 min Scan# 3675
 Delta R.T. -0.02 min
 Lab File: BG037054.D
 Acq: 28 Sep 2018 17:46

Tgt Ion:264 Resp: 308284
 Ion Ratio Lower Upper
 264 100
 260 23.6 19.6 29.4
 265 21.8 17.4 26.0

