


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG092818\
 Data File : BG037052.D
 Acq On : 28 Sep 2018 16:29
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092018.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Sep 24 10:41:23 2018

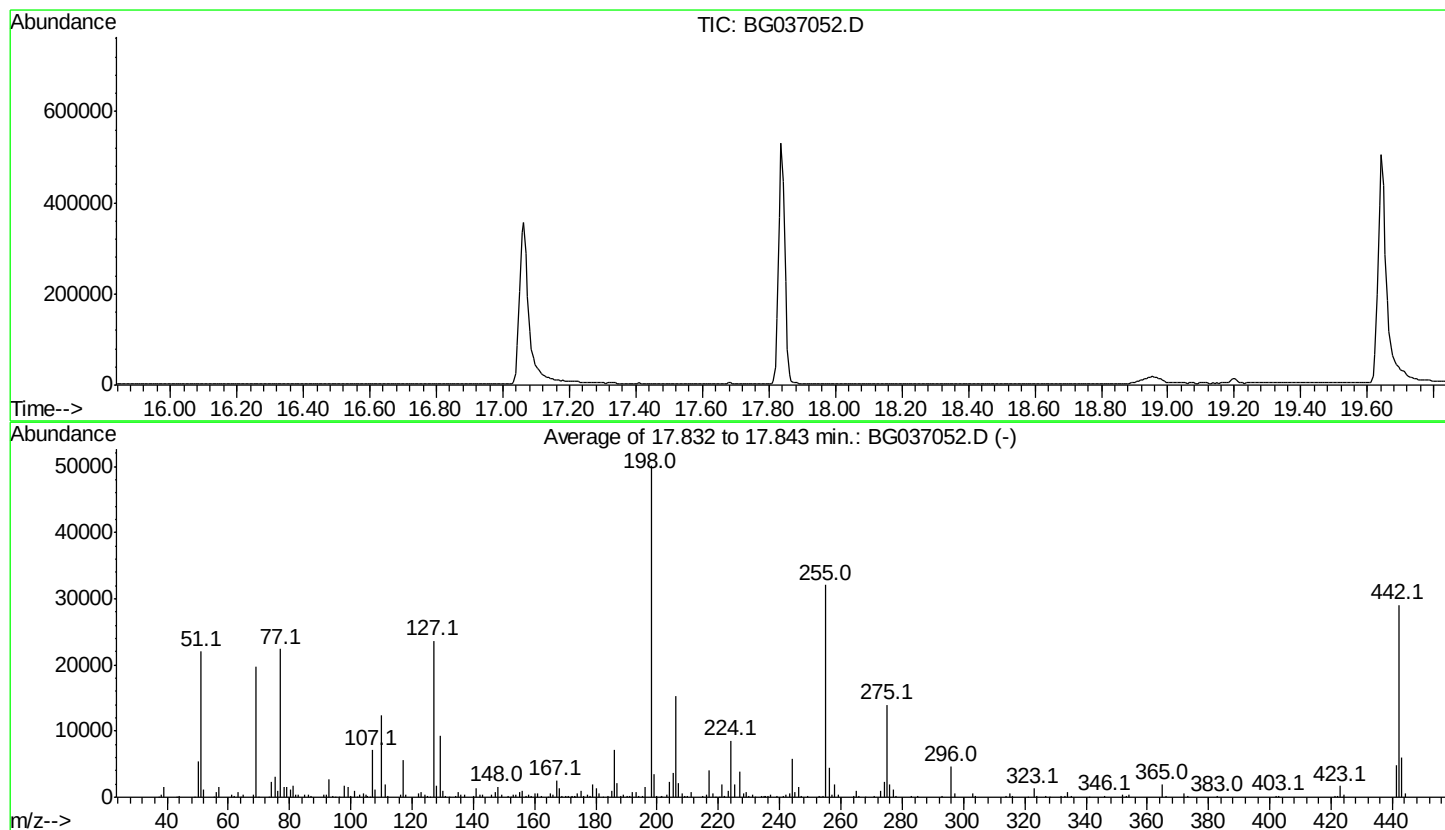

AutoFind: Scans 2475, 2476, 2477; Background Corrected with Scan 2469

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.9	22018	PASS
68	69	0.00	2	1.6	308	PASS
69	198	0.00	100	39.5	19805	PASS
70	69	0.00	2	0.3	52	PASS
127	198	10	80	47.1	23629	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	50149	PASS
199	198	5	9	7.1	3585	PASS
275	198	10	60	27.8	13964	PASS
365	198	1	100	3.8	1929	PASS
441	198	0.01	100	9.7	4861	PASS
442	198	50	100	58.1	29125	PASS
443	442	15	24	20.7	6027	PASS