


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG092818\
 Data File : BG037071.D
 Acq On : 29 Sep 2018 5:27
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092018.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Sep 24 10:41:23 2018

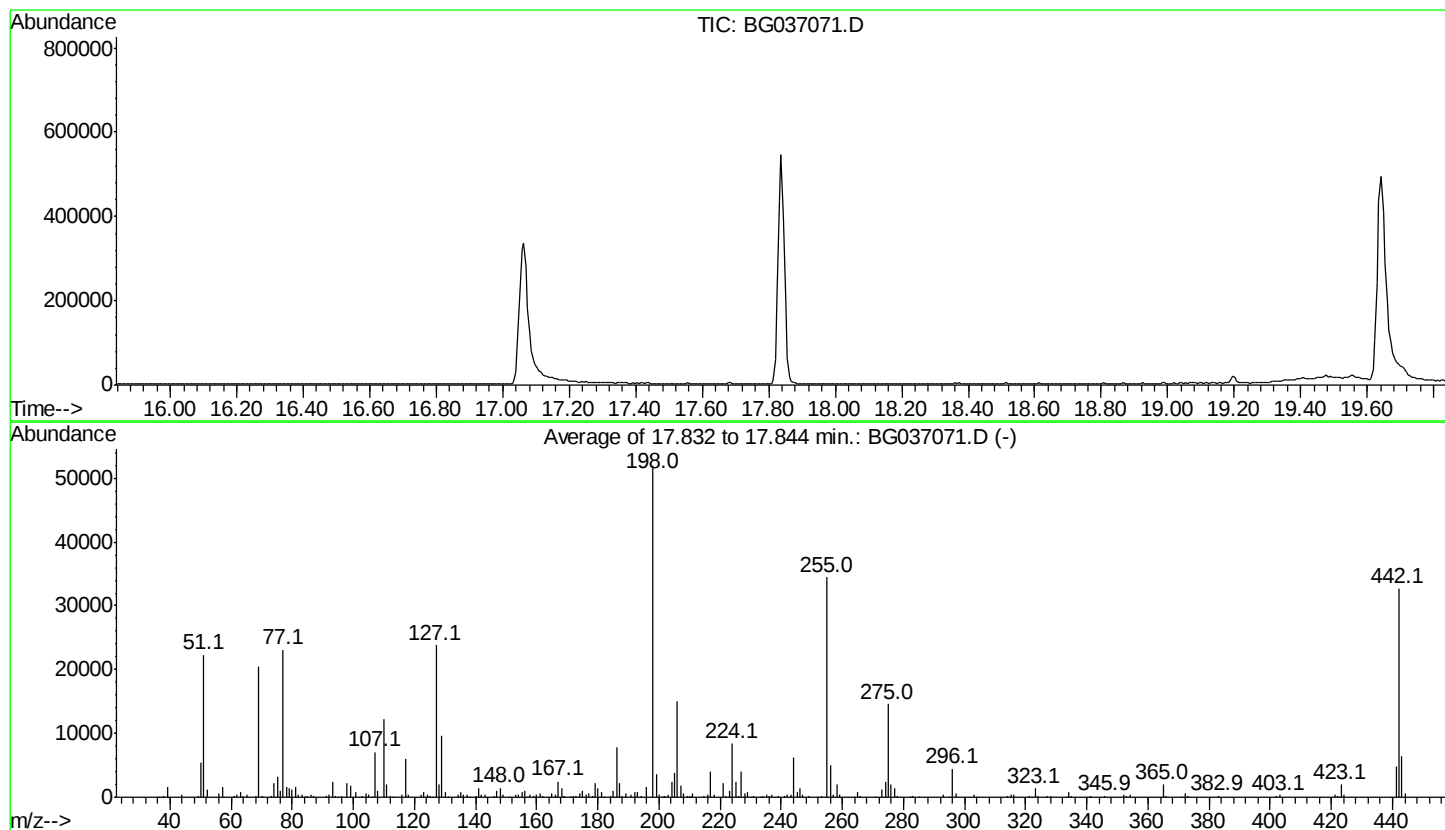

AutoFind: Scans 2475, 2476, 2477; Background Corrected with Scan 2468

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.0	22330	PASS
68	69	0.00	2	1.0	196	PASS
69	198	0.00	100	39.4	20496	PASS
70	69	0.00	2	0.8	155	PASS
127	198	10	80	45.9	23853	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	51968	PASS
199	198	5	9	7.2	3716	PASS
275	198	10	60	28.0	14553	PASS
365	198	1	100	3.8	1967	PASS
441	198	0.01	100	9.5	4921	PASS
442	198	50	100	62.8	32661	PASS
443	442	15	24	19.9	6502	PASS