
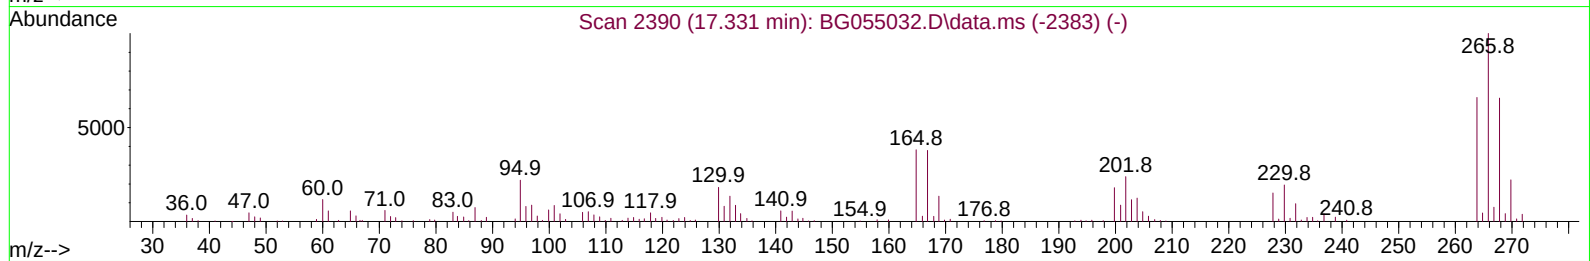
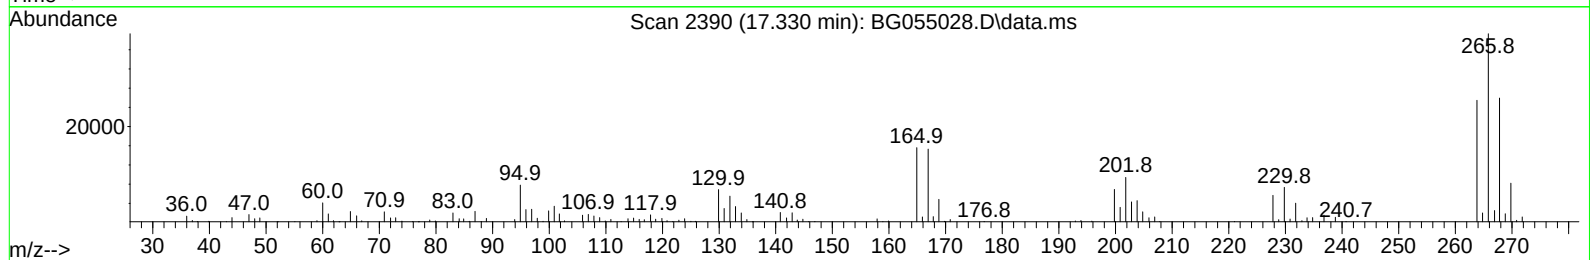


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092822\
Data File : BG055028.D
Acq On : 28 Sep 2022 9:51
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 28 17:10:00 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG092822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 28 15:43:39 2022
Response via : Initial Calibration

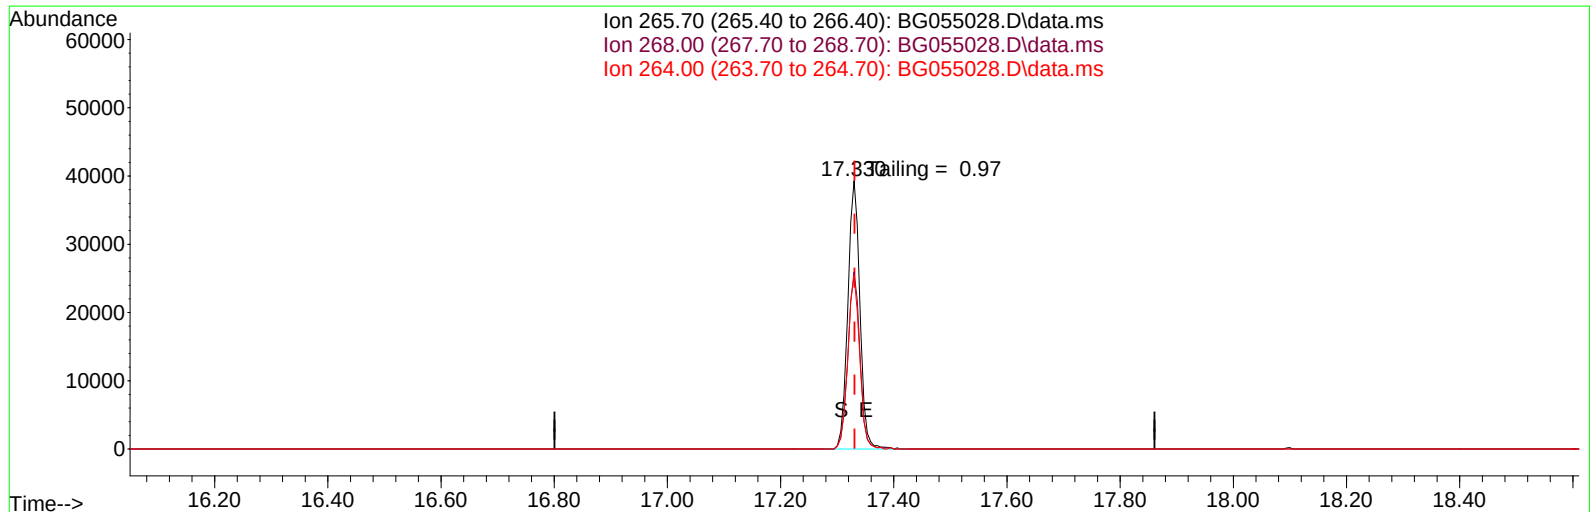

TIC: BG055028.D\data.ms

(70) Pentachlorophenol (C)




17.330min (-0.001) 27531.65 ng

response 58093

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	65.93
264.00	61.70	64.73
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092822\
Data File : BG055028.D
Acq On : 28 Sep 2022 9:51
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 28 17:10:00 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG092822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 28 15:43:39 2022
Response via : Initial Calibration

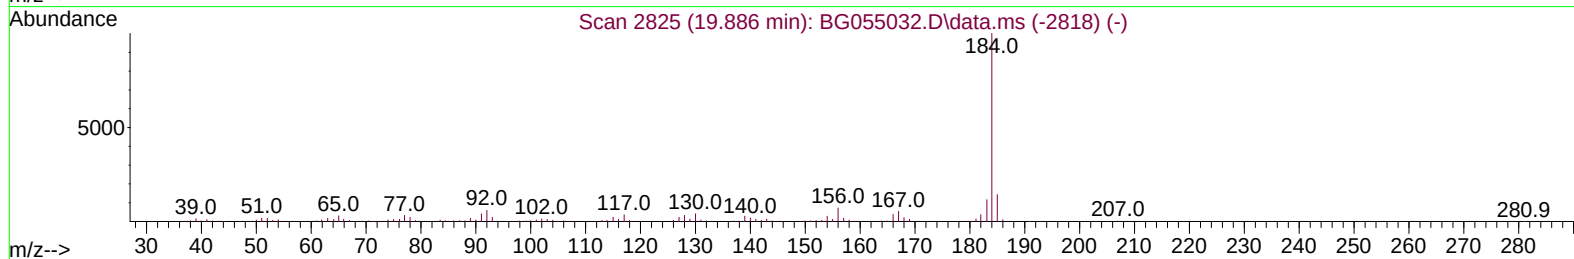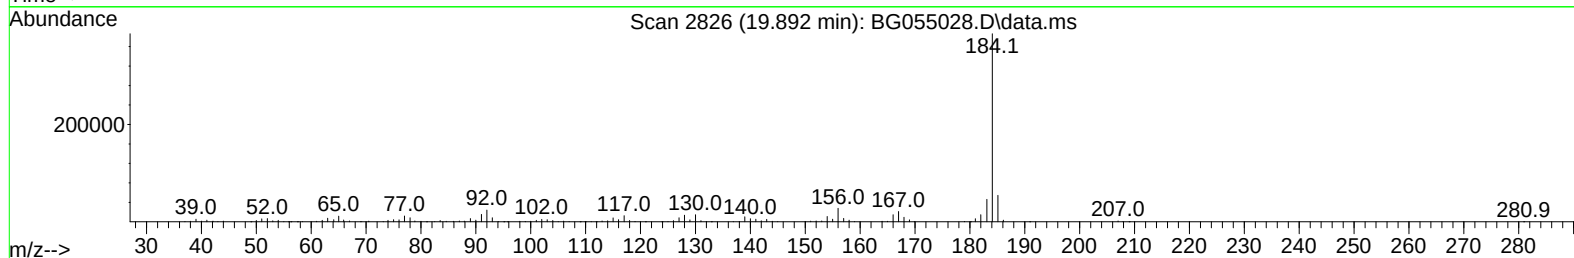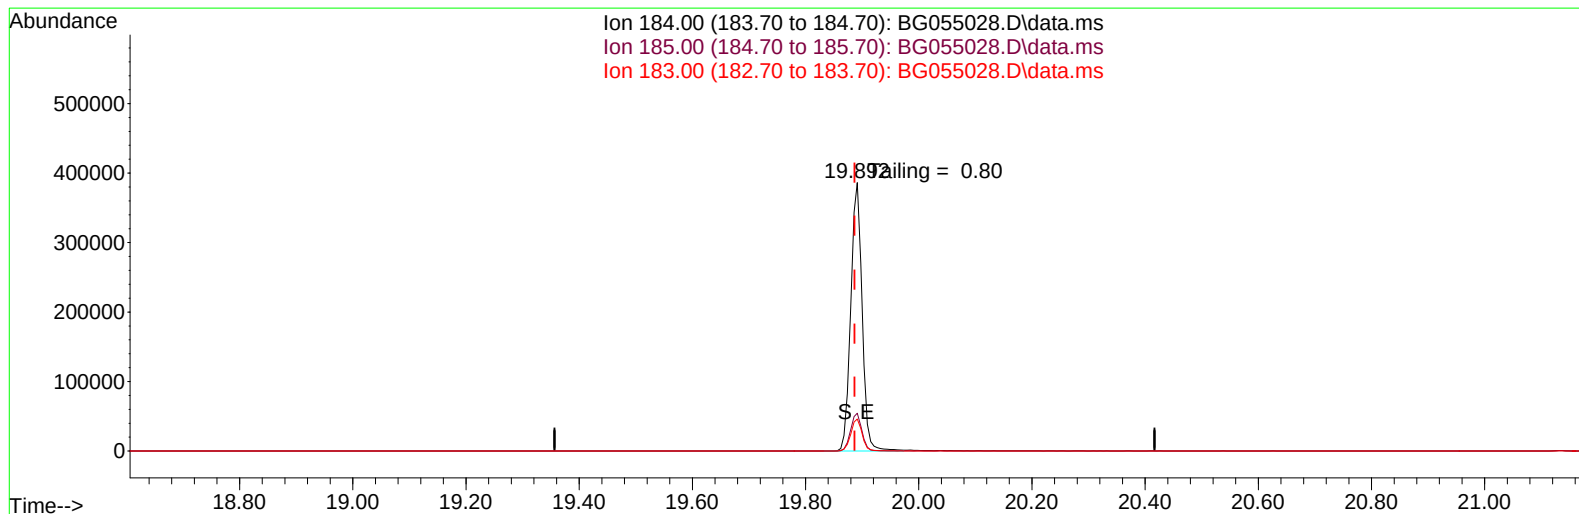

TIC: BG055028.D\data.ms

(77) Benzidine**19.892min (+ 0.005) 0.00 ng****response 538765**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.09
183.00	12.30	11.96
0.00	0.00	0.00