


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092822\
Data File : BG055028.D
Acq On : 28 Sep 2022 9:51
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG092822.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Sep 28 15:43:39 2022

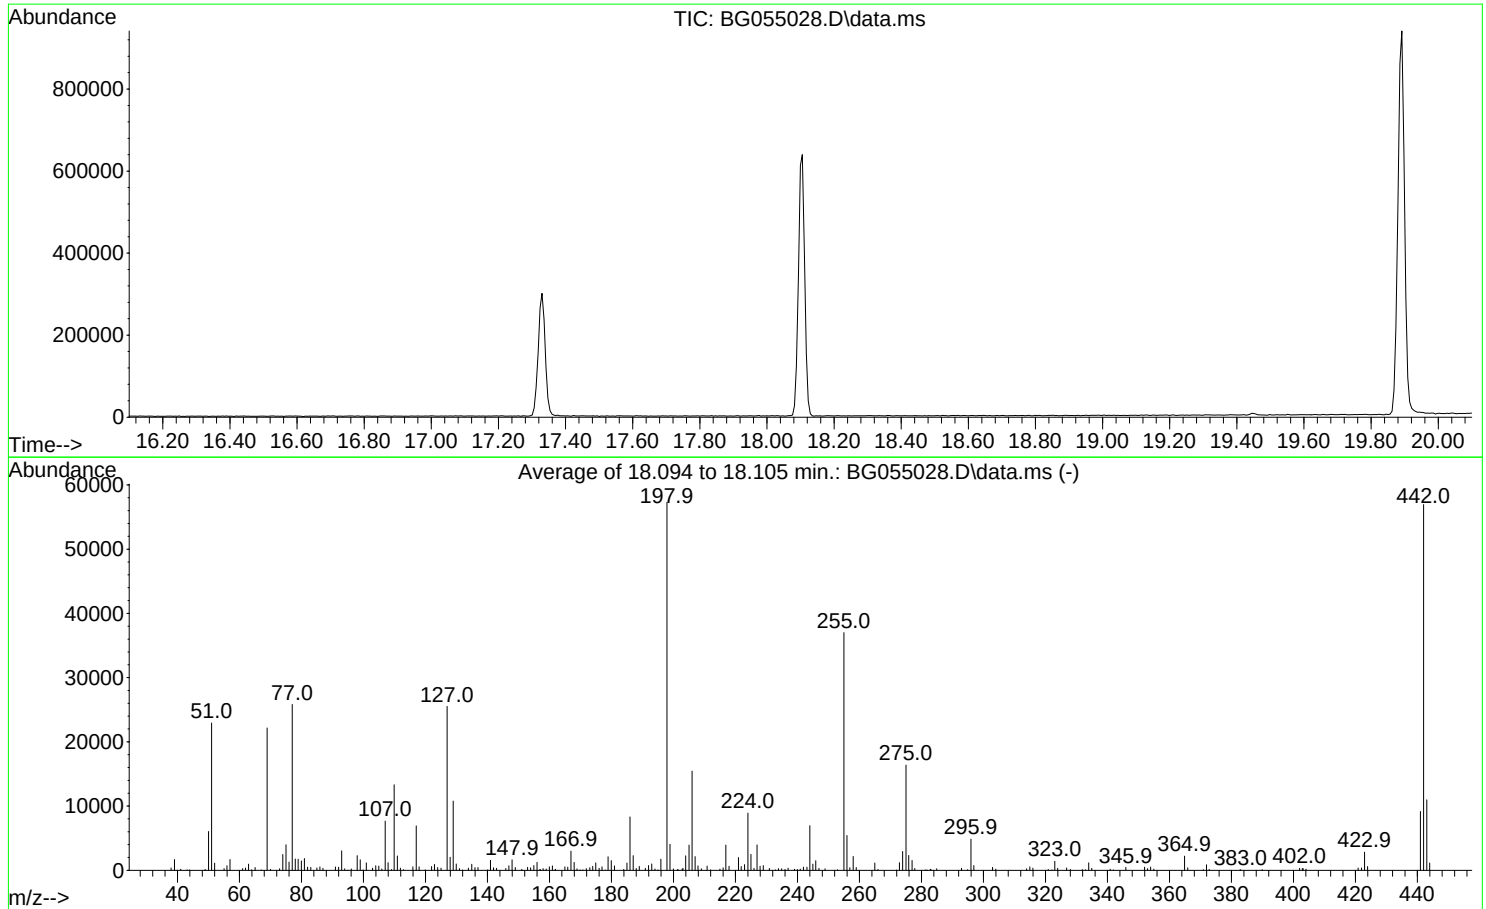




AutoFind: Scans 2520, 2521, 2522; Background Corrected with Scan 2514

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.0	22933	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	38.7	22173	PASS
70	69	0.00	2	0.7	146	PASS
127	198	10	80	44.6	25531	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	57277	PASS
199	198	5	9	7.1	4061	PASS
275	198	10	60	28.6	16390	PASS
365	198	1	100	3.8	2204	PASS
441	198	0.01	100	16.0	9162	PASS
442	442	50	100	100.0	56936	PASS
443	442	15	24	19.3	10972	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092822\
Data File : BG055028.D
Acq On : 28 Sep 2022 9:51
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Sep 28 17:10:00 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG092822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 28 15:43:39 2022
Response via : Initial Calibration

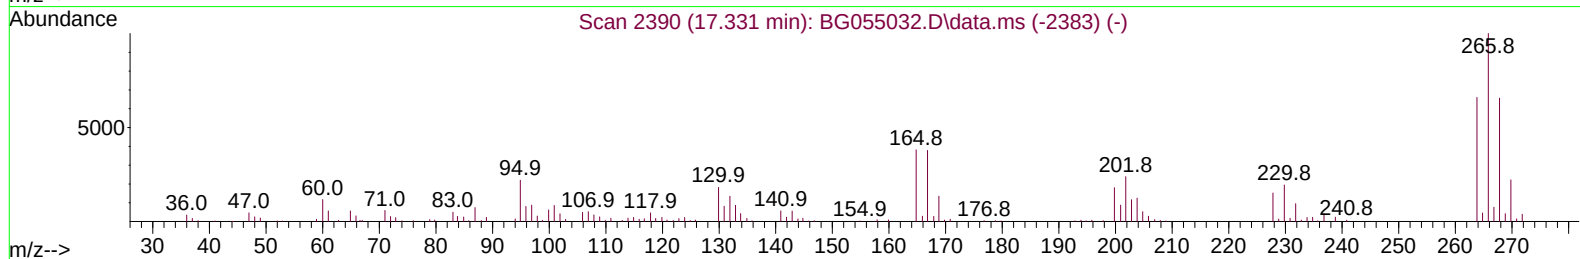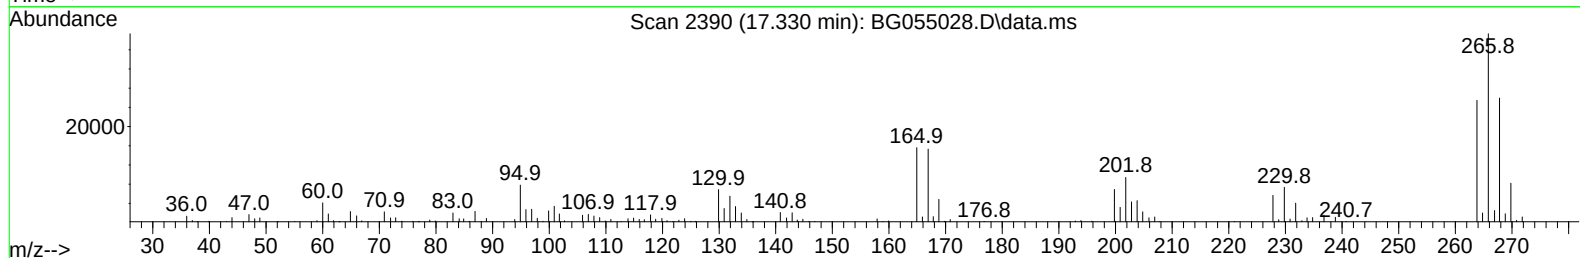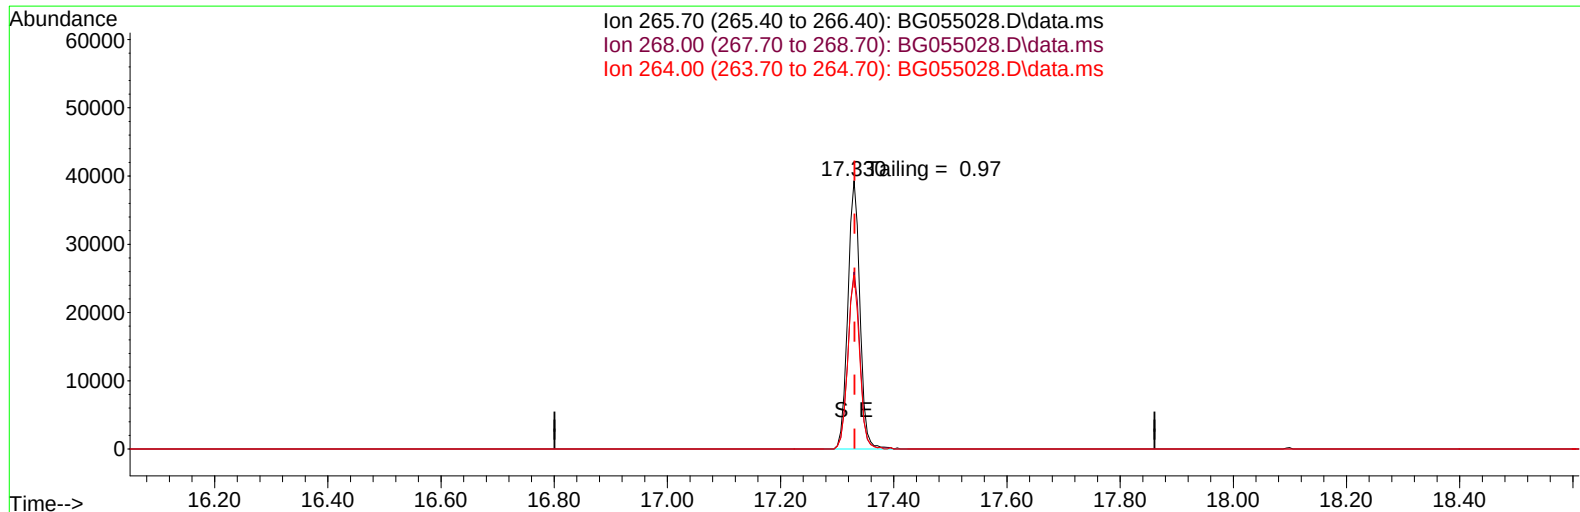

TIC: BG055028.D\data.ms

(70) Pentachlorophenol (C)

17.330min (-0.001) 27531.65 ng




response 58093

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	65.93
264.00	61.70	64.73
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092822\
Data File : BG055028.D
Acq On : 28 Sep 2022 9:51
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Sep 28 17:10:00 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG092822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 28 15:43:39 2022
Response via : Initial Calibration

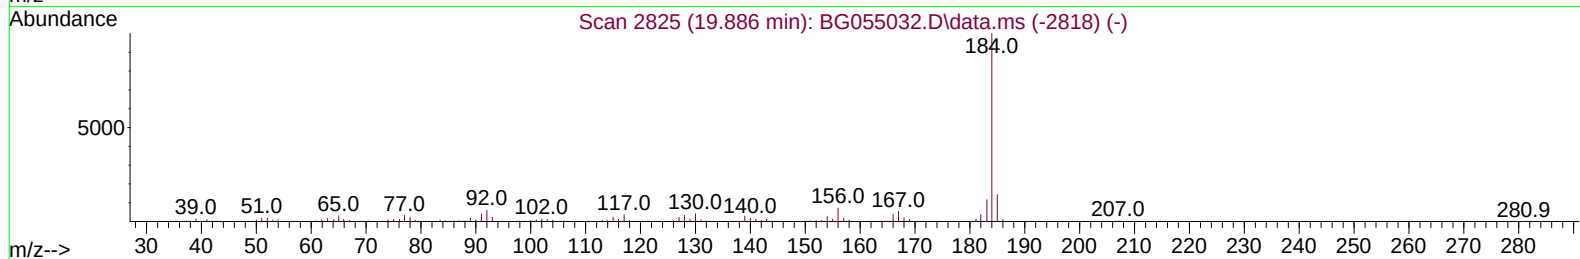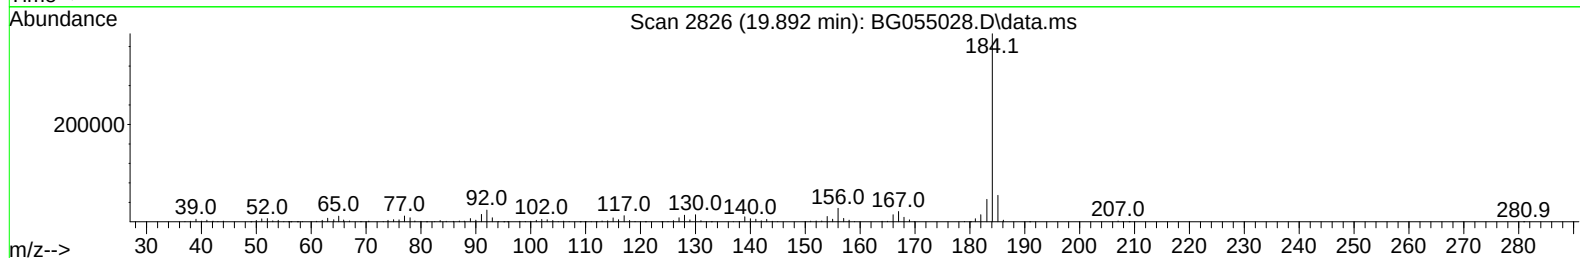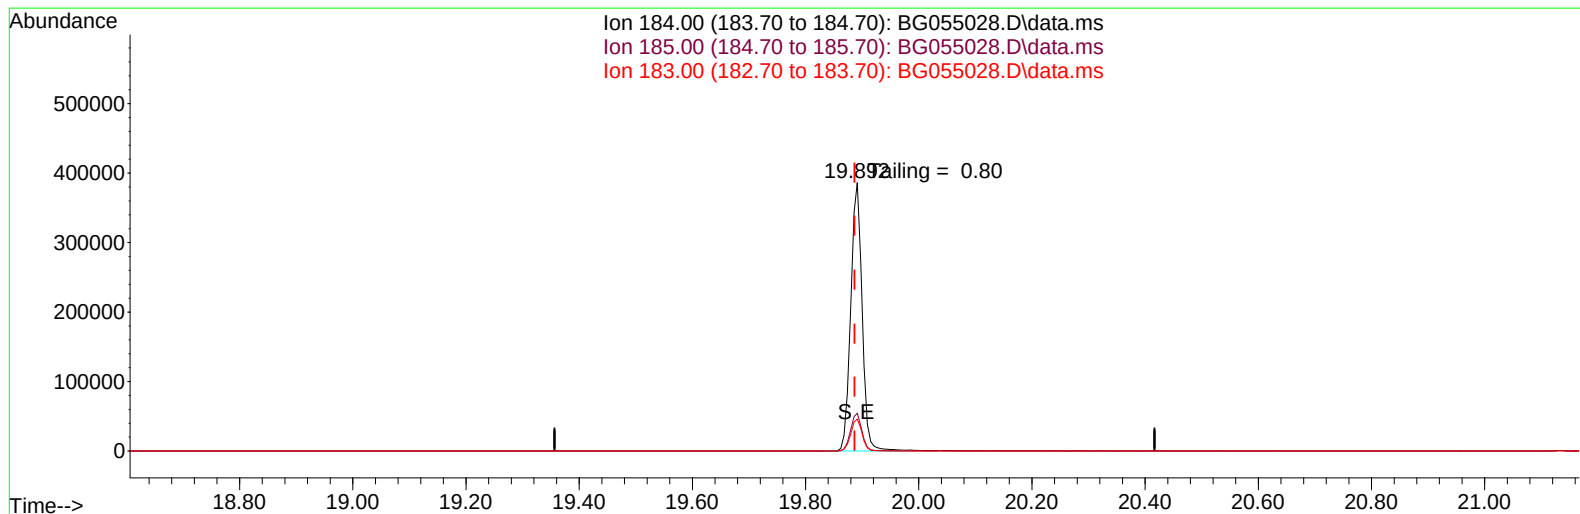

TIC: BG055028.D\data.ms

(77) Benzidine

19.892min (+ 0.005) 0.00 ng

response 538765

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.09
183.00	12.30	11.96
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/28/2022	BNA_G	BG055028.D
Compound Name	Response	Retention Time
DDT	173131	21.13
DDD	72	20.67
DDE	0	19.09
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
72	173203	0.04

Instrument :
BNA_G
ClientSampleId :
DFTPP