
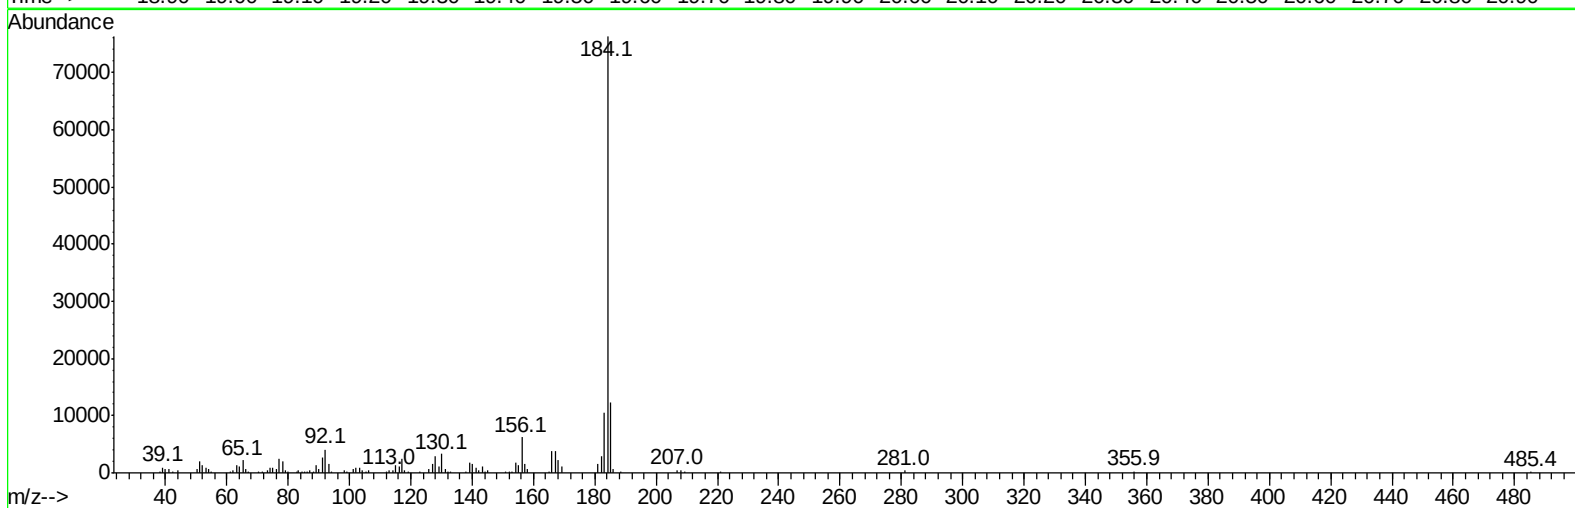


Data Path : Z:\HPCHEM1\BNA G\DATA\BG092917\
Data File : BG028967.D
Acq On : 29 Sep 2017 13:43
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 30 01:06:53 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG091217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 16:57:11 2017
Response via : Initial Calibration

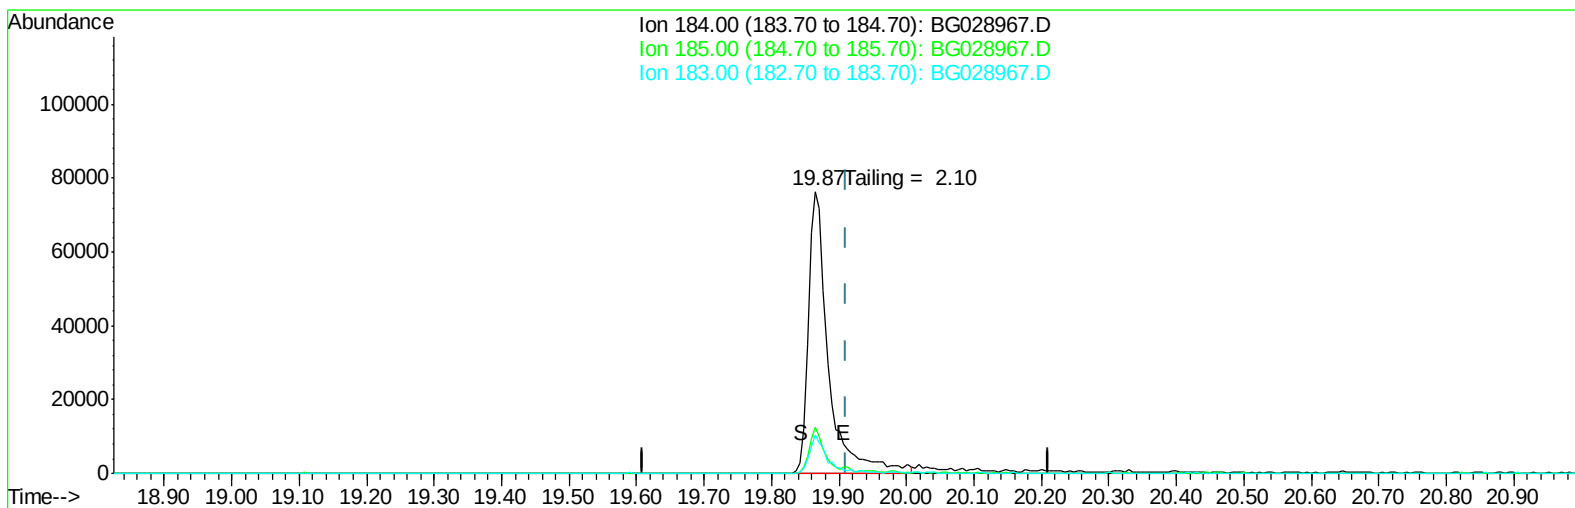

TIC: BG028967.D

(76) Benzidine



19.865min (-0.045) 102201.43ng

response 156369

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	16.27
183.00	13.80	13.85
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG092917\
Data File : BG028967.D
Acq On : 29 Sep 2017 13:43
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 30 01:06:53 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG091217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 16:57:11 2017
Response via : Initial Calibration

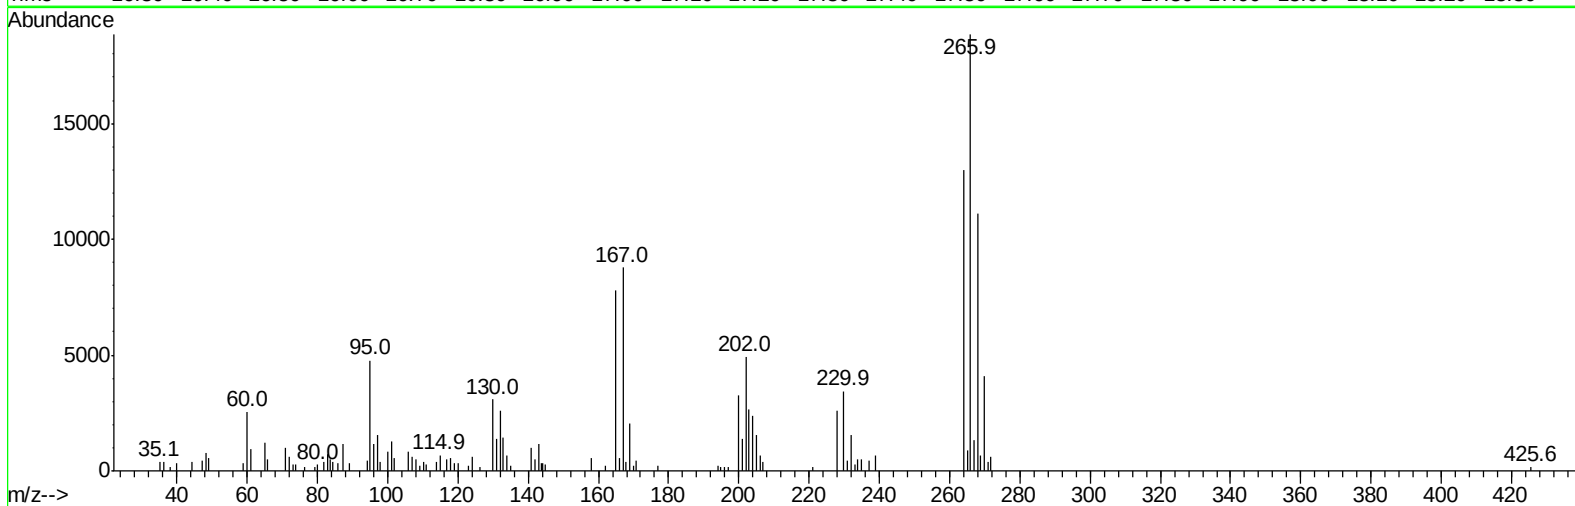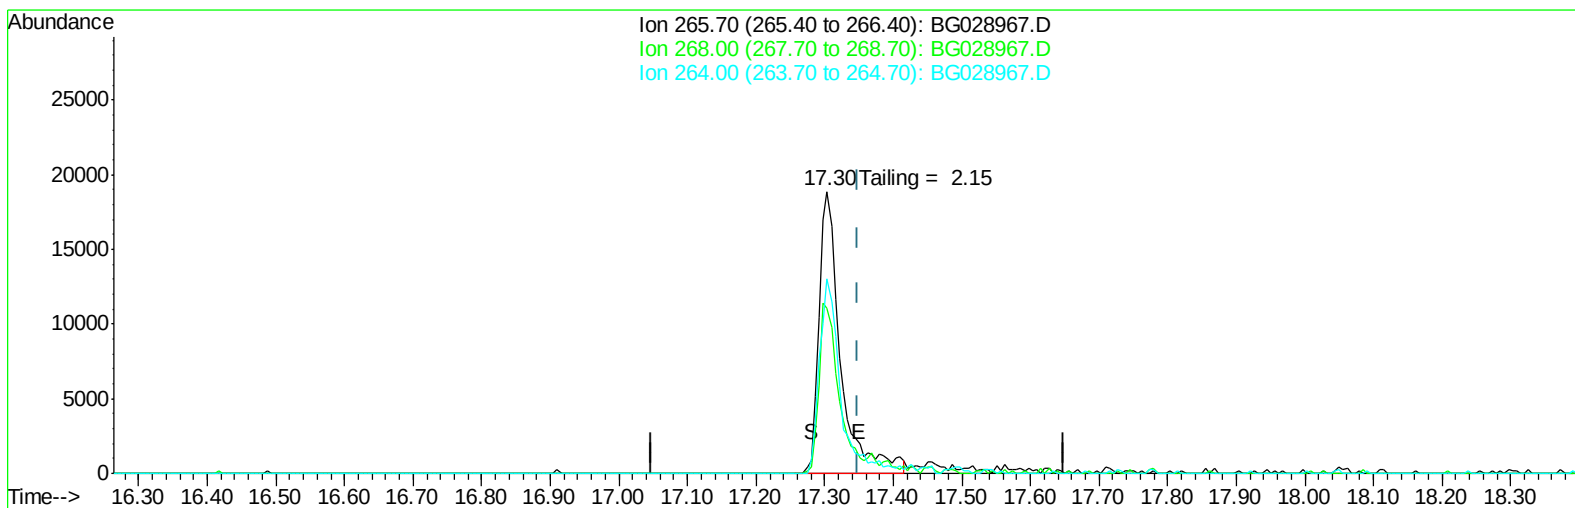

TIC: BG028967.D

(69) Pentachlorophenol (C)

17.304min (-0.045) 100288.84ng m

response 41143

Ion	Exp%	Act%
265.70	100	100
268.00	60.70	58.82
264.00	62.60	68.98
0.00	0.00	0.00