


Data Path : Z:\HPCHEM1\BNA G\Data\BG092917\
 Data File : BG028967.D
 Acq On : 29 Sep 2017 13:43
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG091217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 12 16:57:11 2017

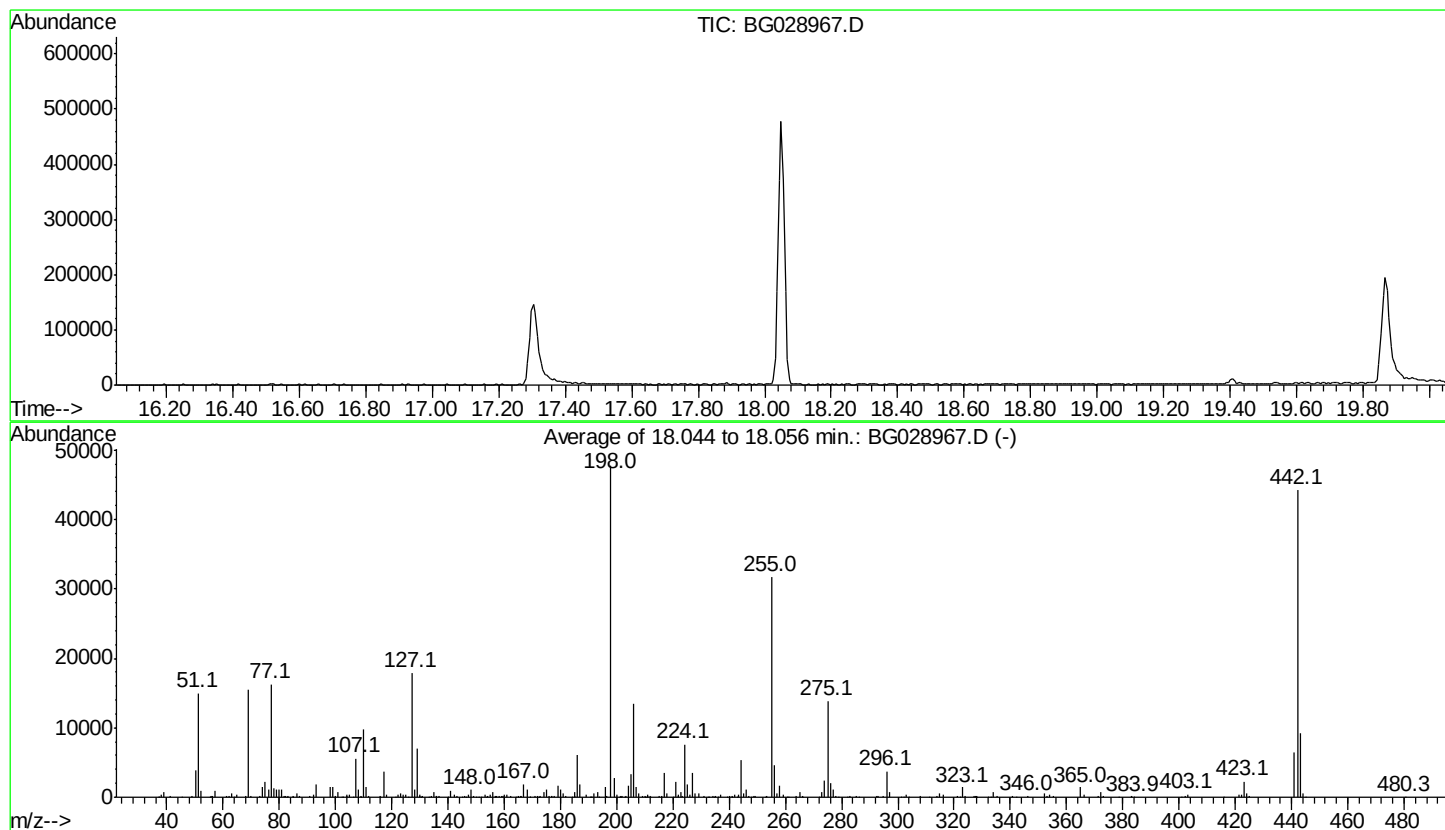

AutoFind: Scans 2460, 2461, 2462; Background Corrected with Scan 2454

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.4	14979	PASS
68	69	0.00	2	1.1	173	PASS
69	198	0.00	100	32.3	15436	PASS
70	69	0.00	2	0.7	115	PASS
127	198	10	80	37.6	17964	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	47744	PASS
199	198	5	9	5.9	2837	PASS
275	198	10	60	29.1	13889	PASS
365	198	1	100	3.0	1454	PASS
441	442	0.01	24	14.7	6516	PASS
442	198	50	100	92.8	44304	PASS
443	442	15	24	20.9	9250	PASS