
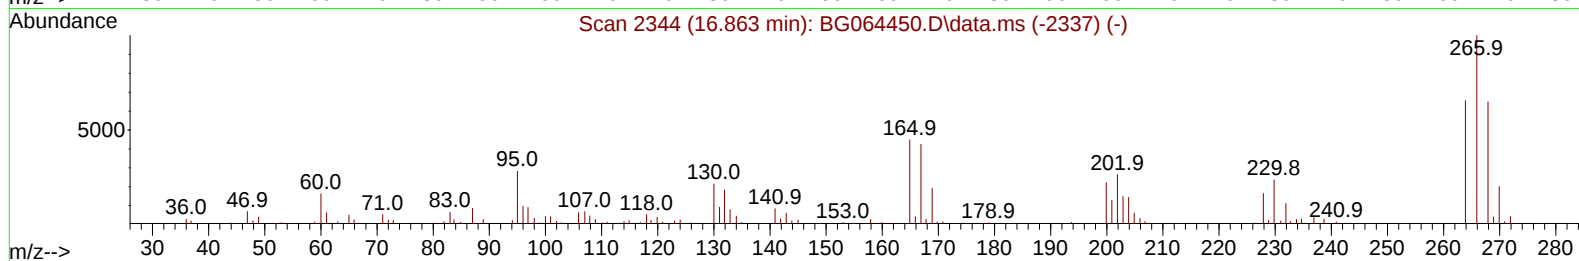
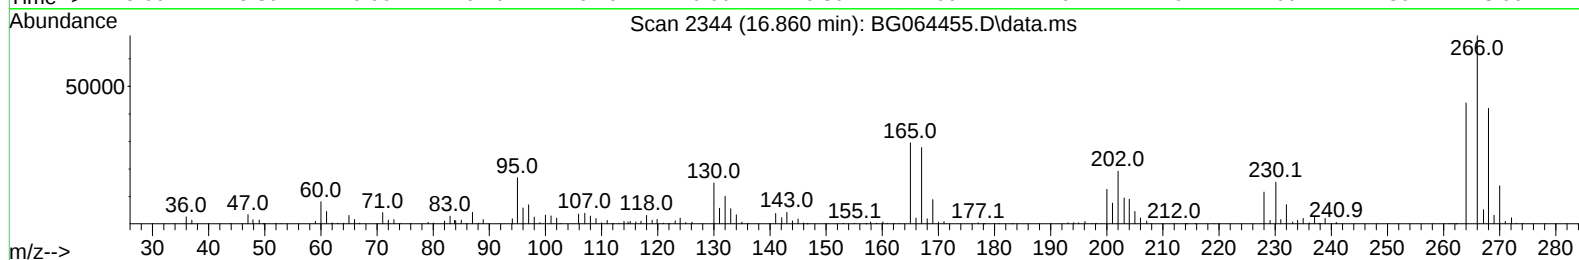


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092925\
Data File : BG064455.D
Acq On : 29 Sep 2025 11:41
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 29 19:15:20 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG092525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 29 18:04:12 2025
Response via : Initial Calibration

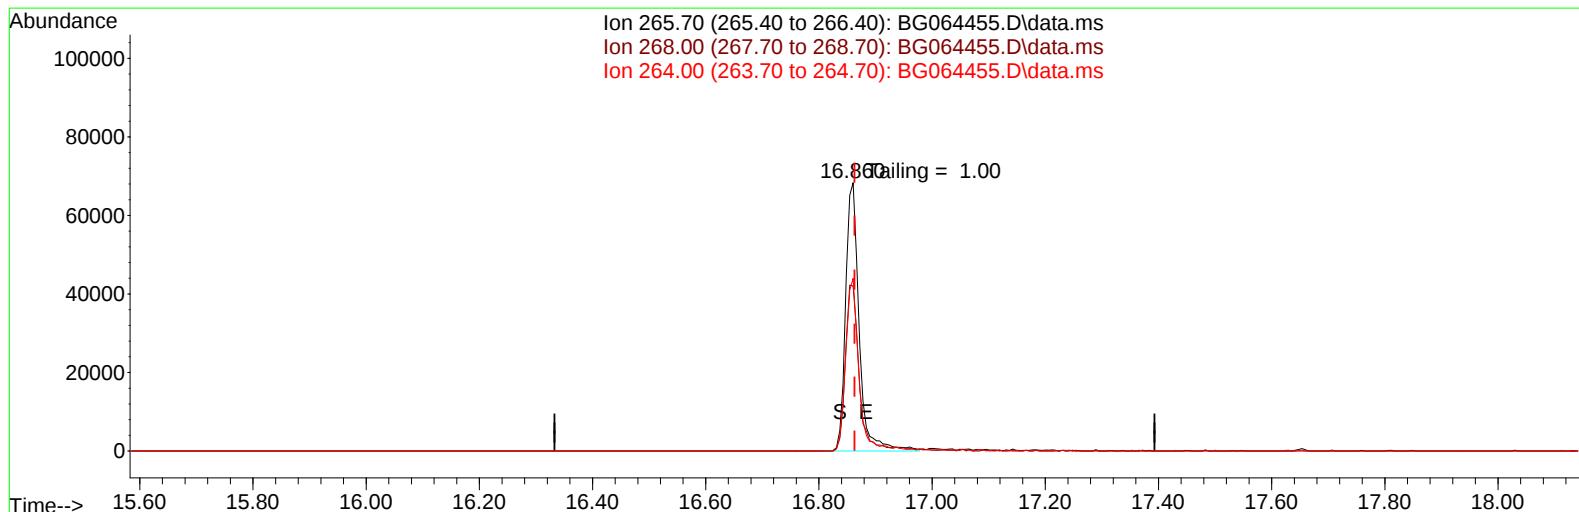

TIC: BG064455.D\data.ms

(70) Pentachlorophenol (C)




16.860min (-0.002) 151423.59 ng

response 113326

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	61.46
264.00	65.50	64.34
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092925\
Data File : BG064455.D
Acq On : 29 Sep 2025 11:41
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 29 19:15:20 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG092525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 29 18:04:12 2025
Response via : Initial Calibration

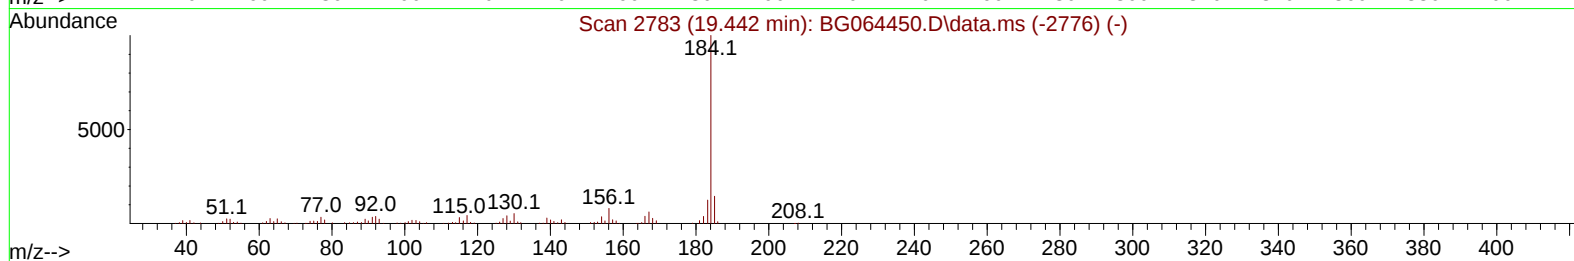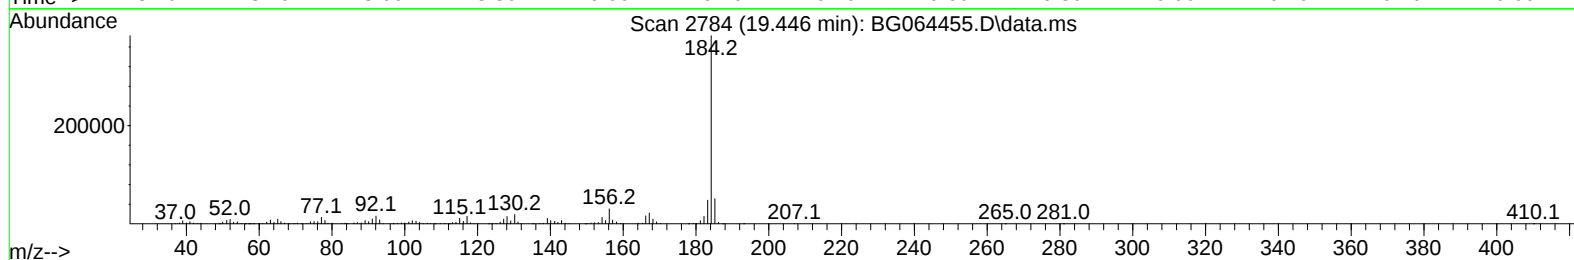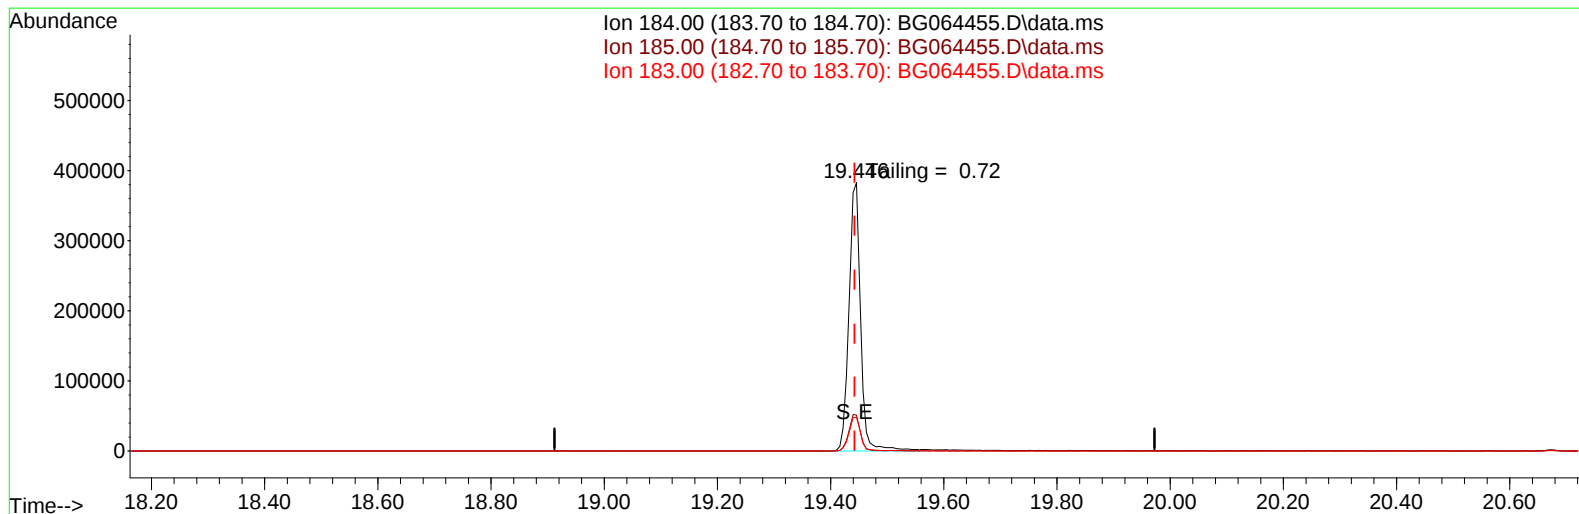

TIC: BG064455.D\data.ms

(77) Benzidine**19.446min (+ 0.003) 35719.25 ng****response 544294**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	13.37
183.00	12.50	12.56
0.00	0.00	0.00