
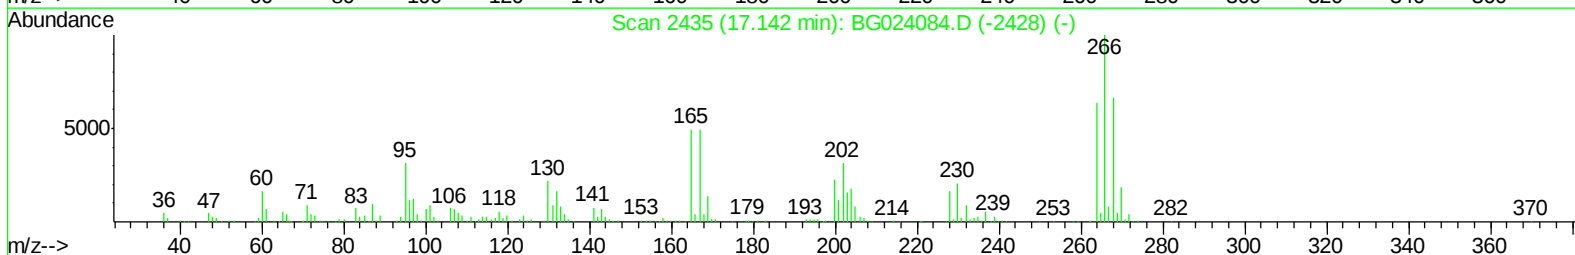
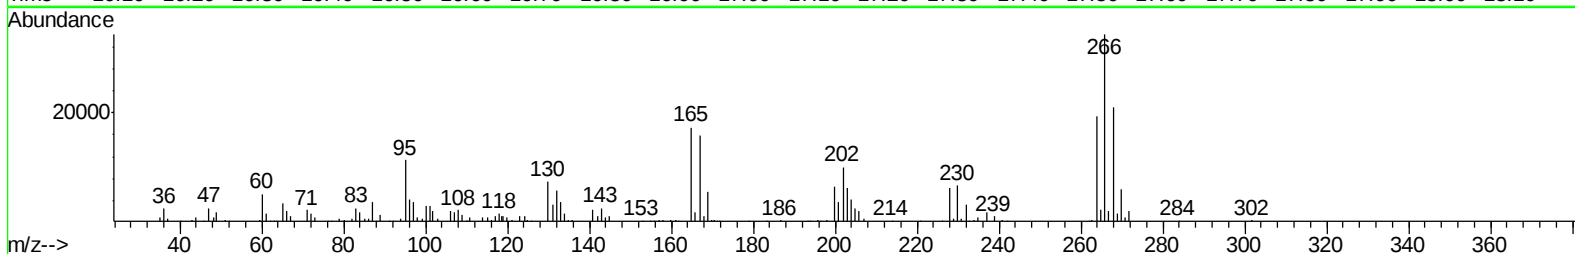


Data Path : Z:\HPCHEM1\BNA_G\Data\BG093016\
Data File : BG024157.D
Acq On : 30 Sep 2016 12:33
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 03 06:45:44 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG092316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 23 15:35:28 2016
Response via : Initial Calibration

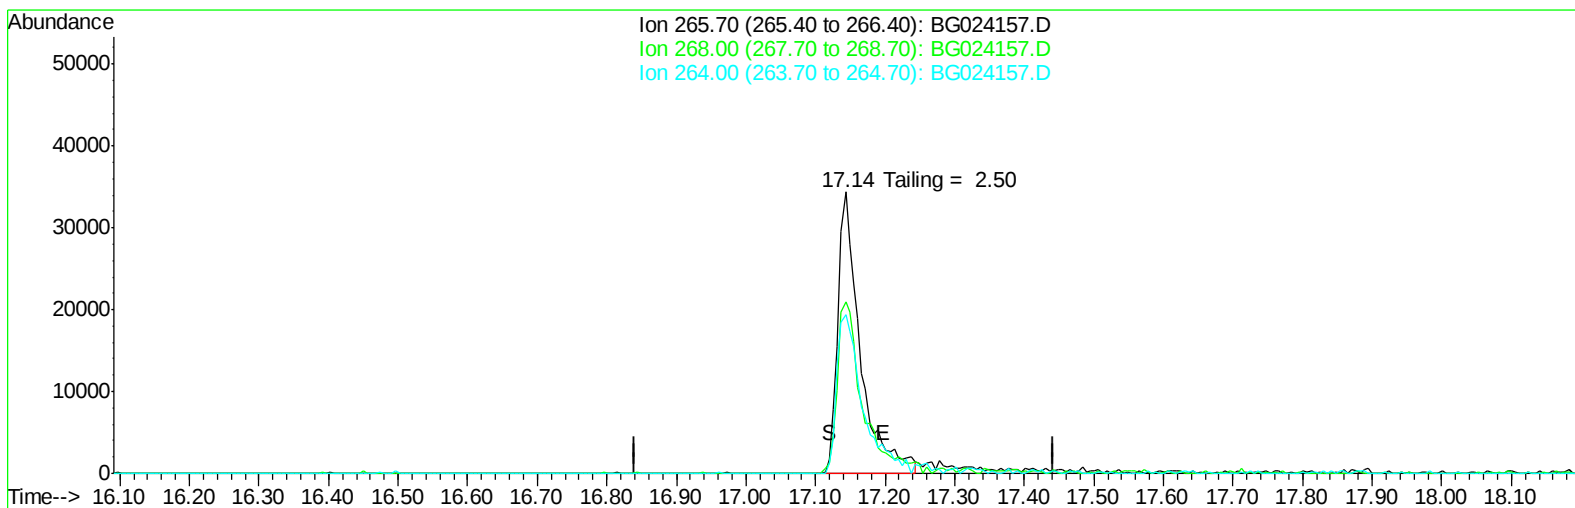

TIC: BG024157.D

(69) Pentachlorophenol (C)




17.142min (-17.142) 0.00ng

response 0

Ion	Exp%	Act%
265.70	100	0.00
268.00	64.90	0.00#
264.00	63.20	0.00#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\Data\BG093016\
Data File : BG024157.D
Acq On : 30 Sep 2016 12:33
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 03 06:45:44 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG092316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 23 15:35:28 2016
Response via : Initial Calibration

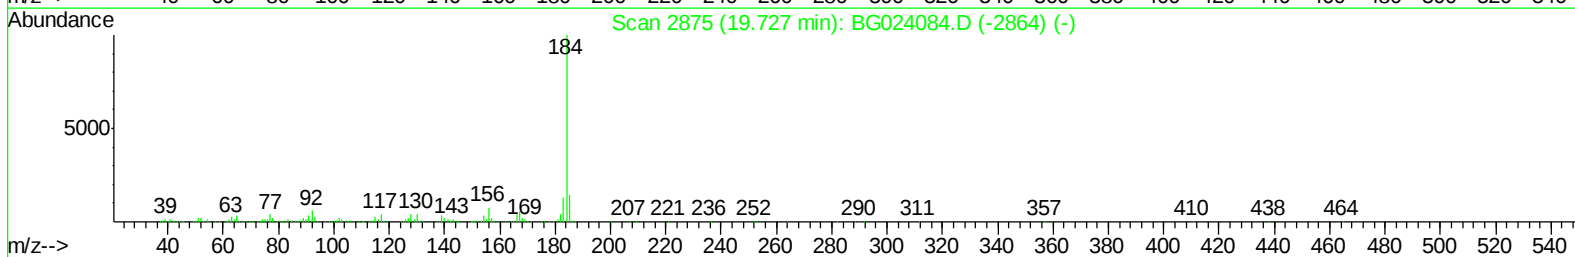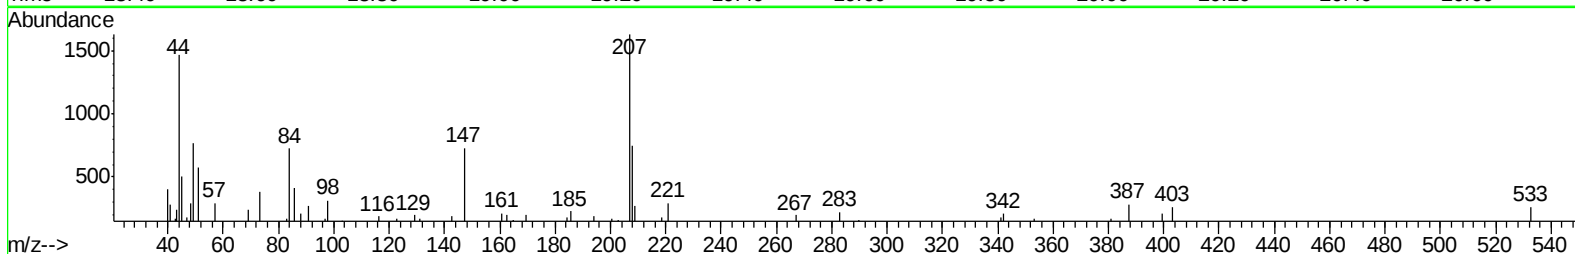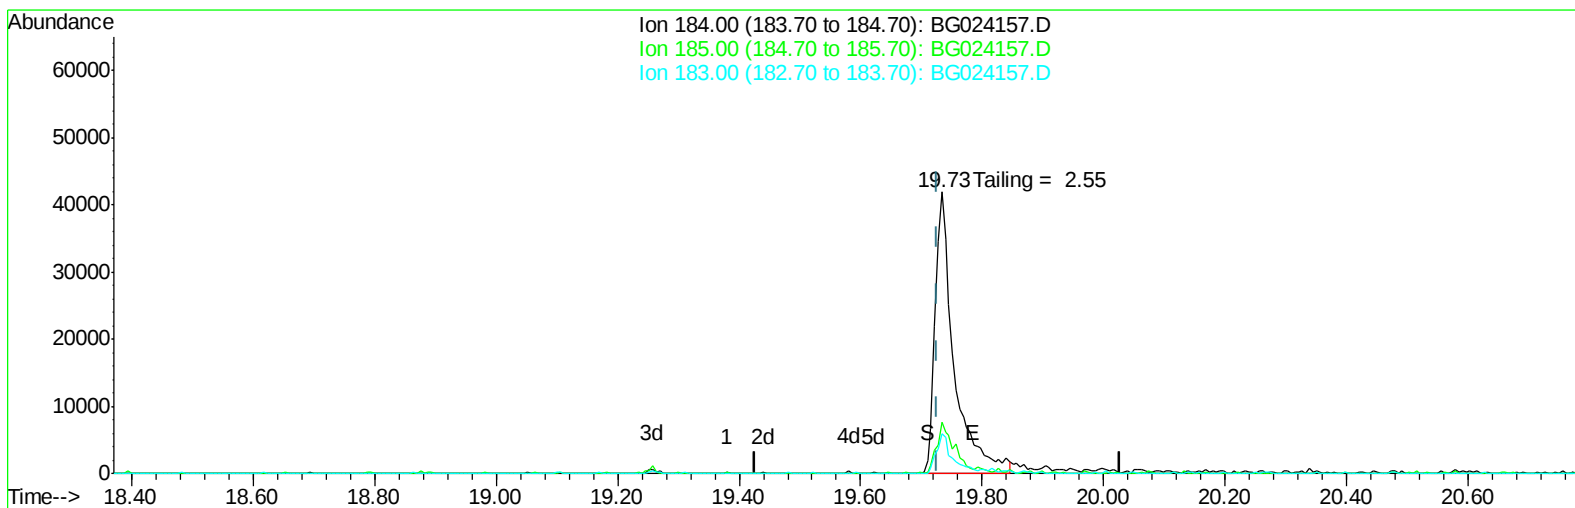

TIC: BG024157.D

(76) Benzidine

19.381min (-0.346) 41.87ng

response 64

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	126.52#
183.00	13.40	0.00#
0.00	0.00	0.00