
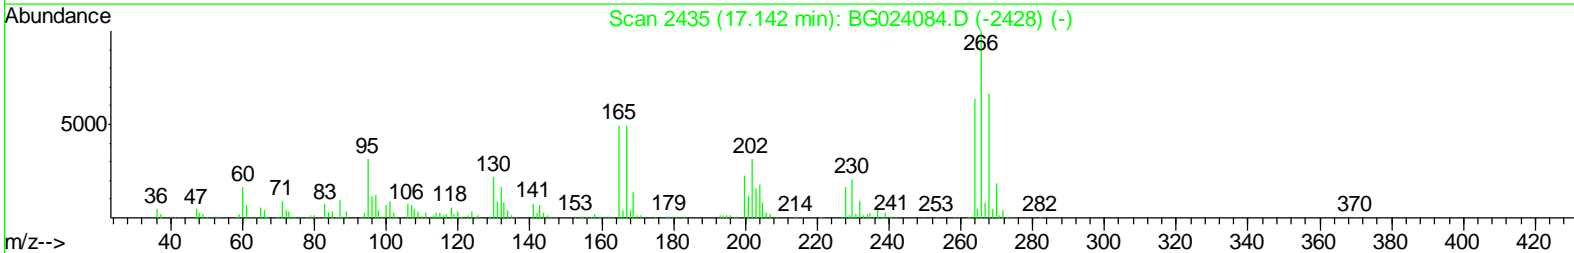
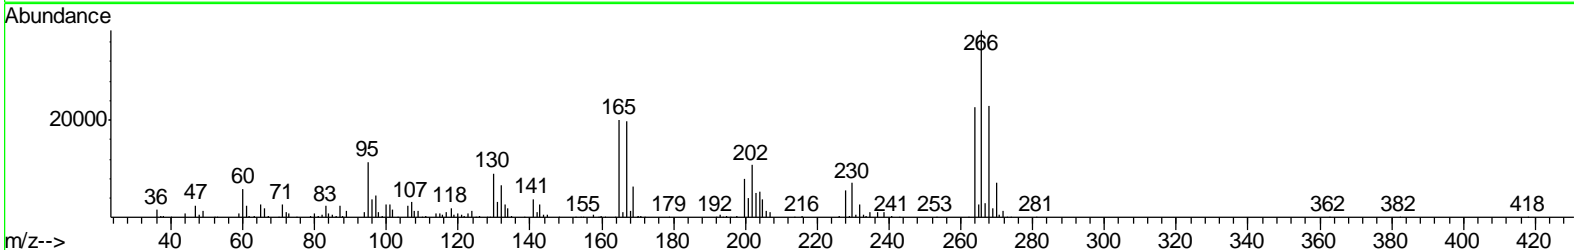


Data Path : Z:\HPCHEM1\BNA\_G\Data\BG093016\  
 Data File : BG024176.D  
 Acq On : 1 Oct 2016 1:45  
 Operator : UM/SJ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 03 06:48:48 2016  
 Quant Method : Z:\HPCHEM1\BNA\_G\METHODS\8270-BG092316.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri Sep 23 15:35:28 2016  
 Response via : Initial Calibration

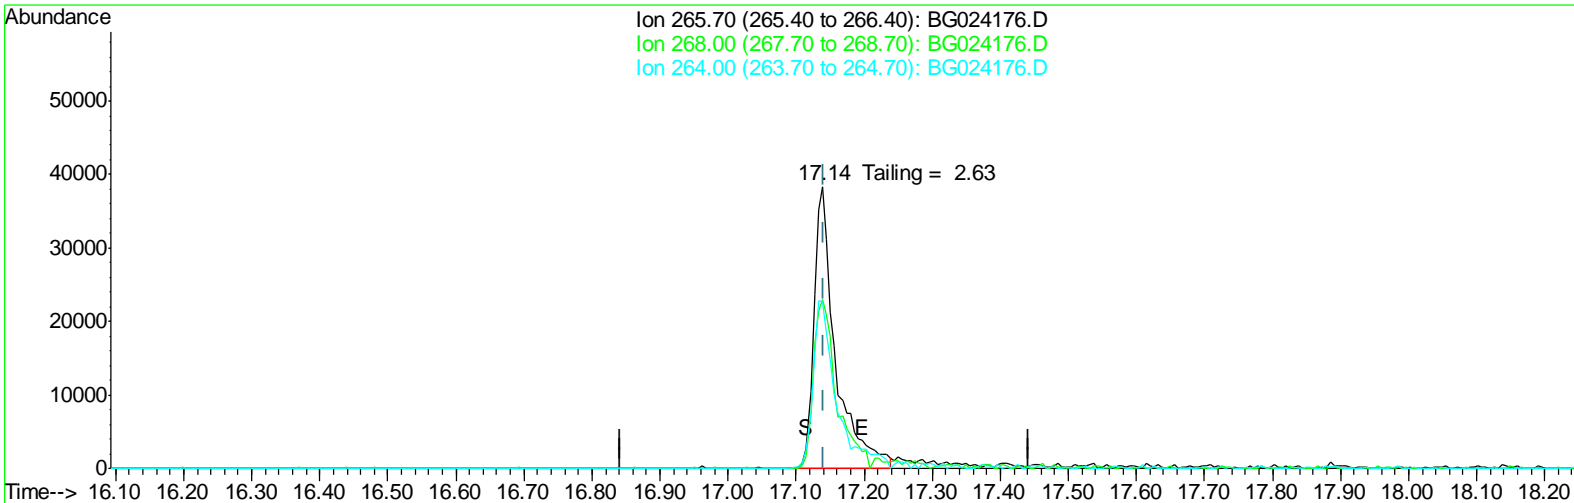




TIC: BG024176.D

(69) Pentachlorophenol (C)  
 17.139min (-0.003) 117561.46ng  
 response 85843

Ion	Exp%	Act%
265.70	100	100
268.00	64.90	60.07
264.00	63.20	58.88
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA\_G\Data\BG093016\  
 Data File : BG024176.D  
 Acq On : 1 Oct 2016 1:45  
 Operator : UM/SJ  
 Sample : DF7TPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 03 06:48:48 2016  
 Quant Method : Z:\HPCHEM1\BNA\_G\METHODS\8270-BG092316.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri Sep 23 15:35:28 2016  
 Response via : Initial Calibration

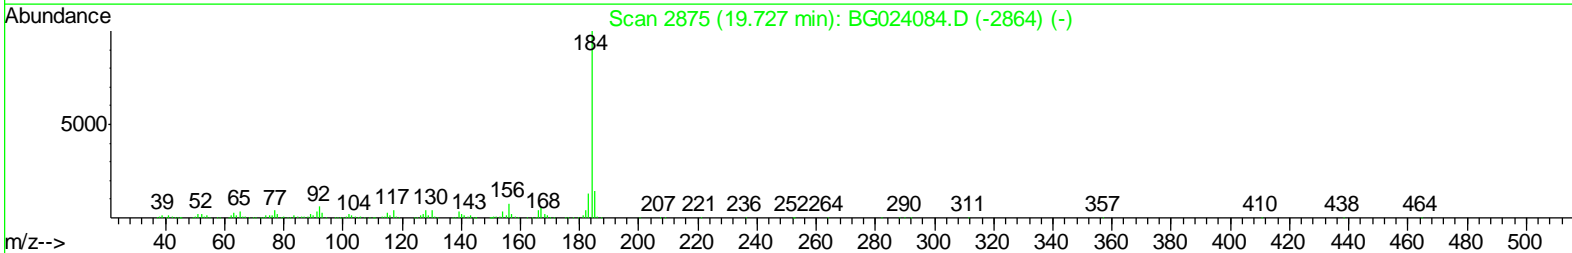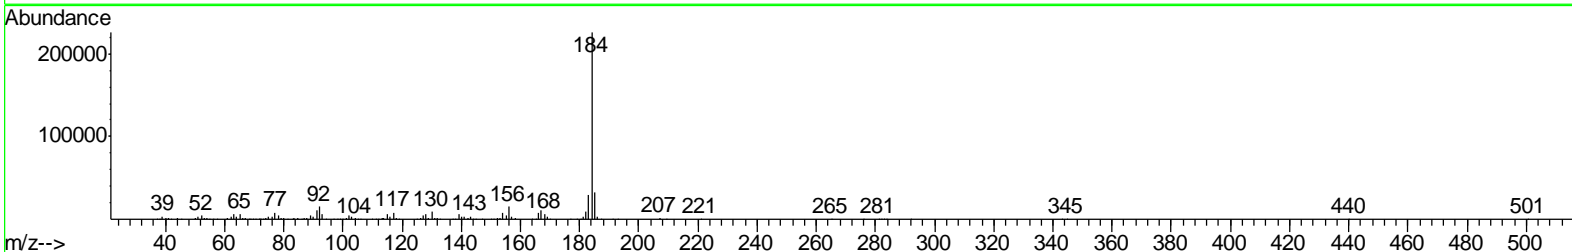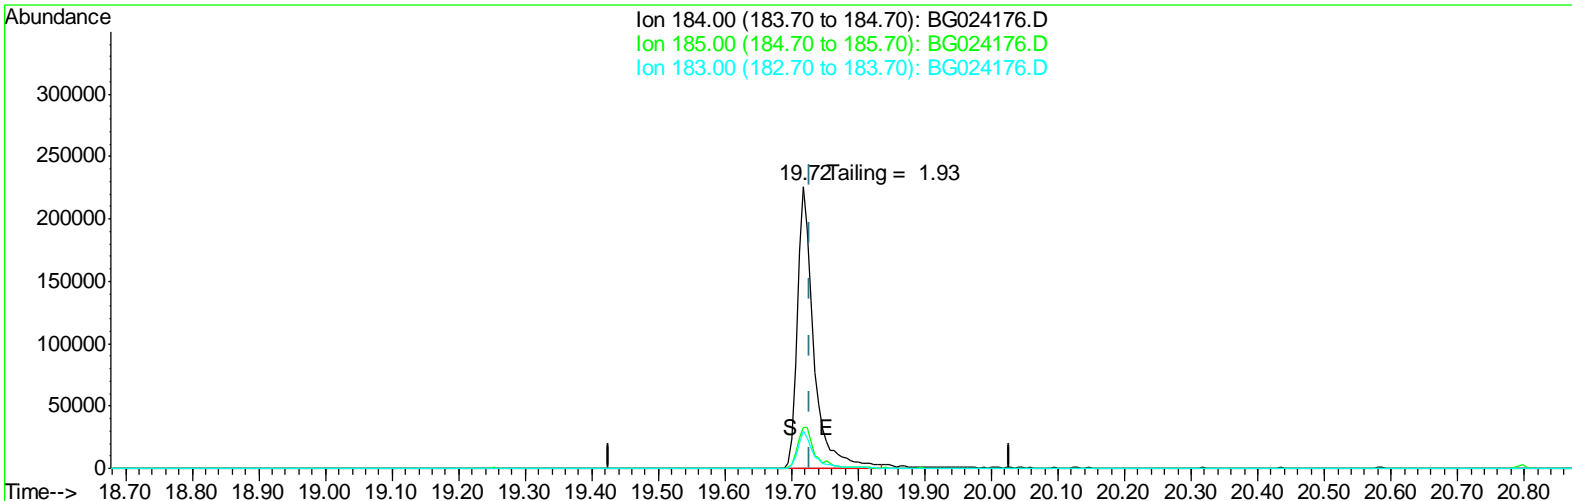

TIC: BG024176.D

(76) Benzidine

19.717min (-0.010) 48278.53ng

response 397697

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	14.57
183.00	13.40	12.98
0.00	0.00	0.00