

Data Path : Z:\HPCHEM1\BNA G\DATA\BG093016\
 Data File : BG024165.D
 Acq On : 30 Sep 2016 18:44
 Operator : UM/SJ
 Sample : H4998-14
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SUP-B046-12-13

Quant Time: Oct 01 01:09:32 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG092316.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 23 15:35:28 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.03	152	46525	20.00	ng	0.00
21) Naphthalene-d8	10.87	136	203043	20.00	ng	0.00
38) Acenaphthene-d10	14.71	164	165199	20.00	ng	0.00
63) Phenanthrene-d10	17.47	188	419923	20.00	ng	0.00
75) Chrysene-d12	21.78	240	477589	20.00	ng	-0.01
86) Perylene-d12	25.10	264	462619	20.00	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.58	112	337575	125.70	ng	0.00
7) Phenol-d6	7.20	99	518274	114.70	ng	0.00
23) Nitrobenzene-d5	9.21	82	381232	74.00	ng	0.00
41) 2,4,6-Tribromophenol	16.21	330	247880	104.39	ng	-0.01
44) 2-Fluorobiphenyl	13.32	172	734174	74.70	ng	-0.01
78) Terphenyl-d14	20.08	244	1361453	58.37	ng	-0.01
Target Compounds						Qvalue
49) Dimethylphthalate	14.16	163	402847	31.79	ng	# 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG093016\
Data File : BG024165.D
Acq On : 30 Sep 2016 18:44
Operator : UM/SJ
Sample : H4998-14
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SUP-B046-12-13

Quant Time: Oct 01 01:09:32 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG092316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 23 15:35:28 2016
Response via : Initial Calibration

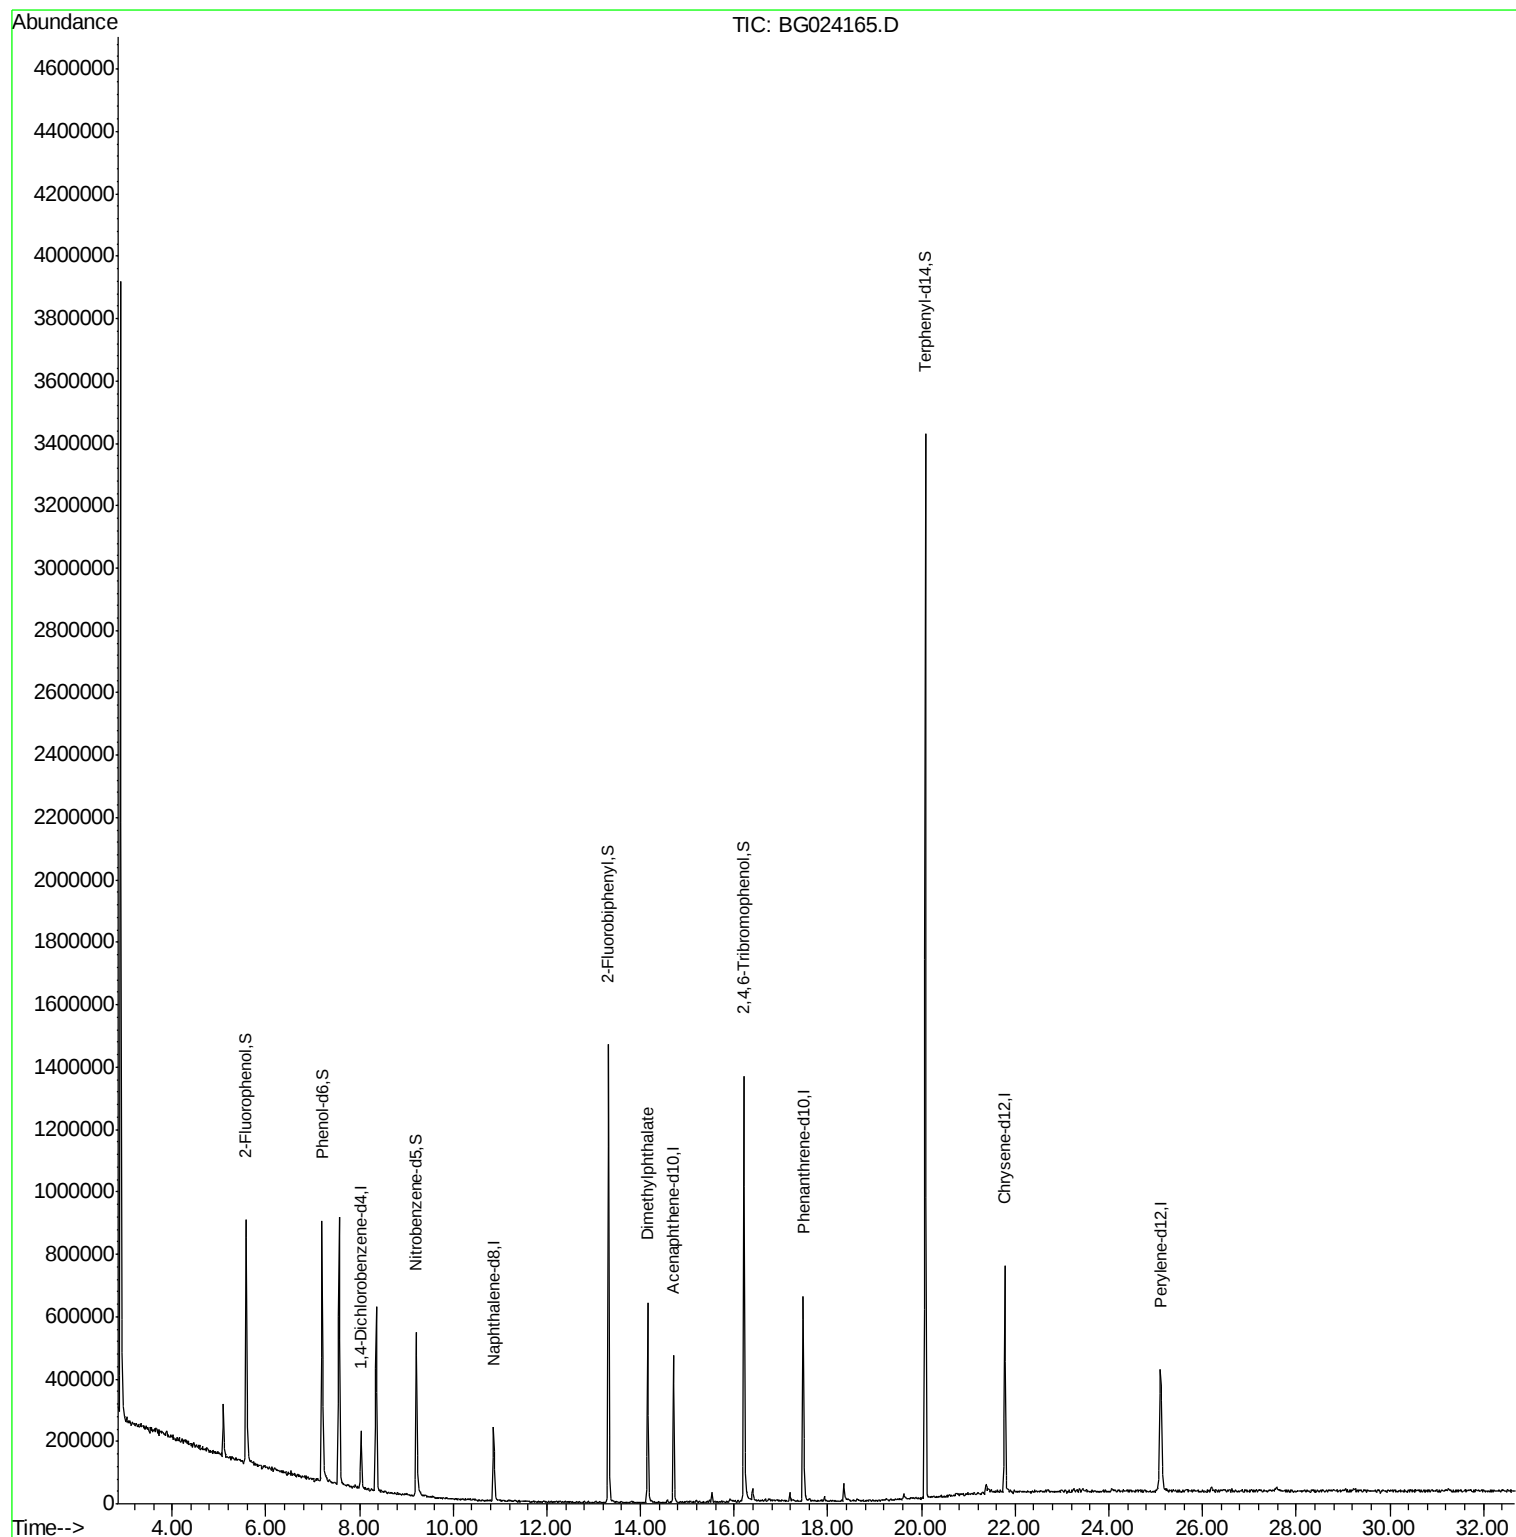







#1

1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 8.03 min Scan# 884
Delta R.T. -0.00 min
Lab File: BG024165.D
Acq: 30 Sep 2016 18:44

Instrument :
BNA_G
ClientSampleId :
SUP-B046-12-13




Tot Ion	Ratio	Lower	Upper
152	100		
150	144.9	144.7	217.1
115	67.0	64.0	96.0

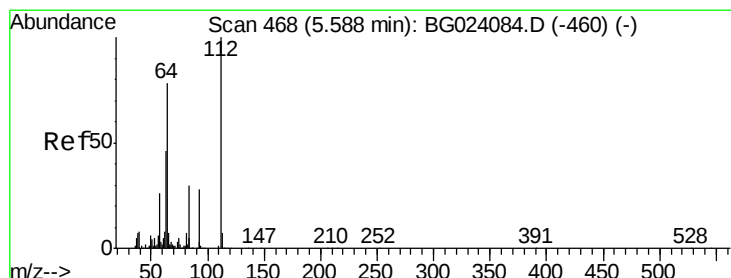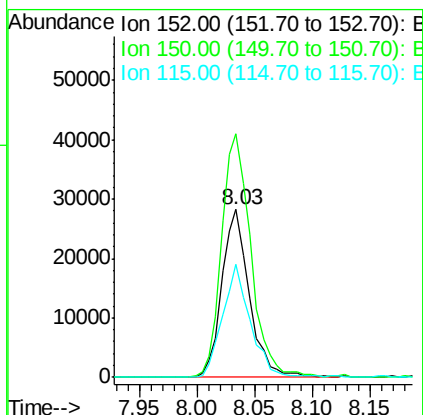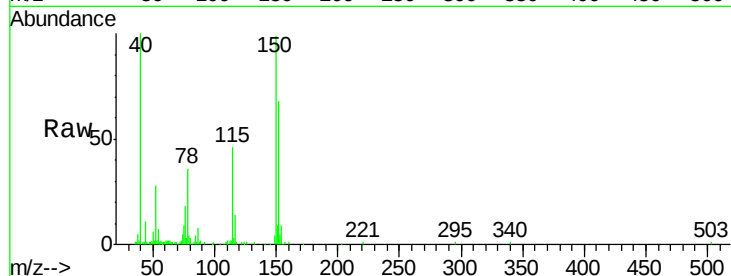


#5

2-Fluorophenol
Concen: 125.70 ng
RT: 5.58 min Scan# 466
Delta R.T. -0.01 min
Lab File: BG024165.D
Acq: 30 Sep 2016 18:44

Tgt Ion	Ratio	Lower	Upper
112	100		
64	76.2	59.0	88.4
63	42.5	37.8	56.8

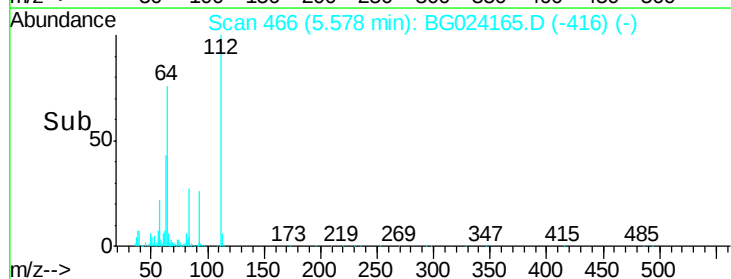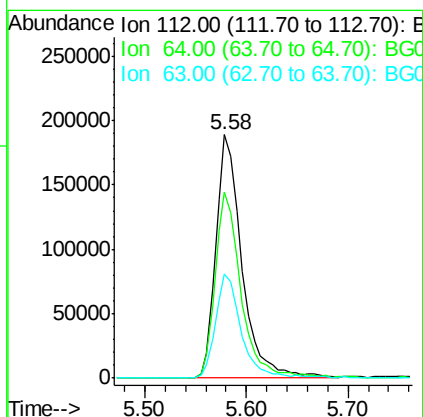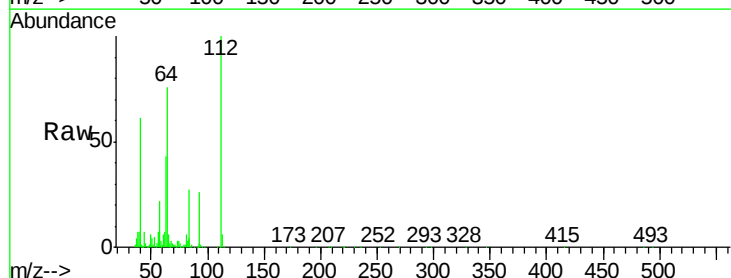

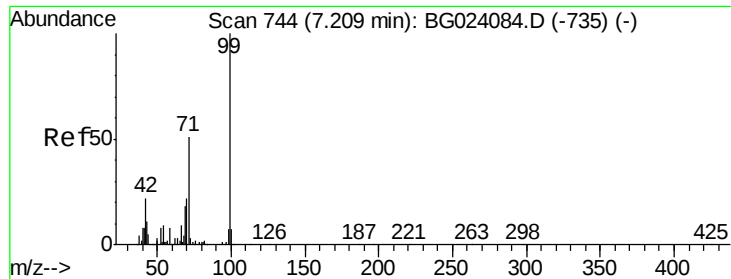

#7

Phenol-d6

Concen: 114.70 ng

RT: 7.20 min Scan# 742

Delta R.T. -0.01 min

Lab File: BG024165.D

Acq: 30 Sep 2016 18:44

Instrument :

BNA_G

ClientSampleId :

SUP-B046-12-13


Tot Ion: 99 Resp: 518274

Ion Ratio Lower Upper




99 100

42 21.1 17.8 26.6

71 45.6 41.5 62.3

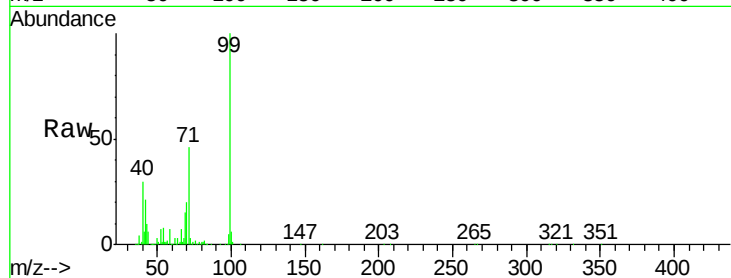

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

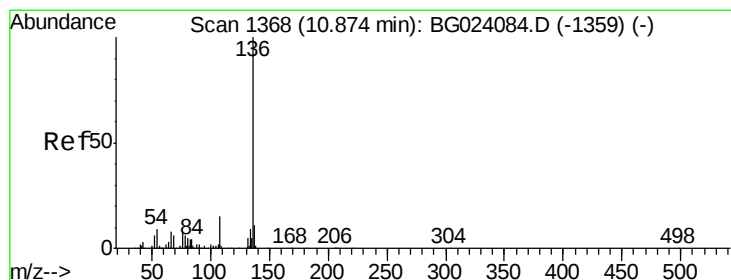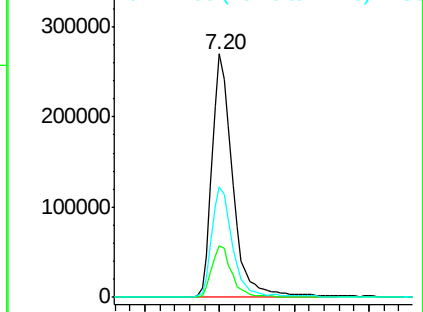

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.87 min Scan# 1366

Delta R.T. -0.01 min

Lab File: BG024165.D

Acq: 30 Sep 2016 18:44

Tgt Ion: 136 Resp: 203043


Ion Ratio Lower Upper

136 100



137 12.5 9.6 14.4


54 8.1 7.3 10.9

68 7.6 5.3 7.9

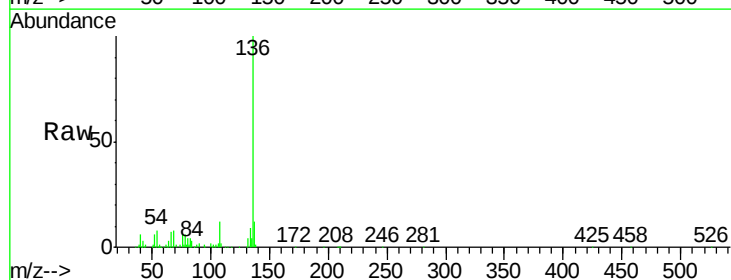

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC




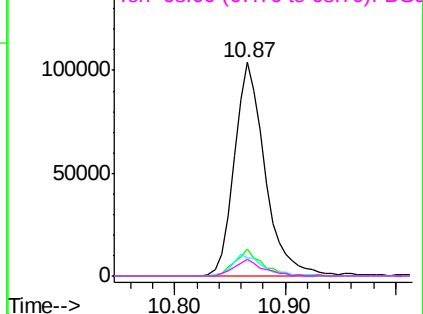


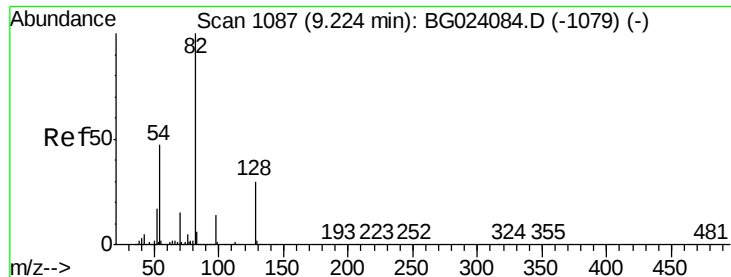

#23
 Nitrobenzene-d5
 Concen: 74.00 ng
 RT: 9.21 min Scan# 1085
 Delta R.T. -0.01 min
 Lab File: BG024165.D
 Acq: 30 Sep 2016 18:44




Instrument :
 BNA_G
 ClientSampleId :
 SUP-B046-12-13


Tot Ion	Ratio	Lower	Upper
82	100		
128	33.0	24.4	36.6
54	51.1	41.4	62.0

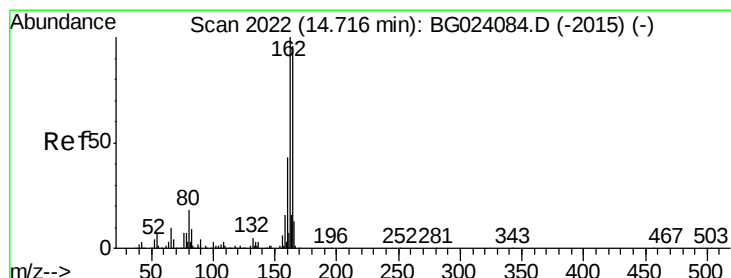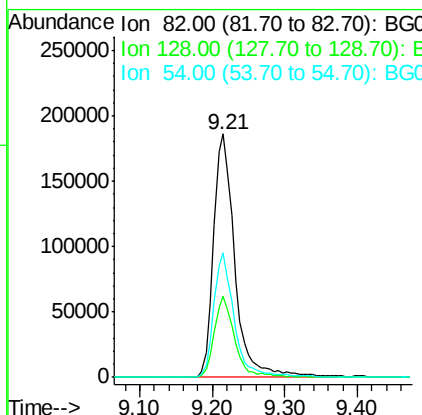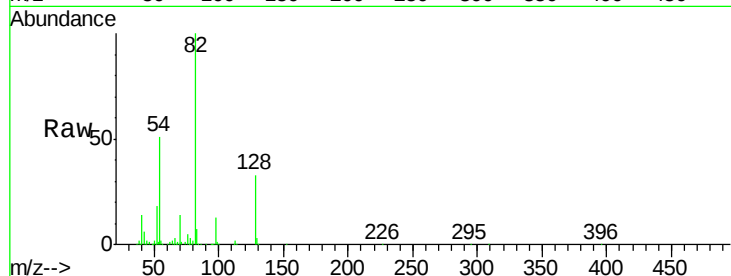

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 14.71 min Scan# 2020
 Delta R.T. -0.01 min
 Lab File: BG024165.D
 Acq: 30 Sep 2016 18:44

Tgt Ion	Ratio	Lower	Upper
164	100		
162	99.3	87.7	131.5
160	47.0	37.2	55.8

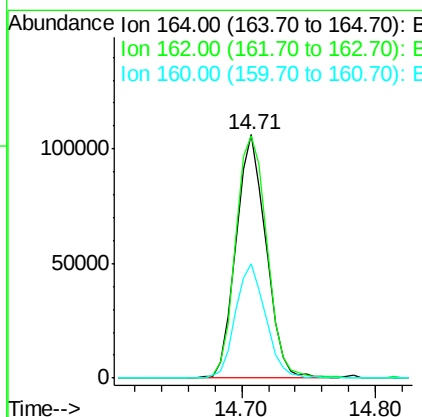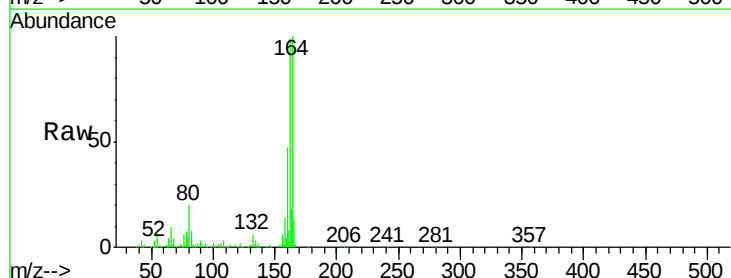


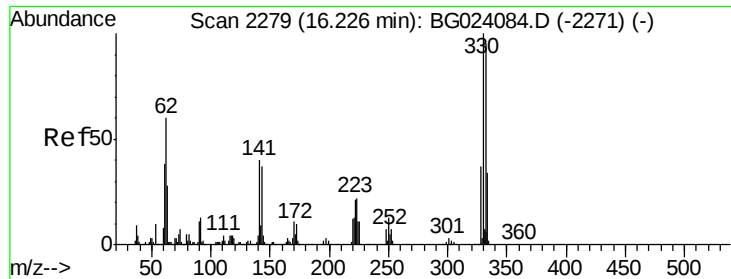




#41
 2,4,6-Tribromophenol
 Concen: 104.39 ng
 RT: 16.21 min Scan# 2276
 Delta R.T. -0.01 min
 Lab File: BG024165.D
 Acq: 30 Sep 2016 18:44

Instrument :
 BNA_G
 ClientSampleId :
 SUP-B046-12-13

Tot Ion:330 Resp: 247880
 Ion Ratio Lower Upper
 330 100
 332 94.5 77.4 116.2
 141 44.1 31.7 47.5

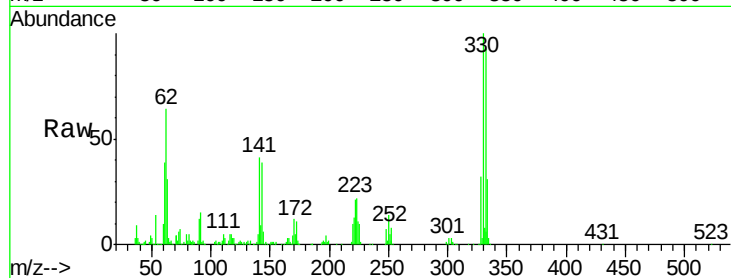


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

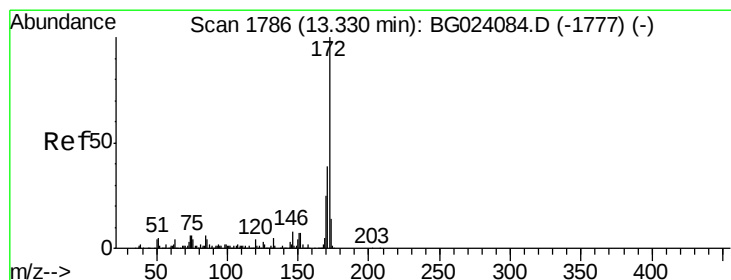
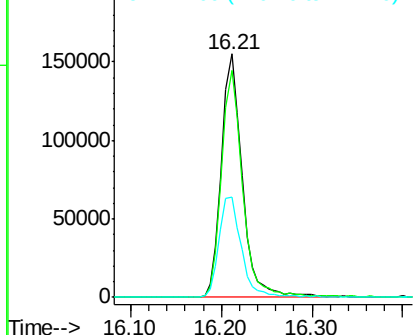



#44
 2-Fluorobiphenyl
 Concen: 74.70 ng
 RT: 13.32 min Scan# 1783
 Delta R.T. -0.01 min
 Lab File: BG024165.D
 Acq: 30 Sep 2016 18:44

Tgt Ion:172 Resp: 734174
 Ion Ratio Lower Upper
 172 100
 171 36.9 31.6 47.4
 170 24.0 21.3 31.9

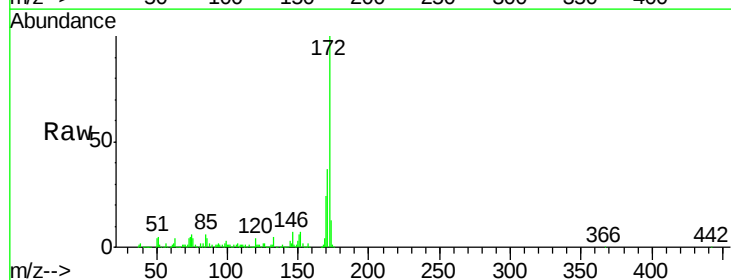

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



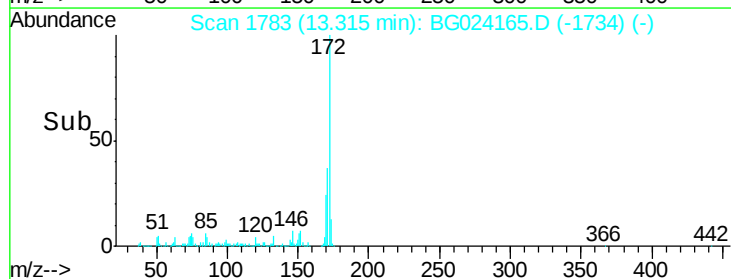
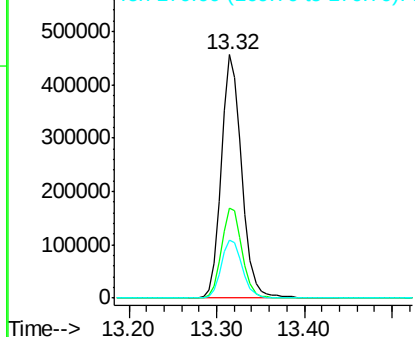


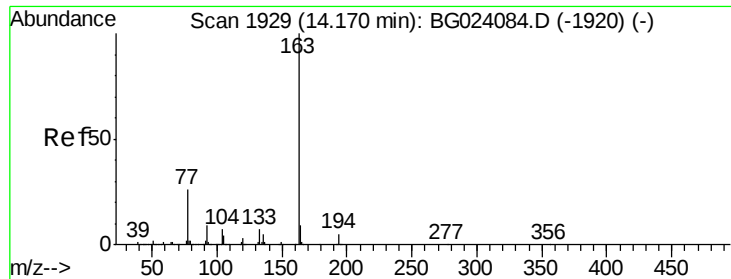

#49
Dimethylphthalate
Concen: 31.79 ng
RT: 14.16 min Scan# 1926
Delta R.T. -0.01 min
Lab File: BG024165.D
Acq: 30 Sep 2016 18:44




Instrument :
BNA_G
ClientSampleId :
SUP-B046-12-13


Tot Ion	Ratio	Lower	Upper
163	100		
194	3.4	3.6	5.4#
164	10.8	8.1	12.1

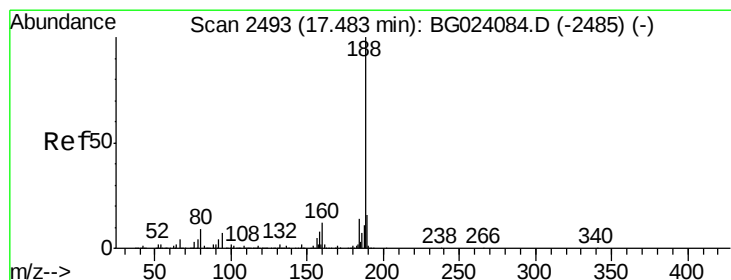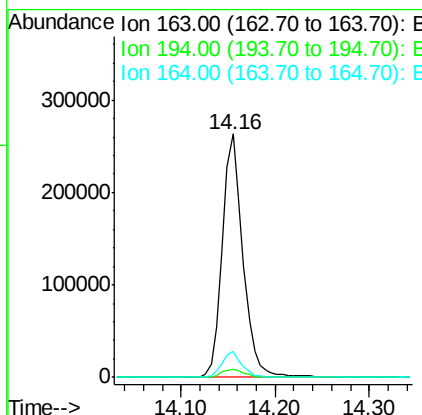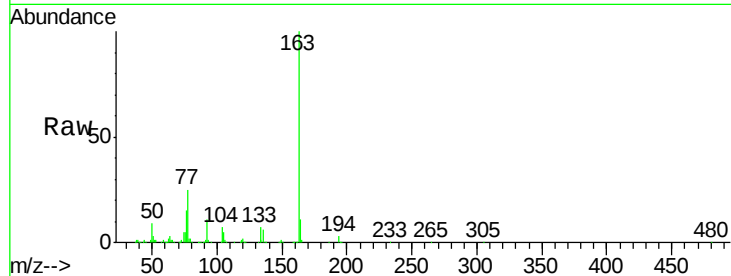

#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.47 min Scan# 2491
Delta R.T. -0.01 min
Lab File: BG024165.D
Acq: 30 Sep 2016 18:44

Tgt Ion	Ratio	Lower	Upper
188	100		
94	7.9	5.2	7.8#
80	8.9	7.2	10.8



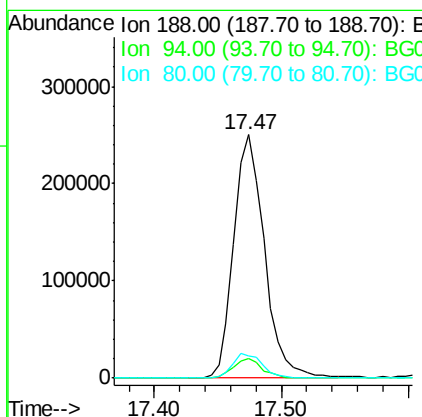
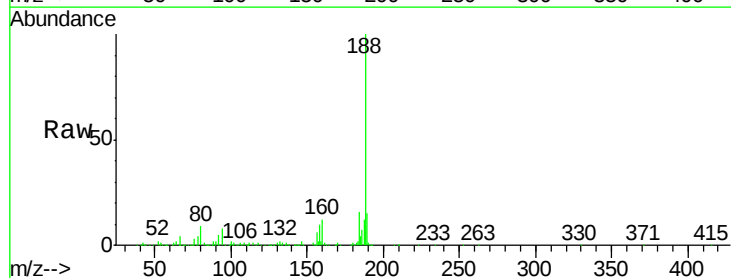


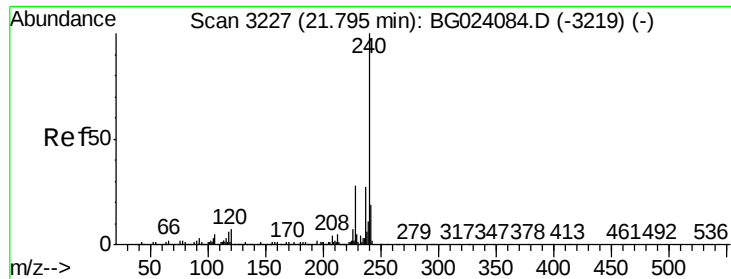

#75
Chrysene-d12
Concen: 20.00 ng
RT: 21.78 min Scan# 3224
Delta R.T. -0.01 min
Lab File: BG024165.D
Acq: 30 Sep 2016 18:44




Instrument :
BNA_G
ClientSampleId :
SUP-B046-12-13


Tot Ion:240 Resp: 477589
Ion Ratio Lower Upper
240 100
120 6.5 4.1 6.1#
236 26.8 21.1 31.7

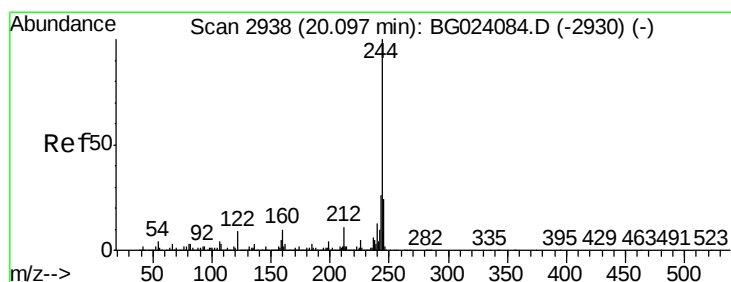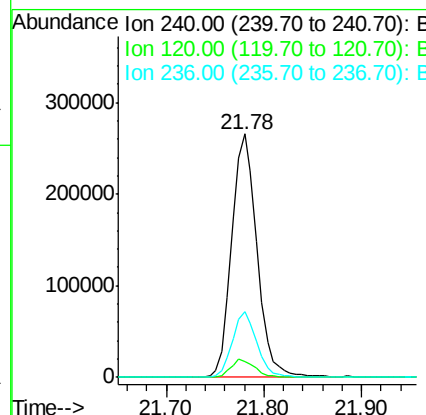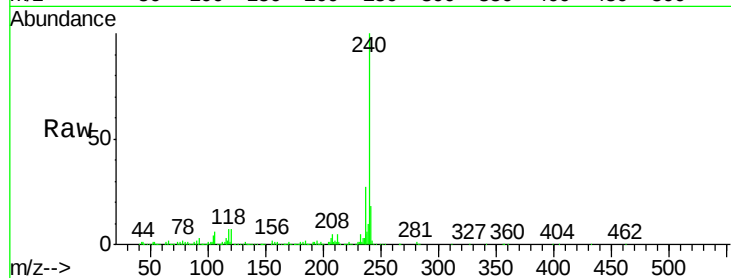

#78
Terphenyl-d14
Concen: 58.37 ng
RT: 20.08 min Scan# 2935
Delta R.T. -0.01 min
Lab File: BG024165.D
Acq: 30 Sep 2016 18:44

Tgt Ion:244 Resp: 1361453
Ion Ratio Lower Upper
244 100
212 9.8 10.8 16.2#
122 8.4 8.0 12.0

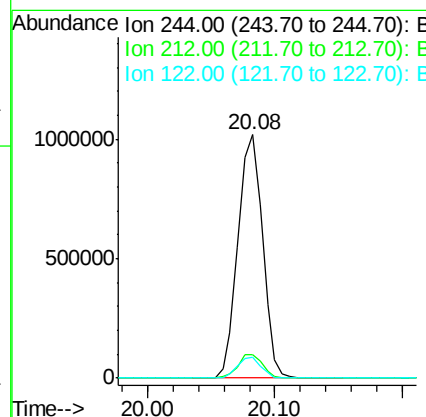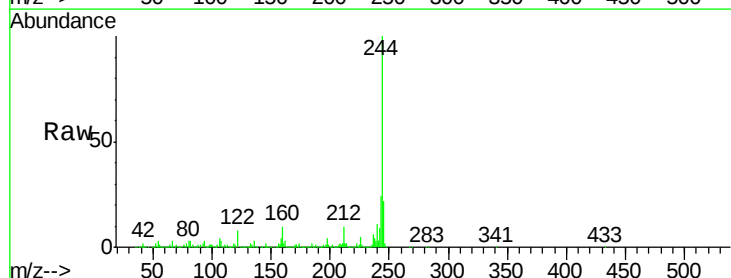

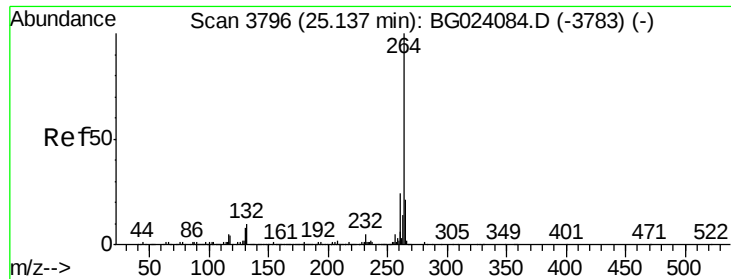

#86
Pervlene-d12
Concen: 20.00 ng
RT: 25.10 min Scan# 3790
Delta R.T. -0.03 min
Lab File: BG024165.D
Acq: 30 Sep 2016 18:44

Instrument :
BNA_G
ClientSampleId :
SUP-B046-12-13

Tot Ion	Ratio	Lower	Upper
264	100		
260	21.9	18.4	27.6
265	20.0	18.9	28.3

