

Data Path : Z:\HPCHEM1\BNA G\DATA\BG093016\
 Data File : BG024172.D
 Acq On : 30 Sep 2016 23:12
 Operator : UM/SJ
 Sample : PB93730TB
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB93730TB

Quant Time: Oct 01 04:21:57 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG092316.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 23 15:35:28 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.03	152	37220	20.00	ng	0.00
21) Naphthalene-d8	10.87	136	165733	20.00	ng	0.00
38) Acenaphthene-d10	14.71	164	137655	20.00	ng	0.00
63) Phenanthrene-d10	17.48	188	357546	20.00	ng	0.00
75) Chrysene-d12	21.78	240	431045	20.00	ng	-0.01
86) Perylene-d12	25.11	264	400314	20.00	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.58	112	251545	117.09	ng	0.00
7) Phenol-d6	7.20	99	370457	102.48	ng	0.00
23) Nitrobenzene-d5	9.22	82	259862	61.80	ng	0.00
41) 2,4,6-Tribromophenol	16.21	330	162256	82.00	ng	-0.02
44) 2-Fluorobiphenyl	13.32	172	547034	66.80	ng	-0.01
78) Terphenyl-d14	20.08	244	1200290	57.02	ng	-0.02


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG093016\
Data File : BG024172.D
Acq On : 30 Sep 2016 23:12
Operator : UM/SJ
Sample : PB93730TB
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB93730TB

Quant Time: Oct 01 04:21:57 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG092316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 23 15:35:28 2016
Response via : Initial Calibration

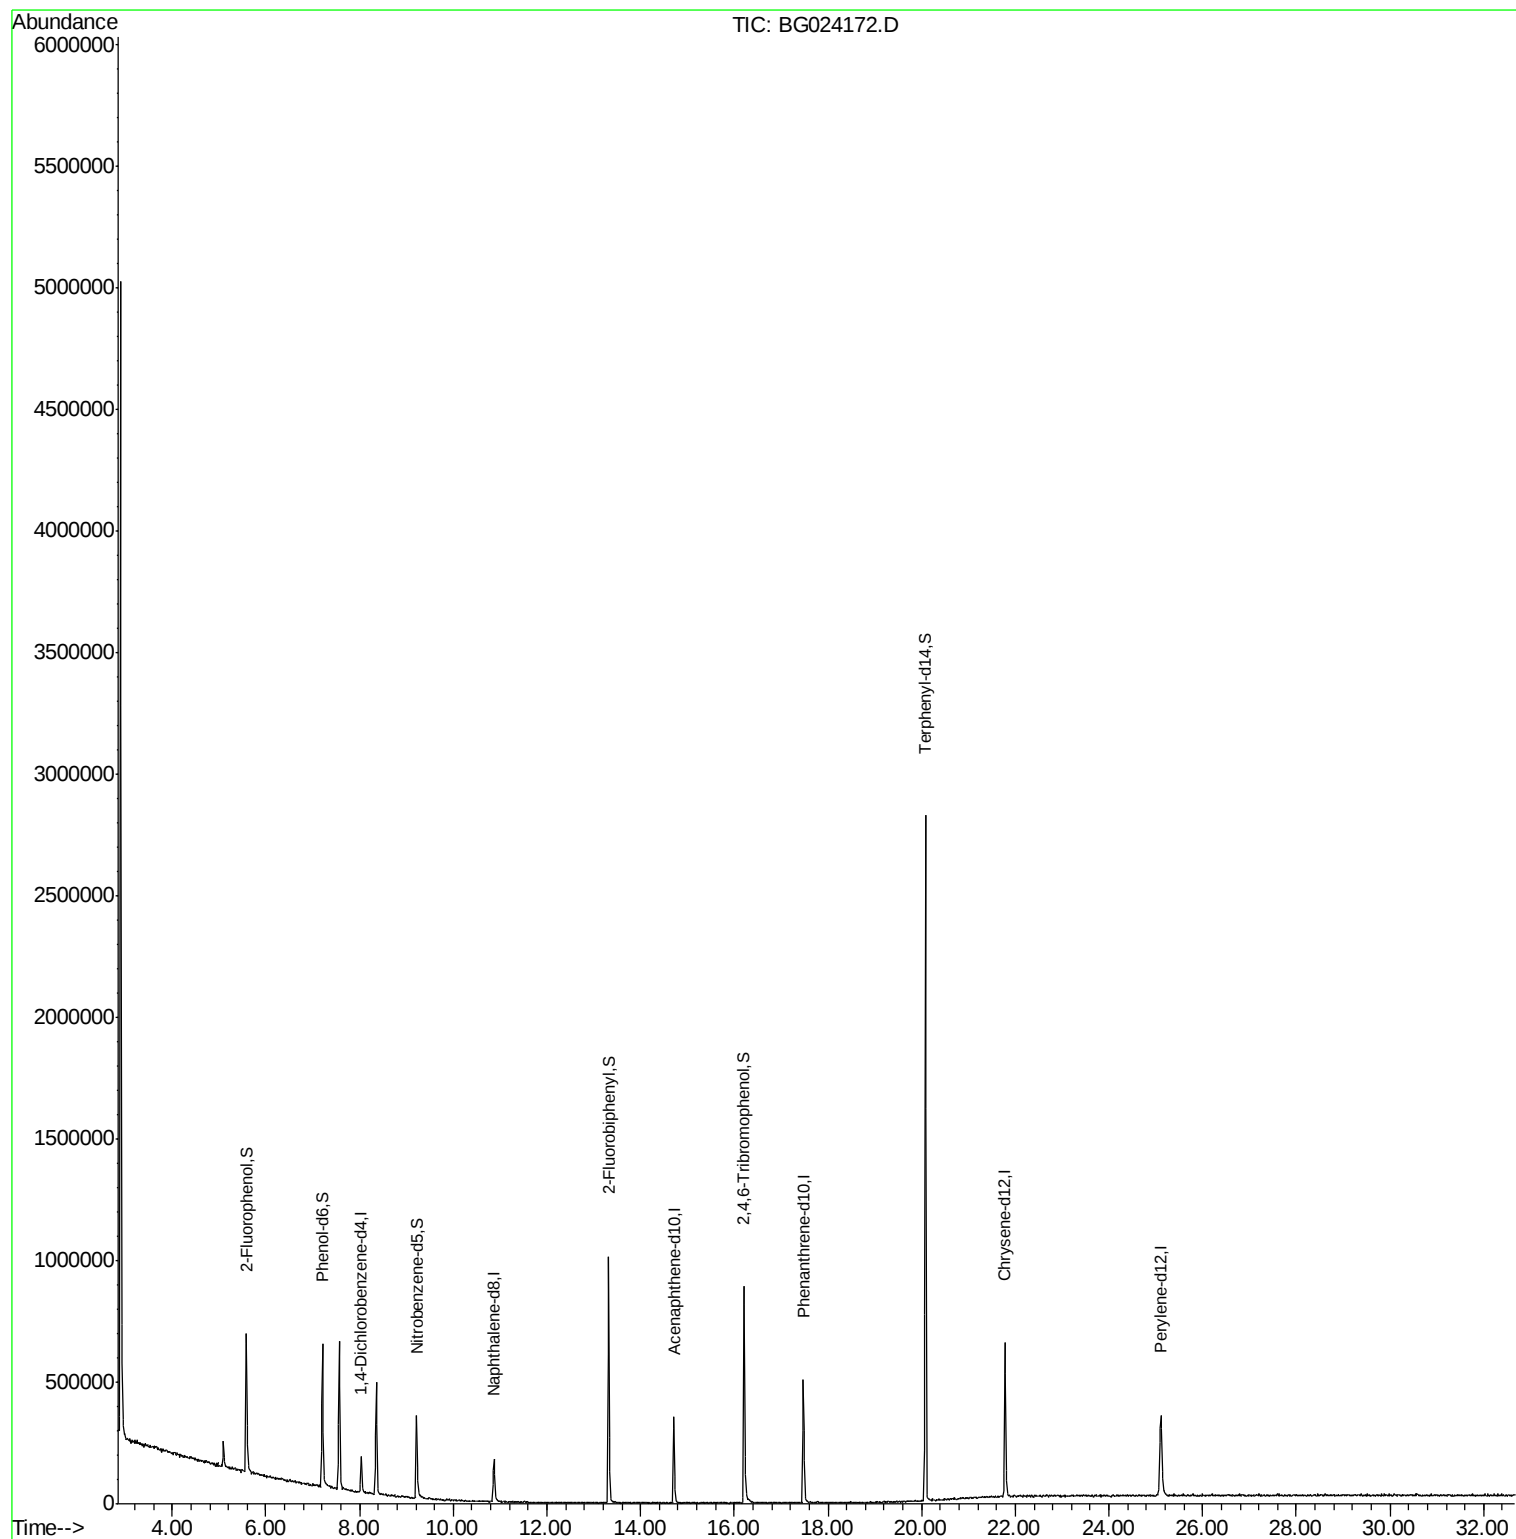

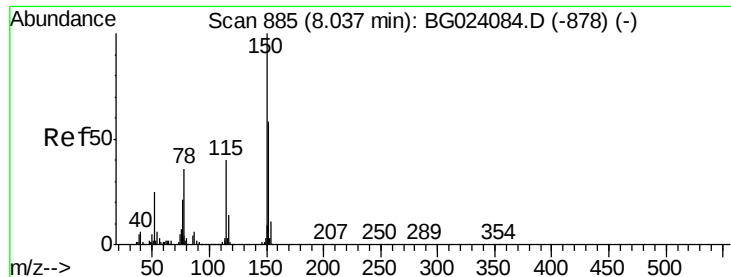

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 8.03 min Scan# 884

Delta R.T. -0.01 min

Lab File: BG024172.D

Acq: 30 Sep 2016 23:12

Instrument :

BNA_G

ClientSampleId :

PB93730TB


Tot Ion:152 Resp: 37220

Ion Ratio Lower Upper

152 100

150 148.2 144.7 217.1




115 73.7 64.0 96.0

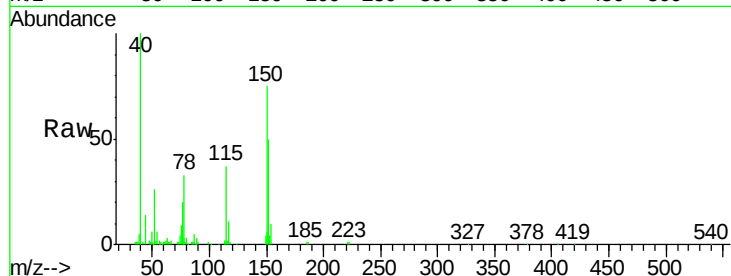

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

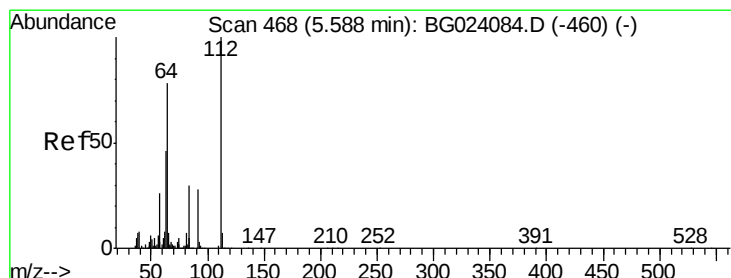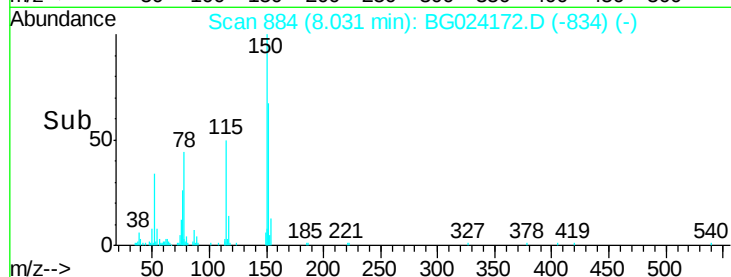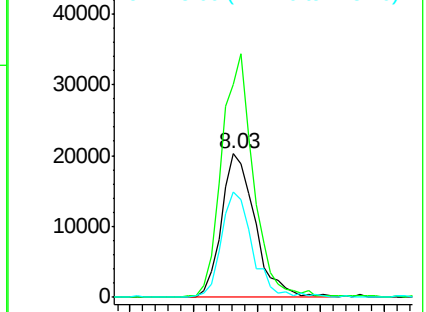

#5

2-Fluorophenol

Concen: 117.09 ng

RT: 5.58 min Scan# 467

Delta R.T. -0.01 min

Lab File: BG024172.D

Acq: 30 Sep 2016 23:12


Tgt Ion:112 Resp: 251545

Ion Ratio Lower Upper

112 100

64 74.9 59.0 88.4



63 42.5 37.8 56.8

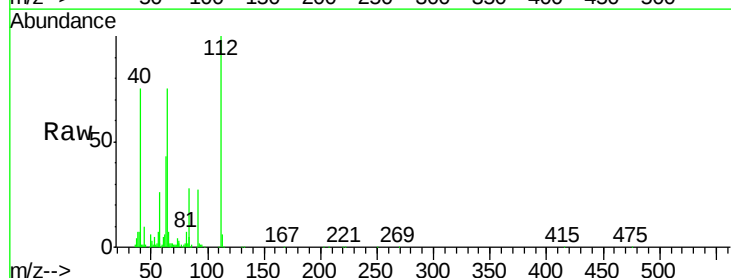


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BG0

Ion 63.00 (62.70 to 63.70): BG0

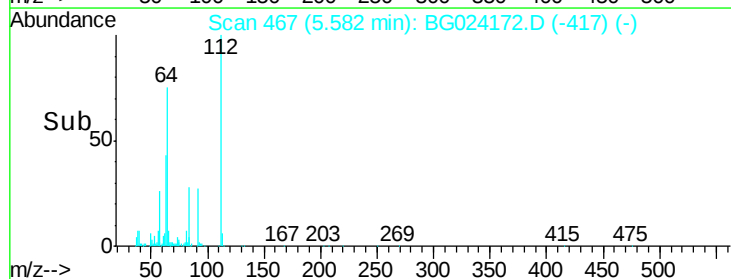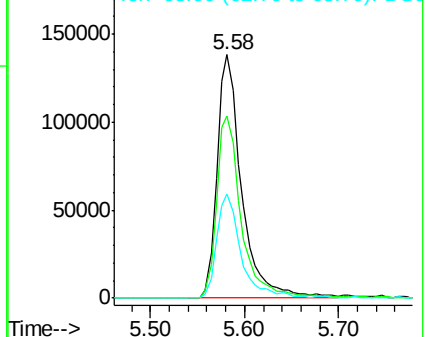

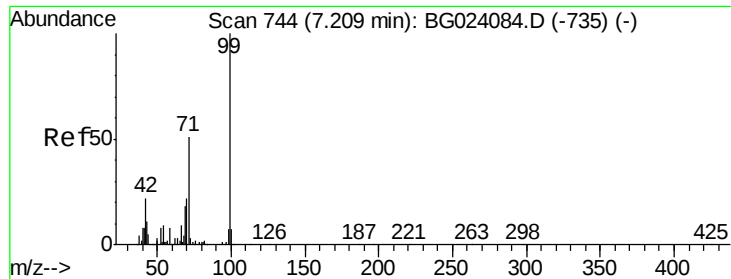

#7

Phenol-d6

Concen: 102.48 ng

RT: 7.20 min Scan# 743

Delta R.T. -0.01 min

Lab File: BG024172.D

Acq: 30 Sep 2016 23:12

Instrument :


BNA_G

ClientSampleId :

PB93730TB

Tot Ion: 99 Resp: 370457

Ion	Ratio	Lower	Upper
99	100		
42	21.3	17.8	26.6
71	45.6	41.5	62.3



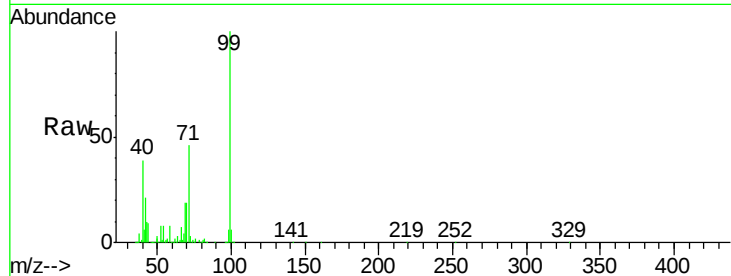


Abundance

Ion 99.00 (98.70 to 99.70): BGC

Ion 42.00 (41.70 to 42.70): BGC

Ion 71.00 (70.70 to 71.70): BGC

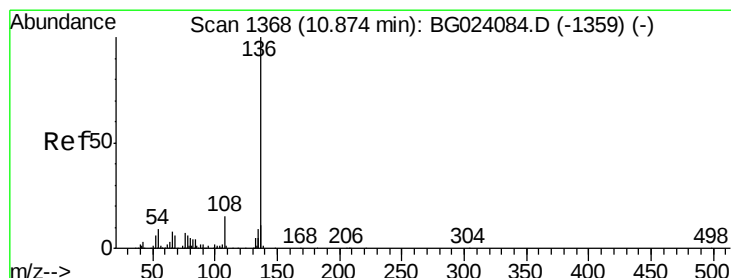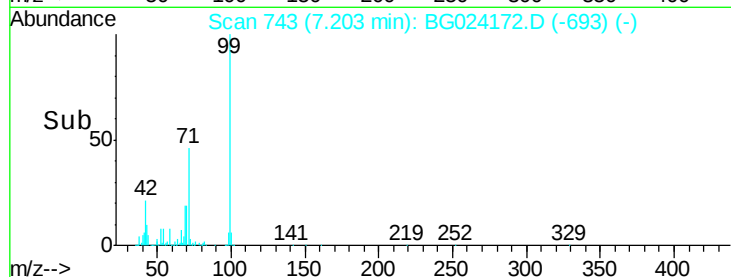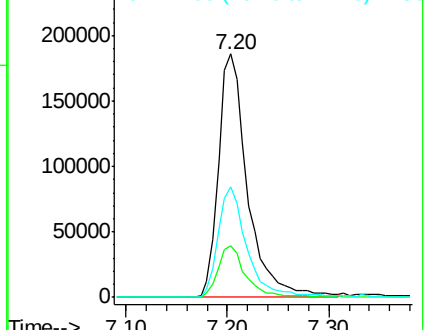

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.87 min Scan# 1367


Delta R.T. -0.01 min

Lab File: BG024172.D

Acq: 30 Sep 2016 23:12

Tgt Ion: 136 Resp: 165733

Ion	Ratio	Lower	Upper
136	100		
137	11.9	9.6	14.4
54	11.9	7.3	10.9
68	6.3	5.3	7.9

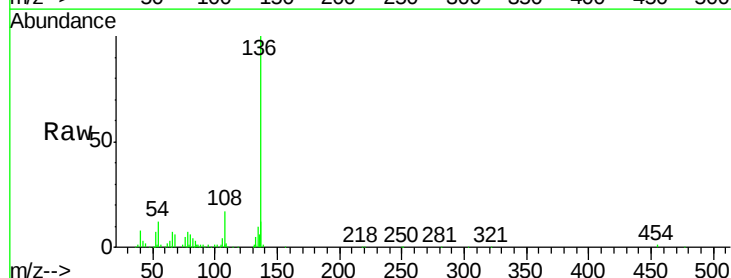



Abundance


Ion 136.00 (135.70 to 136.70): BGC

Ion 137.00 (136.70 to 137.70): BGC

Ion 54.00 (53.70 to 54.70): BGC

Ion 68.00 (67.70 to 68.70): BGC



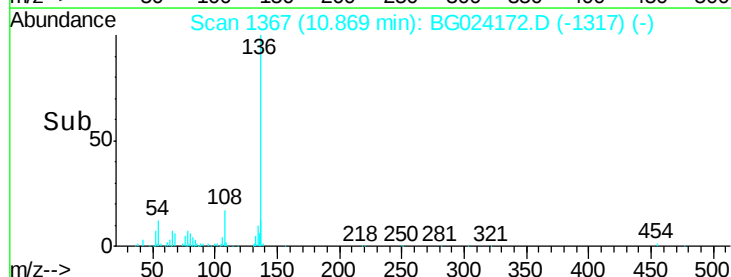
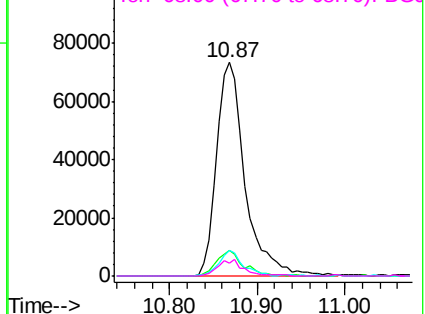


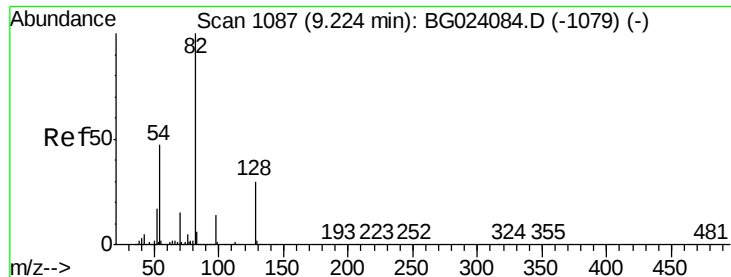

#23
 Nitrobenzene-d5
 Concen: 61.80 ng
 RT: 9.22 min Scan# 1086
 Delta R.T. -0.01 min
 Lab File: BG024172.D
 Acq: 30 Sep 2016 23:12




Instrument :
 BNA_G
 ClientSampleId :
 PB93730TB


Tot Ion	82	Resp	259862
Ion Ratio	Lower	Upper	
82	100		
128	33.7	24.4	36.6
54	49.1	41.4	62.0

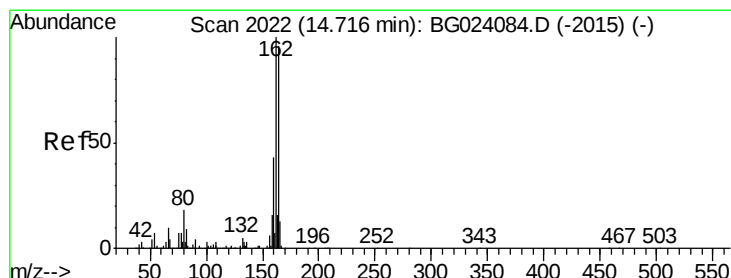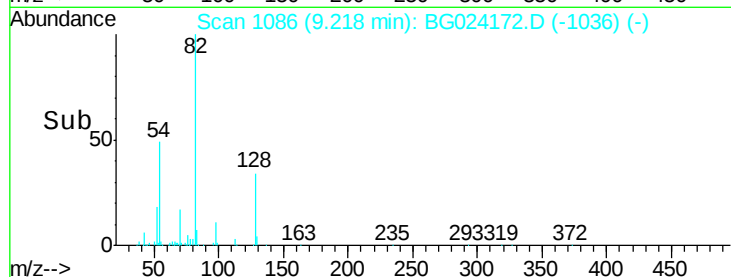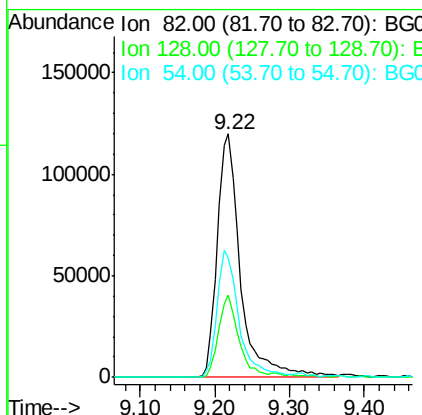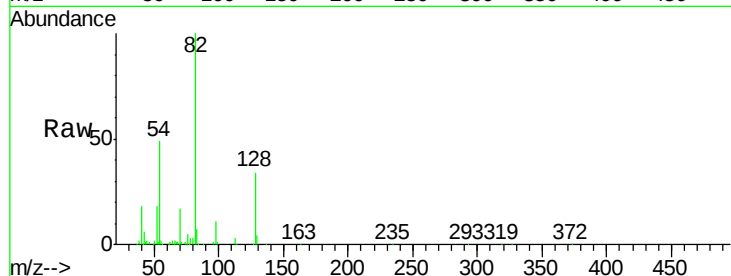

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 14.71 min Scan# 2021
 Delta R.T. -0.01 min
 Lab File: BG024172.D
 Acq: 30 Sep 2016 23:12

Tgt Ion	164	Resp	137655
Ion Ratio	Lower	Upper	
164	100		
162	102.7	87.7	131.5
160	48.7	37.2	55.8

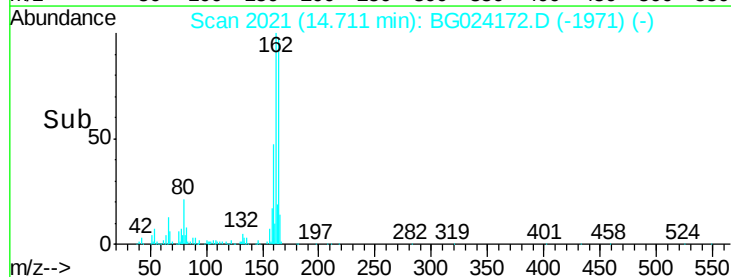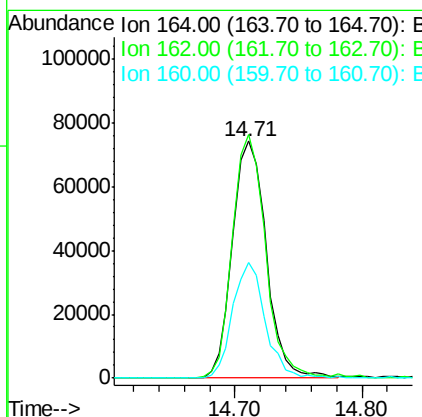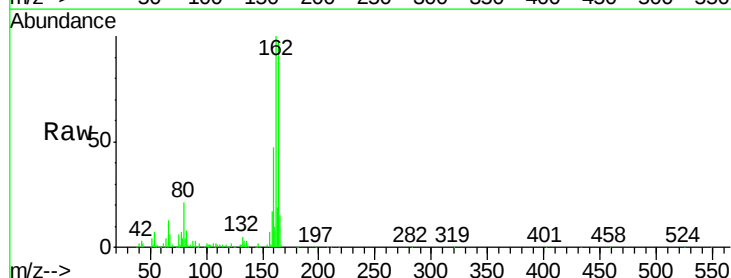


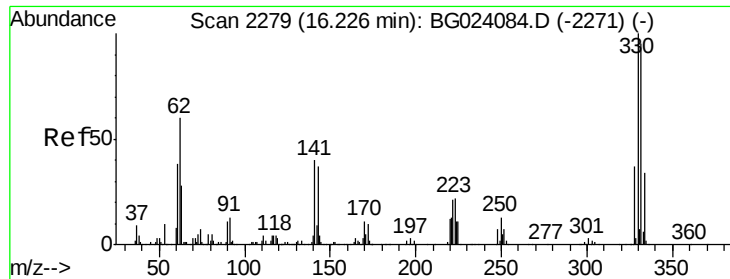




#41
 2,4,6-Tribromophenol
 Concen: 82.00 ng
 RT: 16.21 min Scan# 2276
 Delta R.T. -0.02 min
 Lab File: BG024172.D
 Acq: 30 Sep 2016 23:12

Instrument :
 BNA_G
 ClientSampleId :
 PB93730TB

Tot Ion:330 Resp: 162256
 Ion Ratio Lower Upper
 330 100
 332 98.1 77.4 116.2
 141 46.4 31.7 47.5

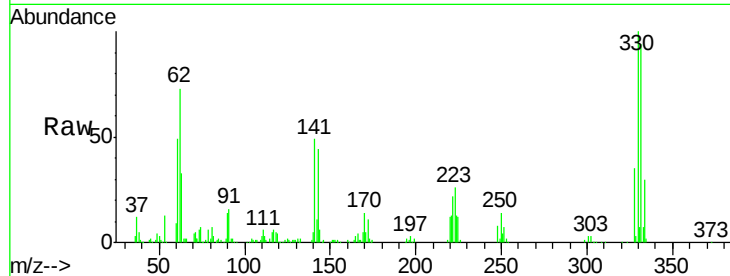


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

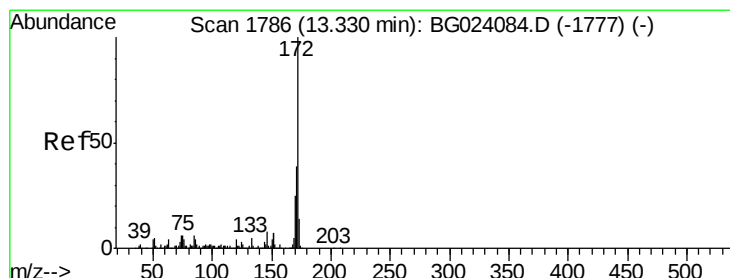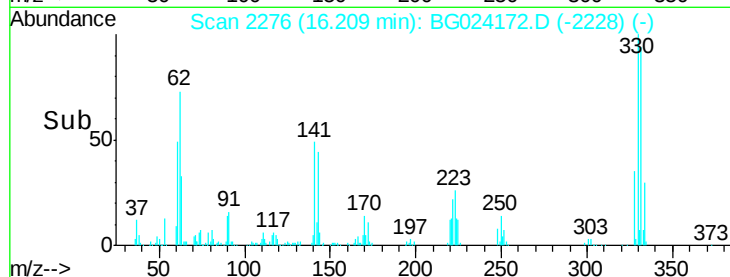
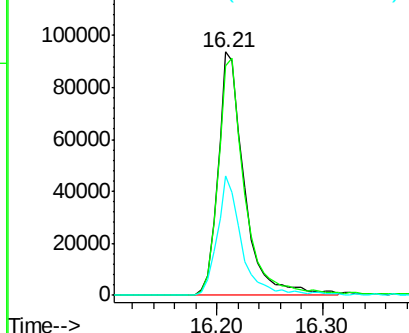



#44
 2-Fluorobiphenyl
 Concen: 66.80 ng
 RT: 13.32 min Scan# 1784
 Delta R.T. -0.01 min
 Lab File: BG024172.D
 Acq: 30 Sep 2016 23:12

Tgt Ion:172 Resp: 547034
 Ion Ratio Lower Upper
 172 100
 171 36.3 31.6 47.4
 170 26.7 21.3 31.9

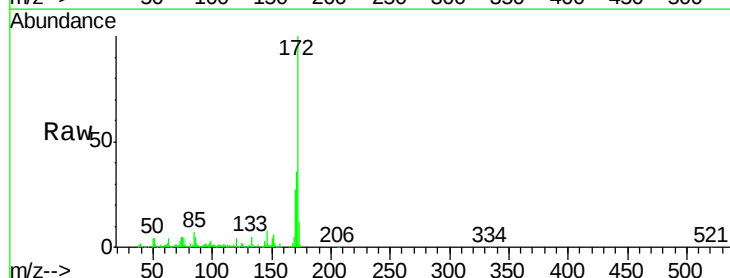

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



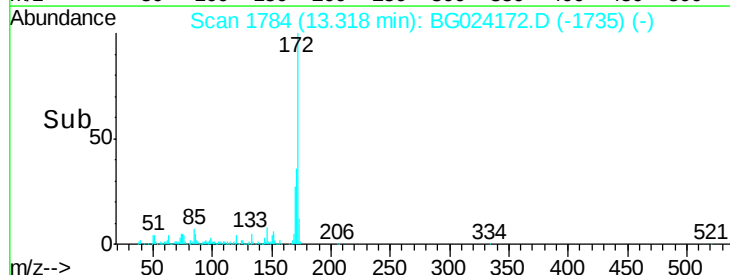
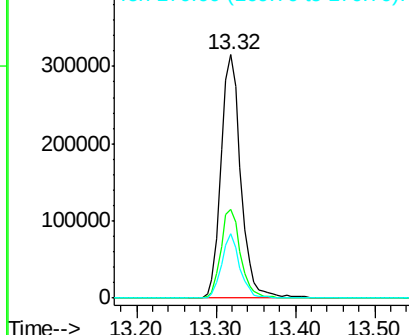


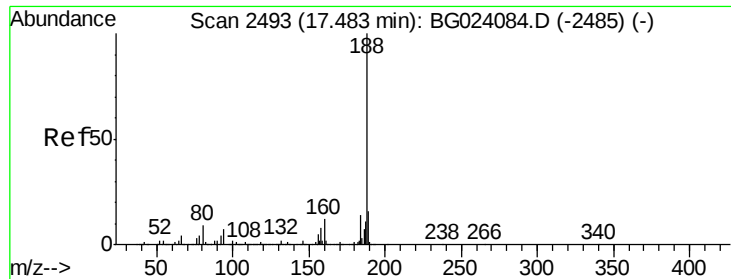

#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.48 min Scan# 2492
Delta R.T. -0.01 min
Lab File: BG024172.D
Acq: 30 Sep 2016 23:12




Instrument :
BNA_G
ClientSampleId :
PB93730TB


Tot Ion:188 Resp: 357546
Ion Ratio Lower Upper
188 100
94 6.8 5.2 7.8
80 9.9 7.2 10.8

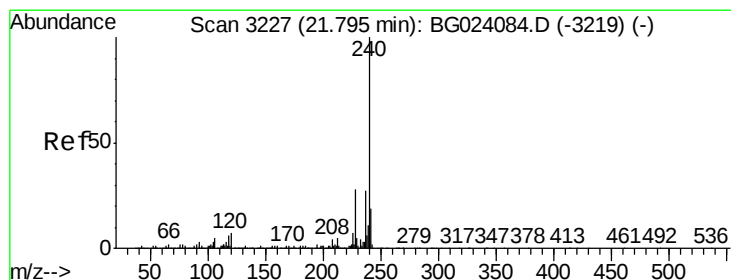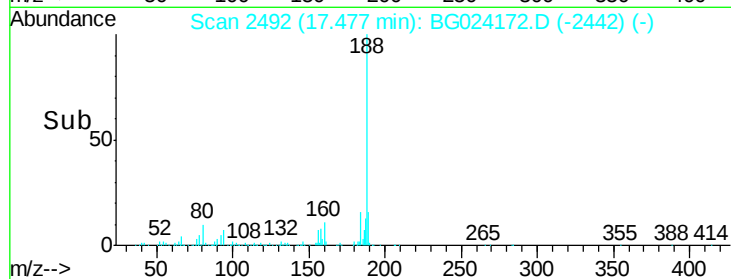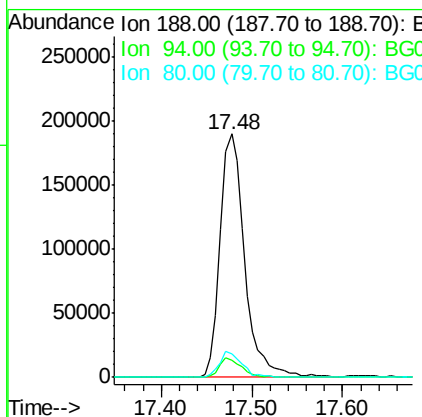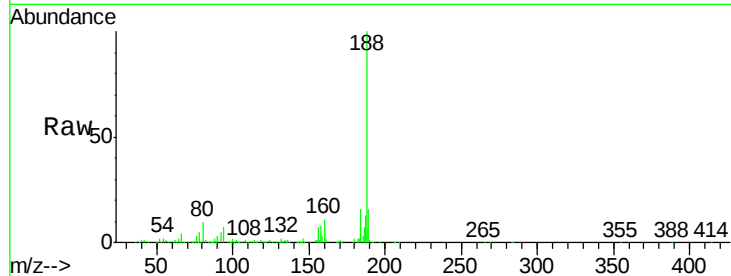

#75
Chrysene-d12
Concen: 20.00 ng
RT: 21.78 min Scan# 3225
Delta R.T. -0.01 min
Lab File: BG024172.D
Acq: 30 Sep 2016 23:12

Tgt Ion:240 Resp: 431045
Ion Ratio Lower Upper
240 100
120 7.1 4.1 6.1#
236 24.8 21.1 31.7

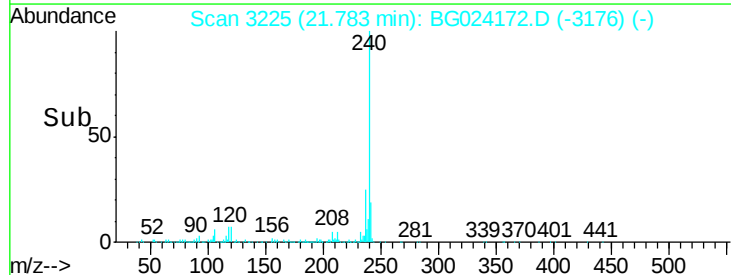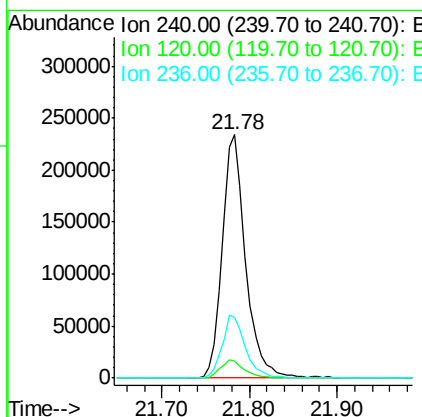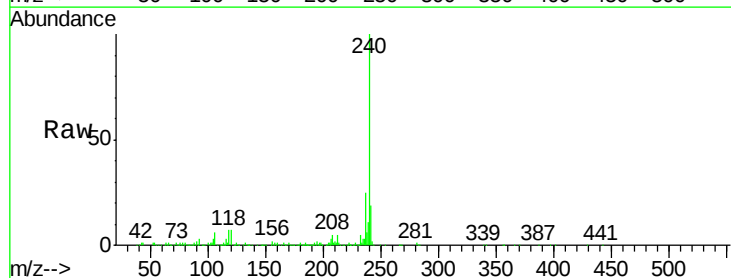

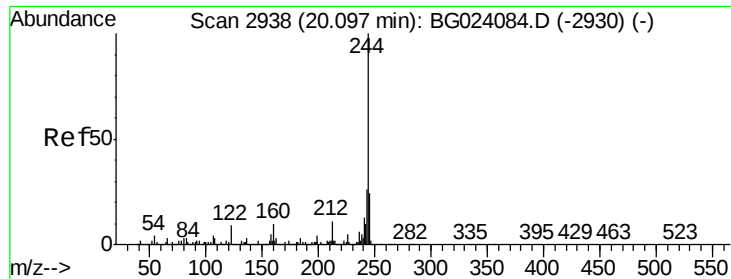

#78

Terphenyl-d14

Concen: 57.02 ng

RT: 20.08 min Scan# 2935

Delta R.T. -0.02 min

Lab File: BG024172.D

Acq: 30 Sep 2016 23:12

Instrument :

BNA_G

ClientSampleId :

PB93730TB


Tot Ion:244 Resp: 1200290

Ion Ratio Lower Upper

244 100

212 10.2 10.8 16.2#




122 9.1 8.0 12.0

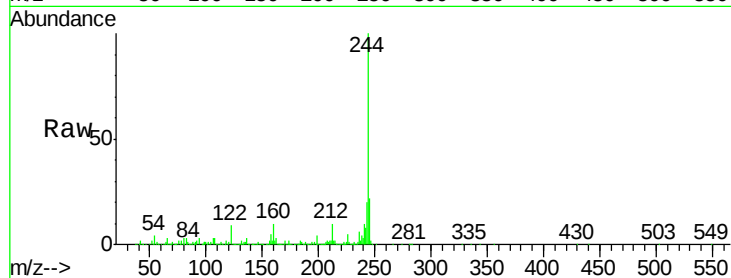

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

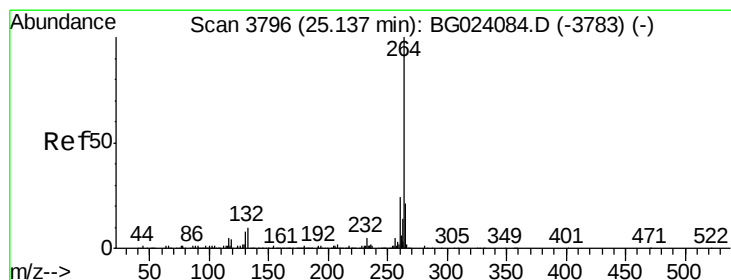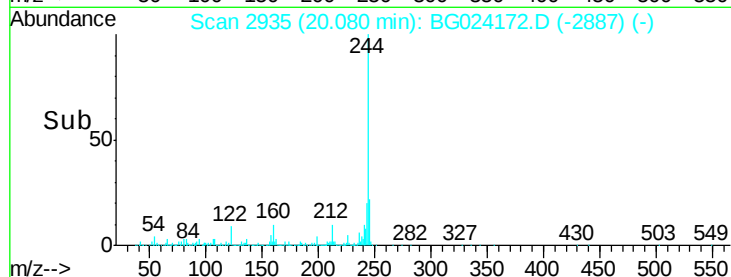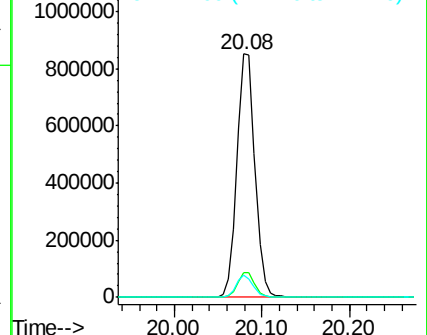

#86

Perylene-d12

Concen: 20.00 ng

RT: 25.11 min Scan# 3791

Delta R.T. -0.03 min

Lab File: BG024172.D

Acq: 30 Sep 2016 23:12


Tgt Ion:264 Resp: 400314

Ion Ratio Lower Upper

264 100

260 24.1 18.4 27.6

265 21.0 18.9 28.3

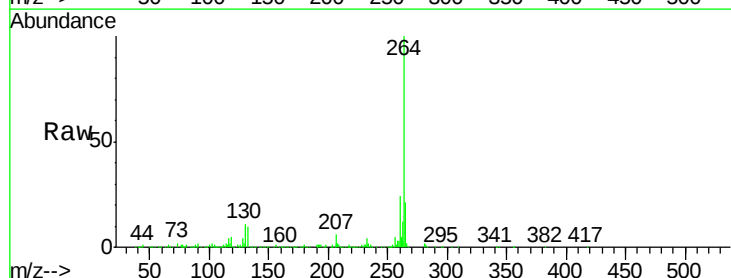

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

