


Data Path : Z:\HPCHEM1\BNA G\DATA\BG093016\
 Data File : BG024157.D
 Acq On : 30 Sep 2016 12:33
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG092316.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 23 15:35:28 2016

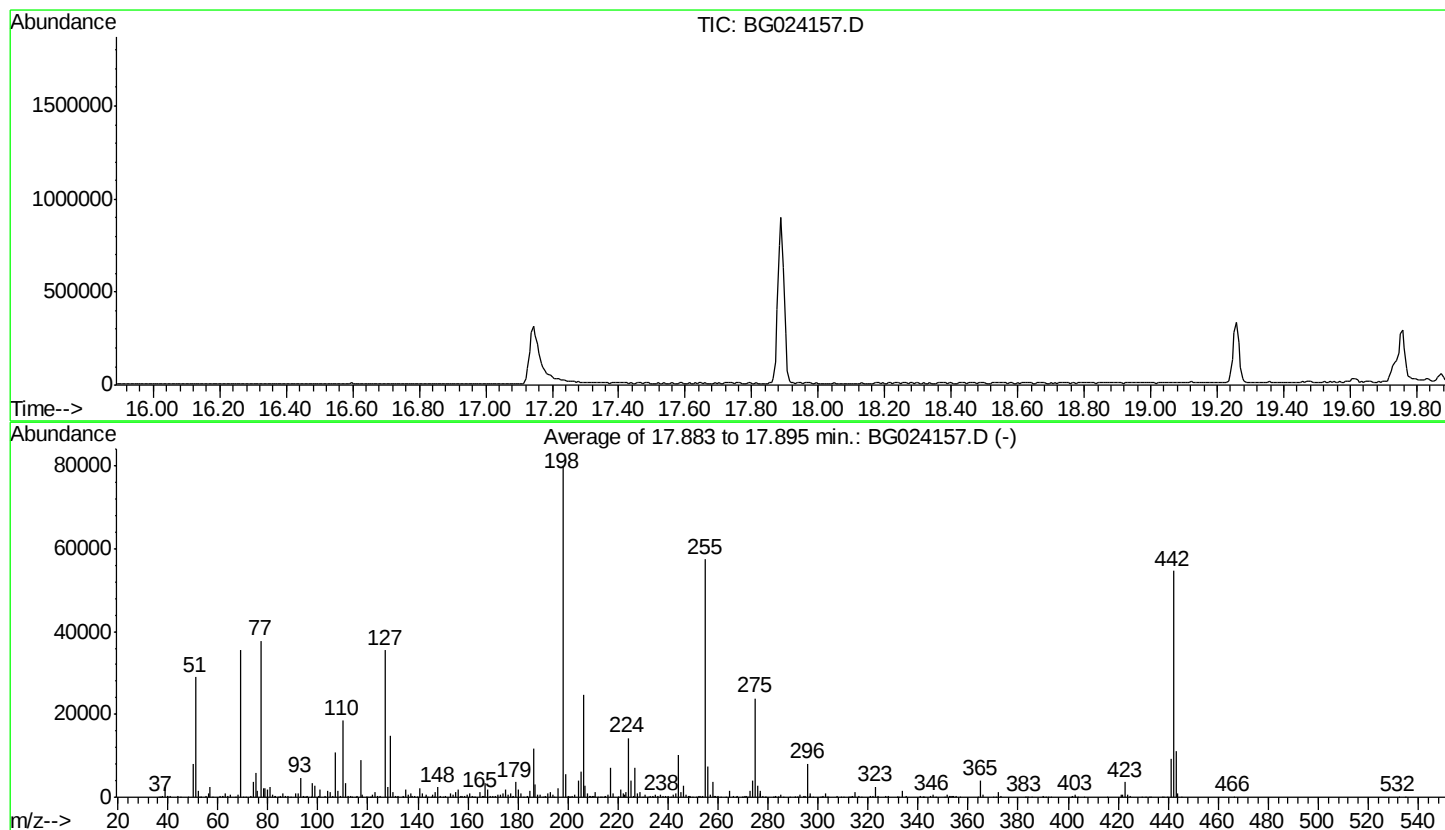

AutoFind: Scans 2561, 2562, 2563; Background Corrected with Scan 2554

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.2	28952	PASS
68	69	0.00	2	1.4	491	PASS
69	198	0.00	100	44.2	35405	PASS
70	69	0.00	2	0.4	139	PASS
127	198	10	80	44.4	35538	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	80056	PASS
199	198	5	9	7.0	5643	PASS
275	198	10	60	29.9	23901	PASS
365	198	1	100	4.9	3950	PASS
441	442	0.01	24	17.1	9332	PASS
442	198	50	100	68.3	54682	PASS
443	442	15	24	20.1	11005	PASS