


Data Path : Z:\HPCHEM1\BNA G\DATA\BG093016\
 Data File : BG024176.D
 Acq On : 1 Oct 2016 1:45
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG092316.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 23 15:35:28 2016

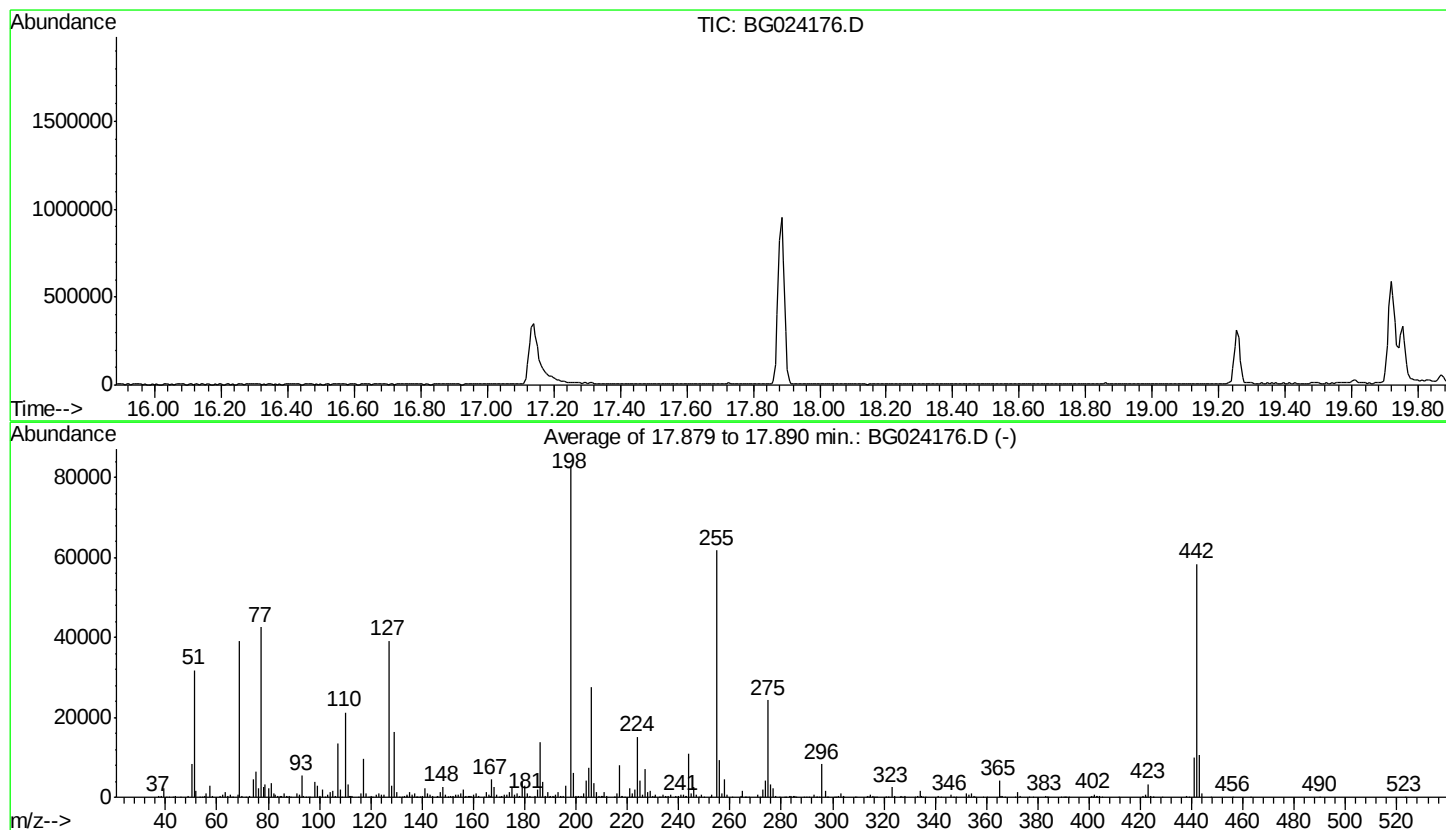

AutoFind: Scans 2560, 2561, 2562; Background Corrected with Scan 2553

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.3	31797	PASS
68	69	0.00	2	1.8	690	PASS
69	198	0.00	100	47.1	39077	PASS
70	69	0.00	2	0.5	200	PASS
127	198	10	80	47.2	39162	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	82952	PASS
199	198	5	9	7.5	6218	PASS
275	198	10	60	29.3	24304	PASS
365	198	1	100	4.9	4100	PASS
441	442	0.01	24	17.1	9969	PASS
442	198	50	100	70.4	58410	PASS
443	442	15	24	18.0	10531	PASS