

Data Path : Z:\HPCHEM1\BNA G\DATA\BG093017\
 Data File : BG028990.D
 Acq On : 30 Sep 2017 22:04
 Operator : SJ/JU
 Sample : I5491-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Oct 01 02:23:00 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG091217.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 12 16:57:11 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.25	152	29855	20.00	ng	-0.08
21) Naphthalene-d8	11.07	136	123107	20.00	ng	-0.08
38) Acenaphthene-d10	14.87	164	96097	20.00	ng	-0.07
63) Phenanthrene-d10	17.62	188	277965	20.00	ng	-0.07
75) Chrysene-d12	21.94	240	322822	20.00	ng	-0.09
86) Perylene-d12	25.37	264	340025	20.00	ng	-0.16
System Monitoring Compounds						
5) 2-Fluorophenol	5.82	112	284496	157.24	ng	-0.08
7) Phenol-d6	7.41	99	341186	125.24	ng	-0.08
23) Nitrobenzene-d5	9.43	82	273851	106.41	ng	-0.08
41) 2,4,6-Tribromophenol	16.37	330	296797	186.74	ng	-0.07
44) 2-Fluorobiphenyl	13.49	172	726402	100.79	ng	-0.07
78) Terphenyl-d14	20.22	244	1547242	102.21	ng	-0.06
Target Compounds						
15) Benzyl Alcohol	8.59	79	4465	2.100	ng	Qvalue # 52

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG093017\
Data File : BG028990.D
Acq On : 30 Sep 2017 22:04
Operator : SJ/JU
Sample : I5491-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Oct 01 02:23:00 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG091217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 16:57:11 2017
Response via : Initial Calibration

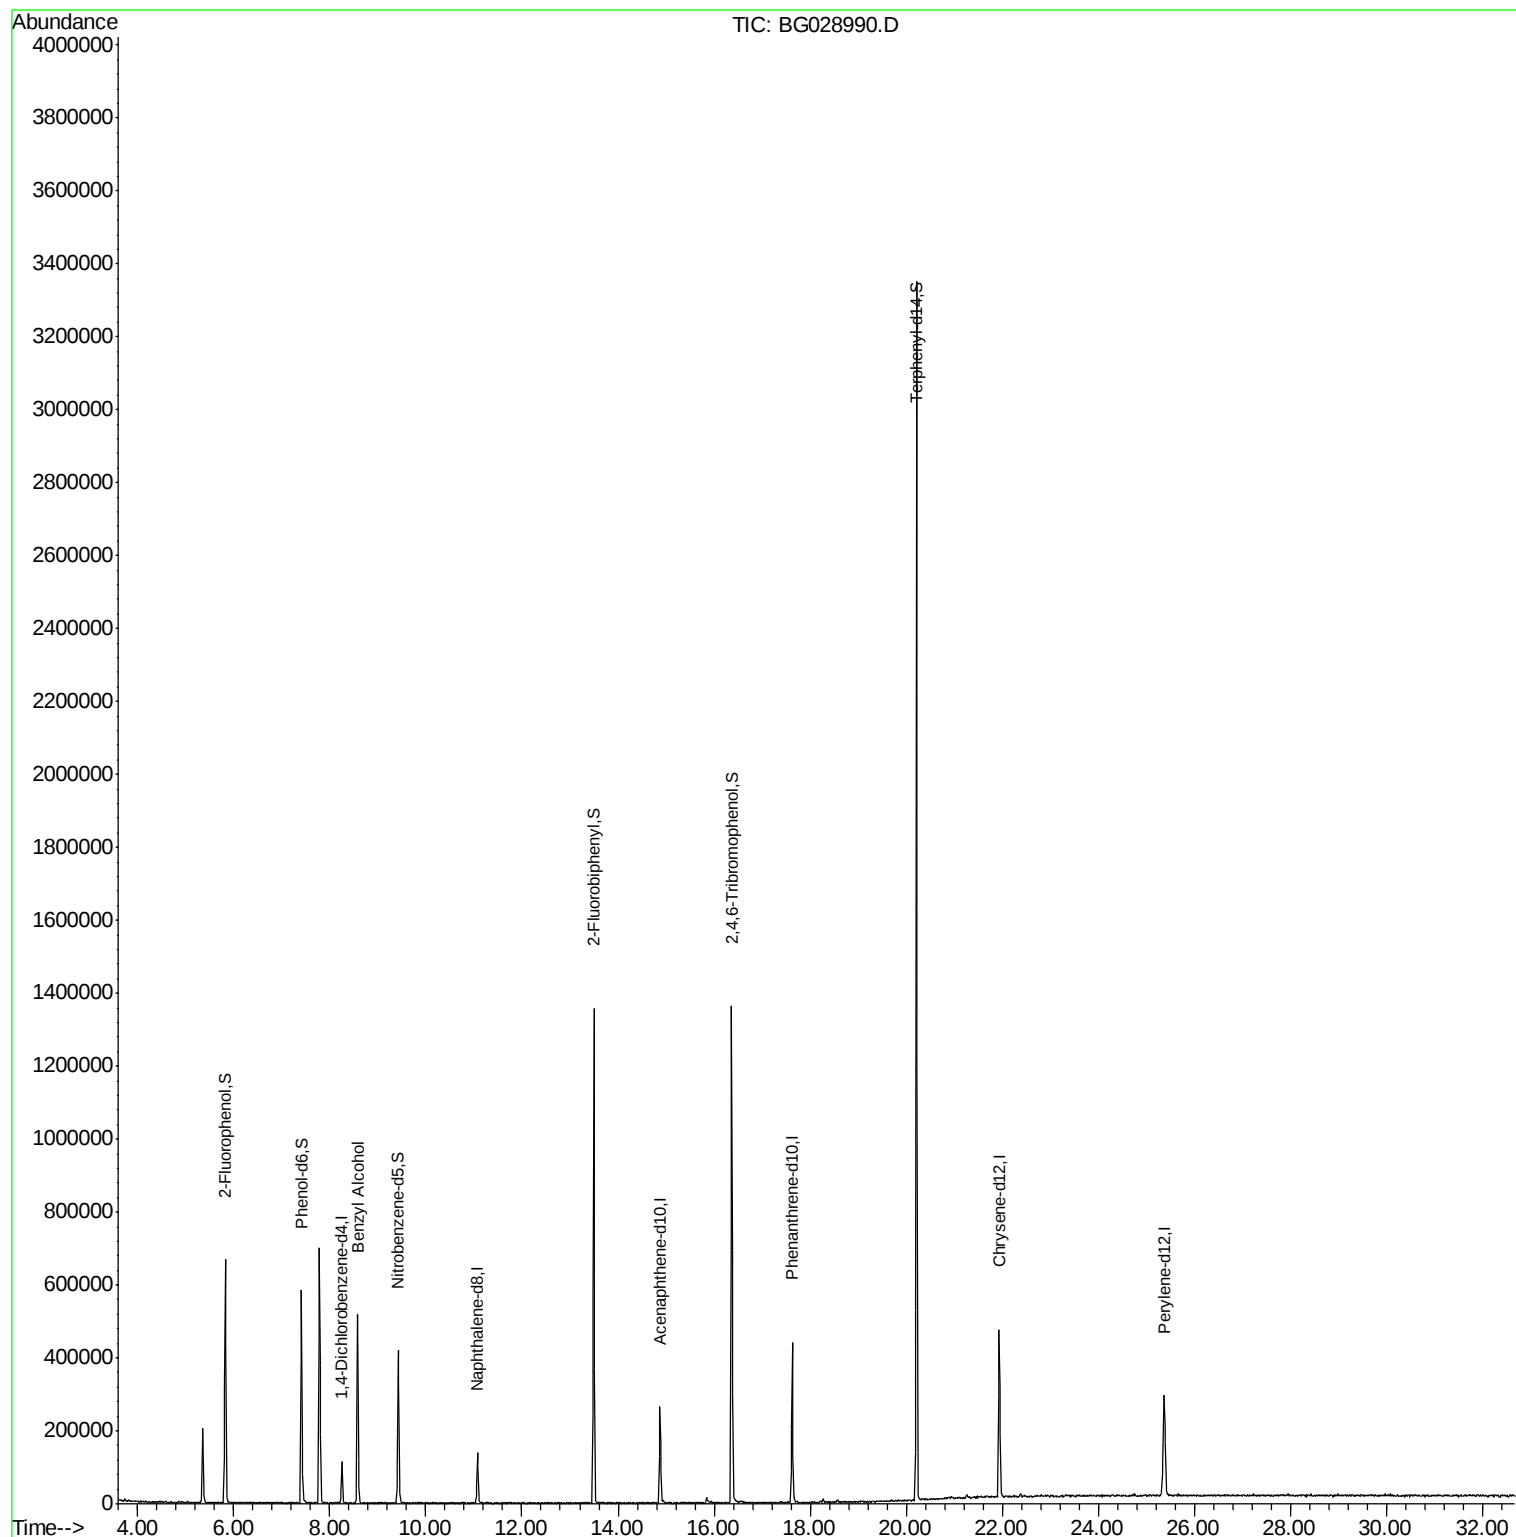






#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.25 min Scan# 794
Delta R.T. -0.08 min
Lab File: BG028990.D
Acq: 30 Sep 2017 22:04

Instrument :
BNA_G
ClientSampleId :




Tot Ion	Ratio	Lower	Upper
152	100		
150	152.3	114.0	171.0
115	57.3	48.1	72.1

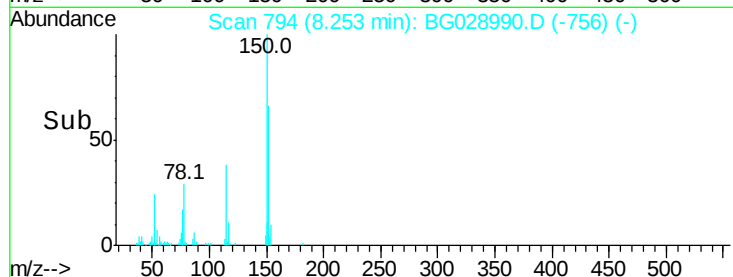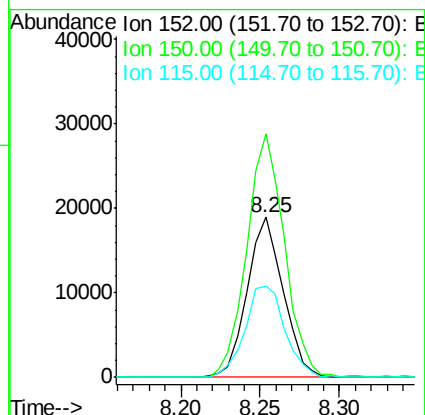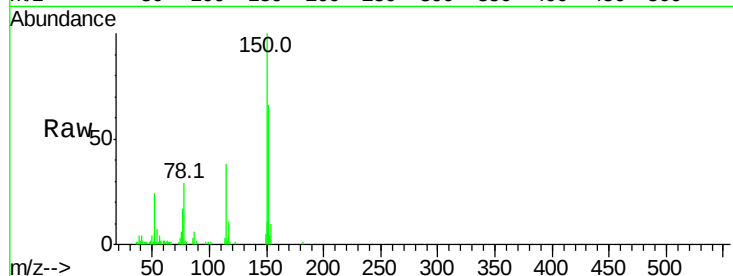


#5

2-Fluorophenol
Concen: 157.237 ng
RT: 5.82 min Scan# 380
Delta R.T. -0.08 min
Lab File: BG028990.D
Acq: 30 Sep 2017 22:04

Tgt Ion	Ratio	Lower	Upper
112	100		
64	70.8	61.8	92.6
63	39.3	37.2	55.8

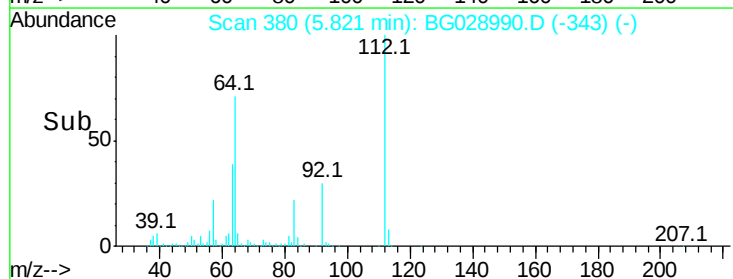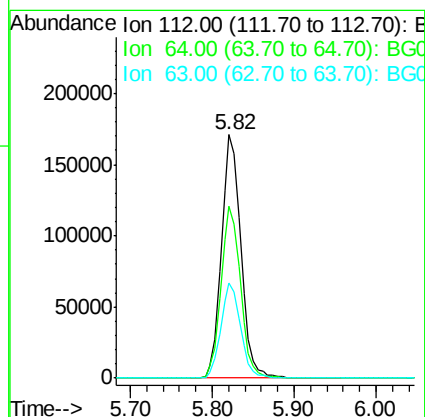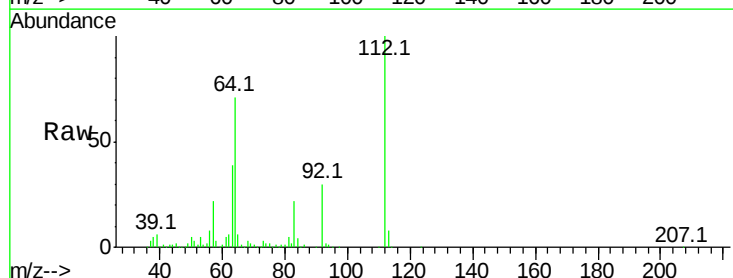

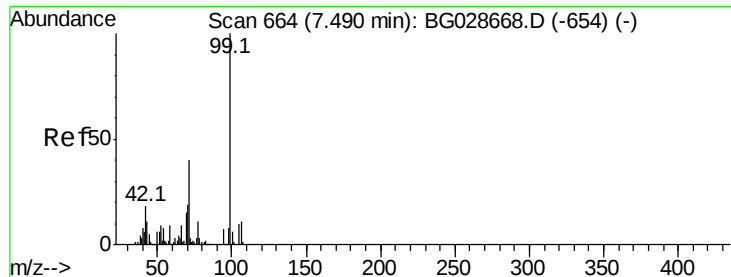

#7

Phenol-d6

Concen: 125.244 ng

RT: 7.41 min Scan# 651

Delta R.T. -0.08 min

Lab File: BG028990.D

Acq: 30 Sep 2017 22:04

Instrument :

BNA_G

ClientSampleId :





Tot Ion: 99 Resp: 341186

Ion Ratio Lower Upper

99 100

42 18.5 20.5 30.7#

71 42.2 37.6 56.4

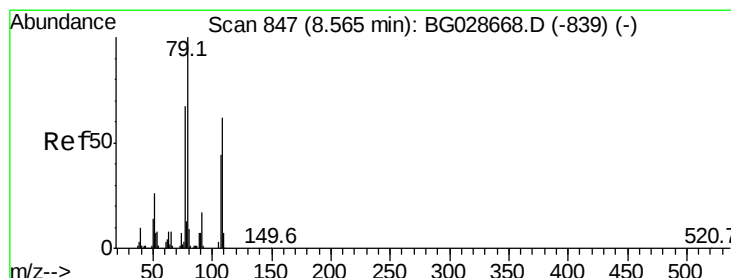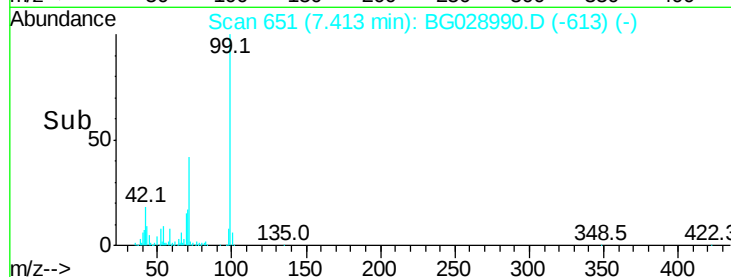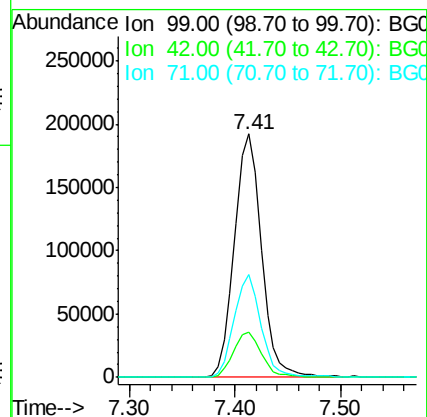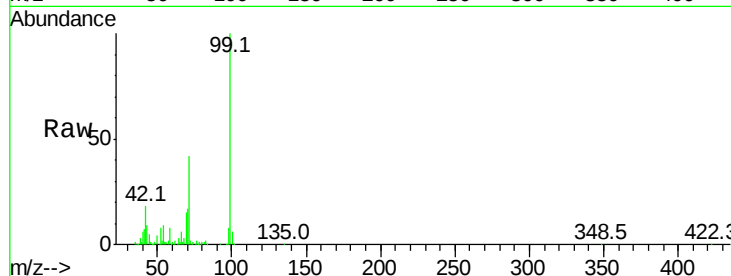

#15

Benzyl Alcohol

Concen: 2.100 ng

RT: 8.59 min Scan# 851

Delta R.T. 0.02 min

Lab File: BG028990.D

Acq: 30 Sep 2017 22:04




Tgt Ion: 79 Resp: 4465


Ion Ratio Lower Upper

79 100

108 16.7 45.5 68.3#

77 102.5 54.3 81.5#

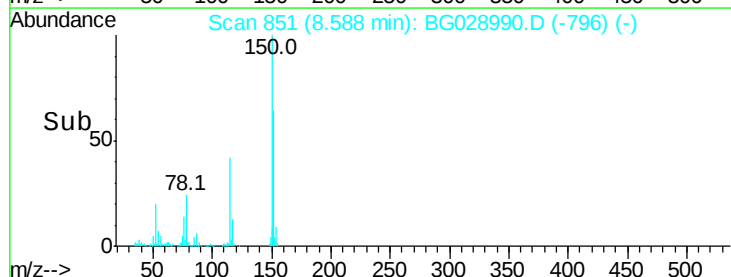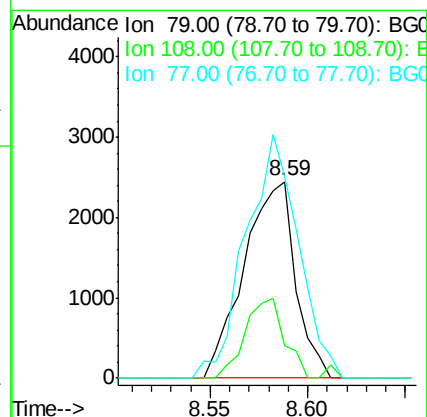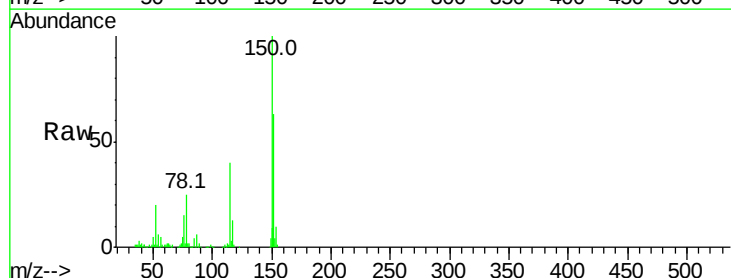


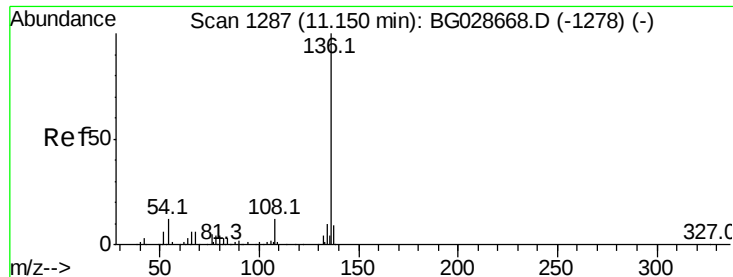




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 11.07 min Scan# 1274
Delta R.T. -0.08 min
Lab File: BG028990.D
Acq: 30 Sep 2017 22:04

Instrument :
BNA_G
ClientSampleId :

Tot Ion:	136	Resp:	123107
Ion	Ratio	Lower	Upper
136	100		
137	11.2	8.9	13.3
54	13.4	9.3	13.9
68	5.5	5.1	7.7

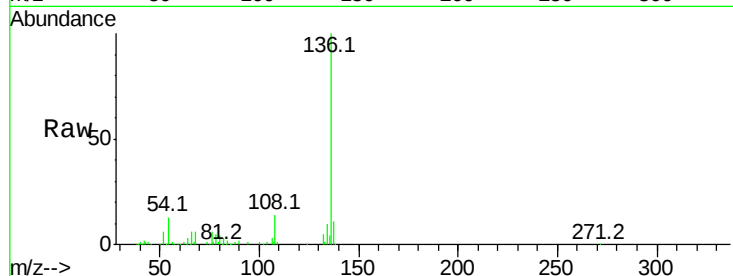


Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

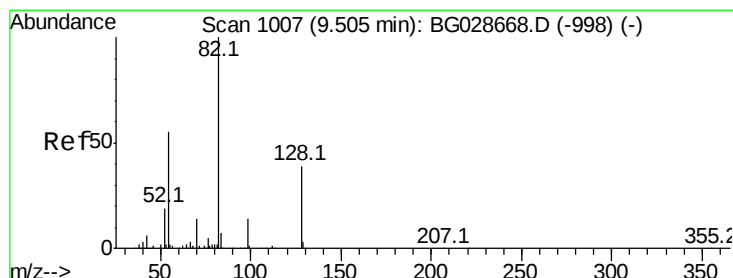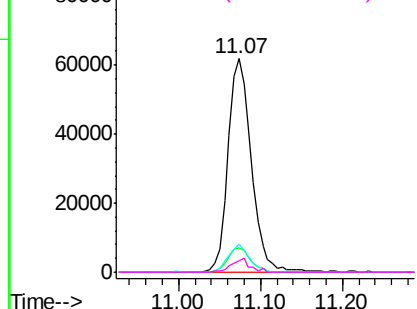
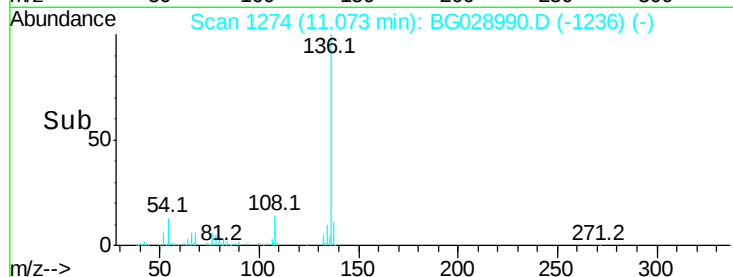



#23
Nitrobenzene-d5
Concen: 106.414 ng
RT: 9.43 min Scan# 994
Delta R.T. -0.08 min
Lab File: BG028990.D
Acq: 30 Sep 2017 22:04

Tgt Ion:	82	Resp:	273851
Ion	Ratio	Lower	Upper
82	100		
128	39.3	26.4	39.6
54	56.9	49.4	74.2

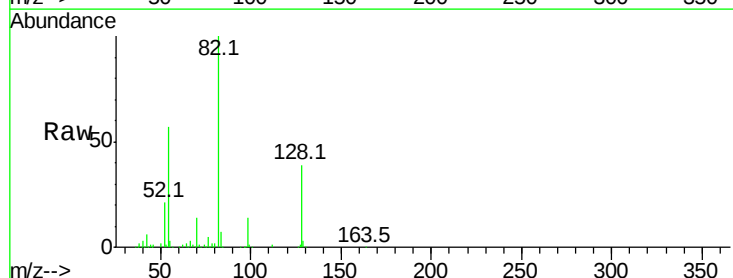

Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): BGC
Ion 54.00 (53.70 to 54.70): BGC



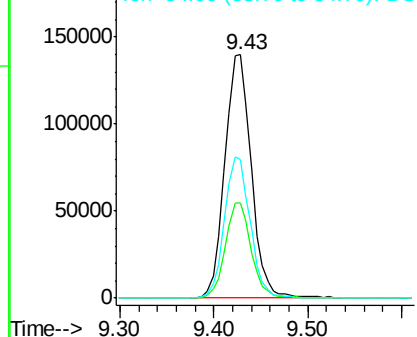
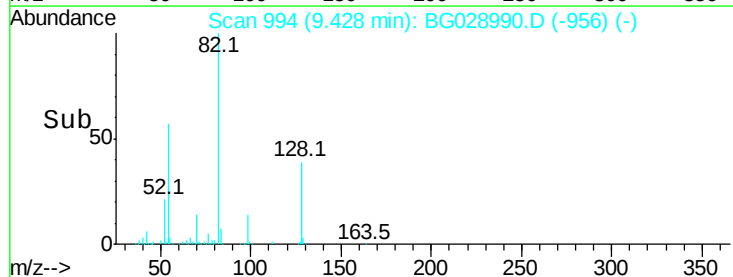


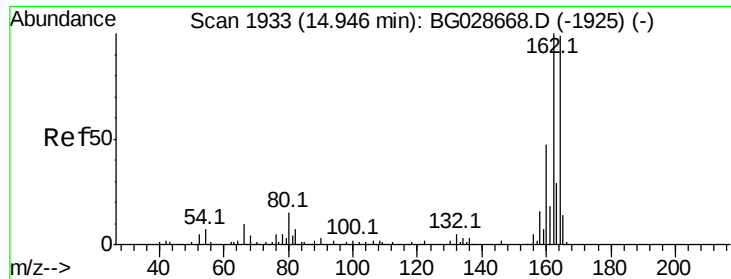

#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.87 min Scan# 1921
 Delta R.T. -0.07 min
 Lab File: BG028990.D
 Acq: 30 Sep 2017 22:04




Instrument :
 BNA_G
 ClientSampleId :


Tot Ion	Ratio	Lower	Upper
164	100		
162	100.9	85.1	127.7
160	43.5	34.7	52.1

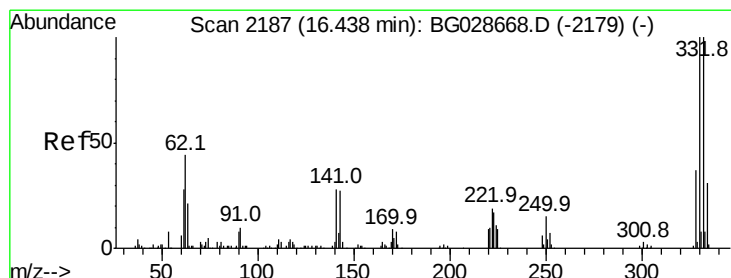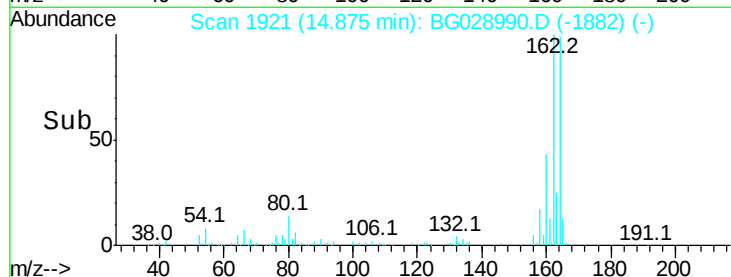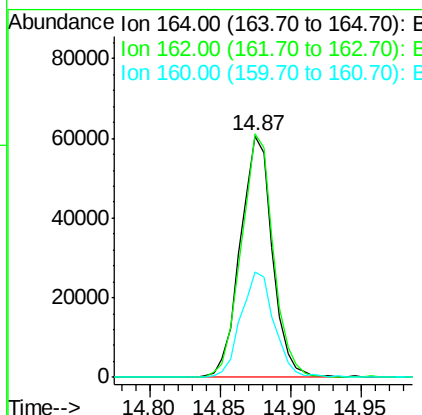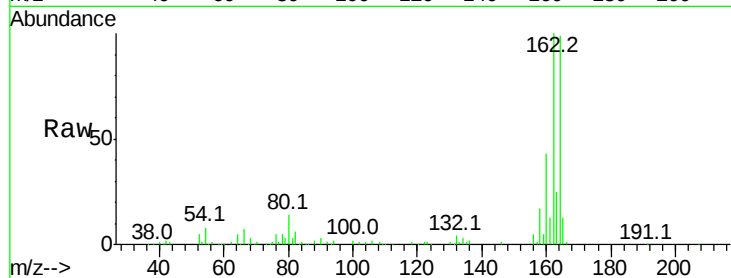

#41
 2,4,6-Tribromophenol
 Concen: 186.737 ng
 RT: 16.37 min Scan# 2175
 Delta R.T. -0.07 min
 Lab File: BG028990.D
 Acq: 30 Sep 2017 22:04

Tgt Ion	Ratio	Lower	Upper
330	100		
332	97.8	77.3	115.9
141	29.9	32.1	48.1#

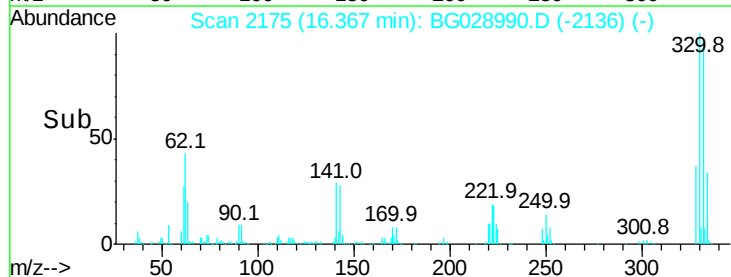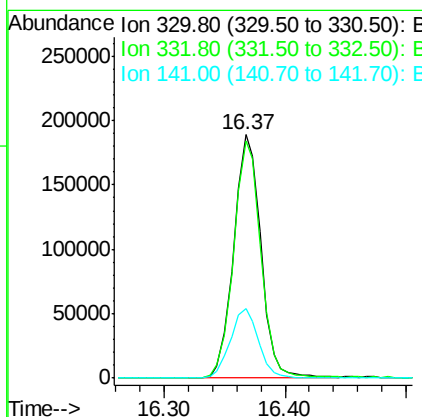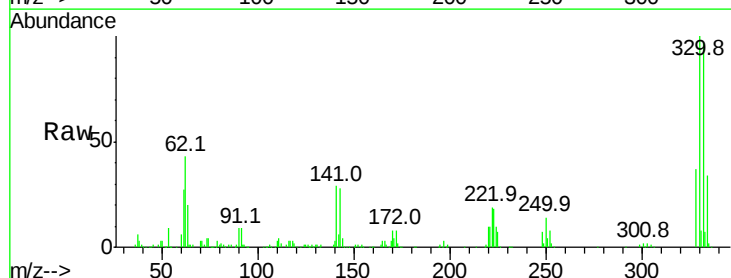




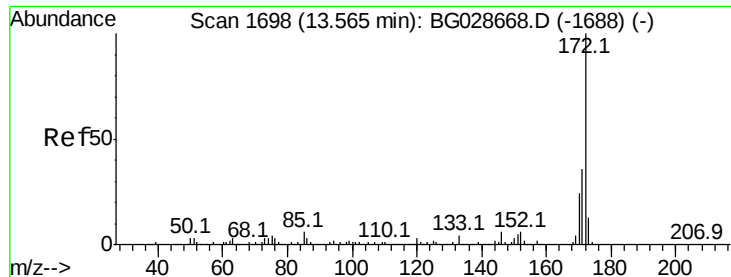


#44
 2-Fluorobiphenyl
 Concen: 100.794 ng
 RT: 13.49 min Scan# 1686
 Delta R.T. -0.07 min
 Lab File: BG028990.D
 Acq: 30 Sep 2017 22:04

Instrument :
 BNA_G
 ClientSampled :

Tot Ion:172 Resp: 726402




Ion	Ratio	Lower	Upper
172	100		
171	35.2	32.2	48.2
170	23.3	21.8	32.6

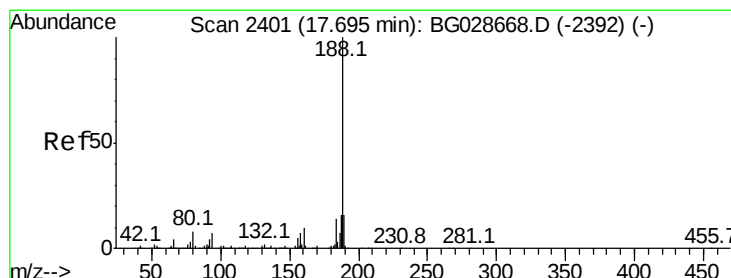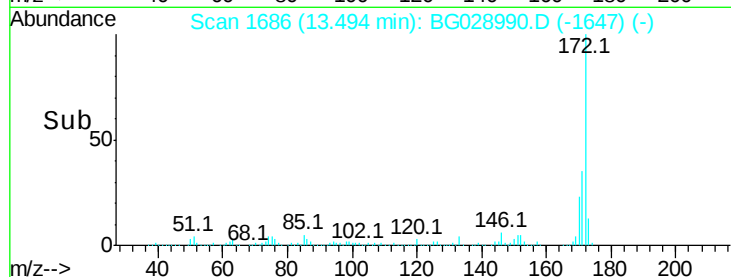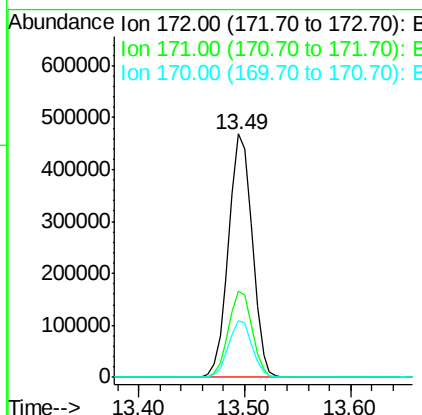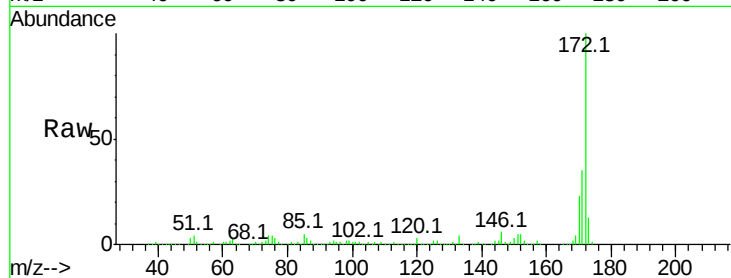

#63
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 17.62 min Scan# 2389
 Delta R.T. -0.07 min
 Lab File: BG028990.D
 Acq: 30 Sep 2017 22:04

Tgt Ion:188 Resp: 277965

Ion	Ratio	Lower	Upper
188	100		
94	6.9	5.8	8.8
80	7.5	7.5	11.3#

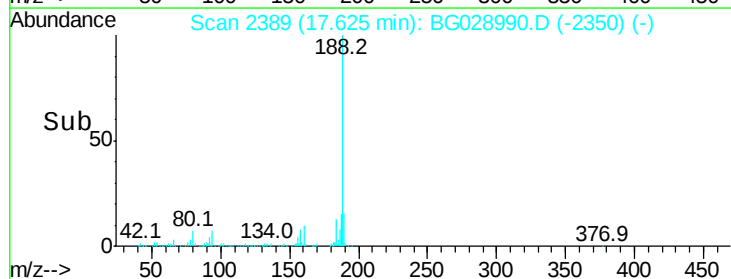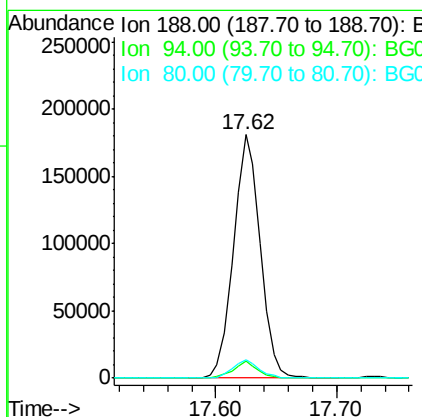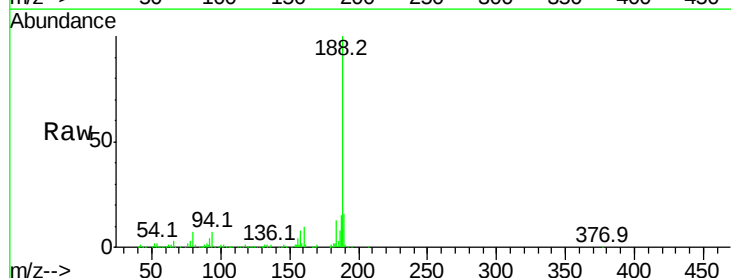



#75

Chrysene-d12

Concen: 20.000 ng

RT: 21.94 min Scan# 3123

Delta R.T. -0.09 min

Lab File: BG028990.D

Acq: 30 Sep 2017 22:04

Instrument :

BNA_G

ClientSampleId :


Tot Ion:240 Resp: 322822

Ion Ratio Lower Upper

240 100

120 5.8 5.7 8.5




236 26.4 22.2 33.4

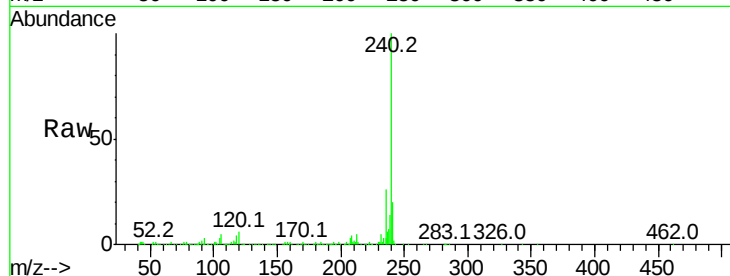

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

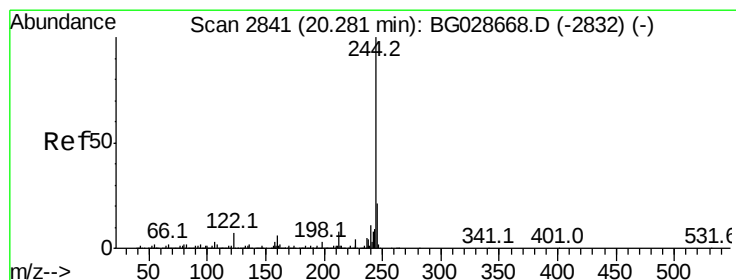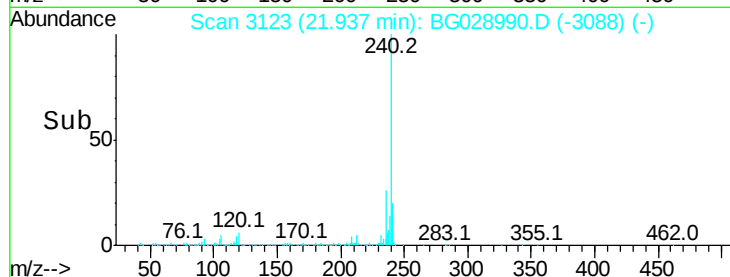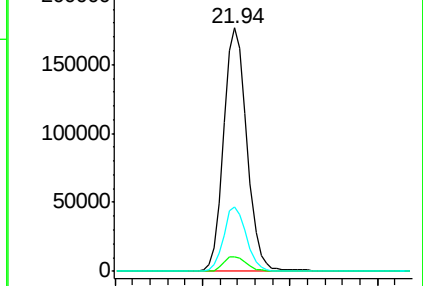

#78

Terphenyl-d14

Concen: 102.211 ng

RT: 20.22 min Scan# 2830

Delta R.T. -0.06 min

Lab File: BG028990.D

Acq: 30 Sep 2017 22:04


Tgt Ion:244 Resp: 1547242

Ion Ratio Lower Upper

244 100

212 8.2 10.0 15.0#



122 7.5 8.6 12.8#



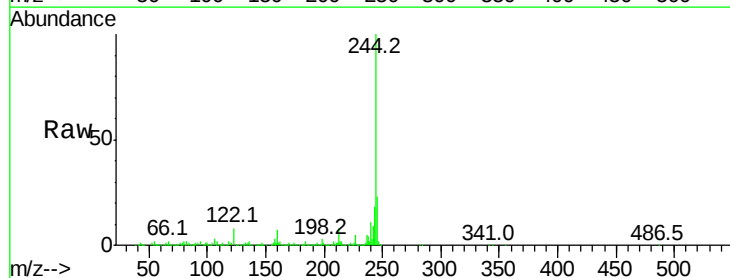


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

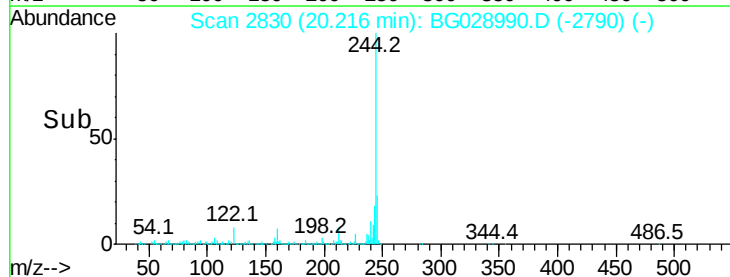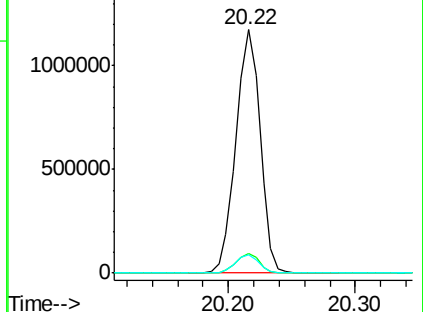

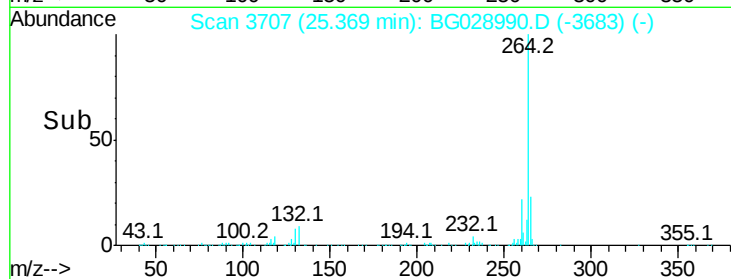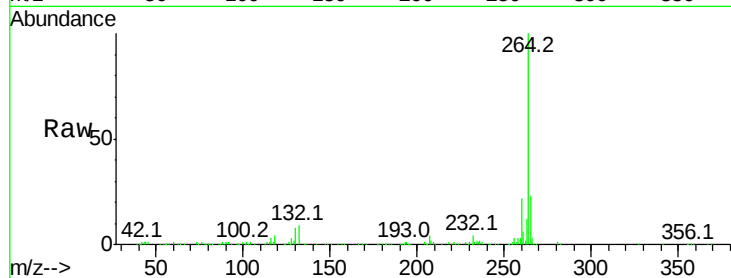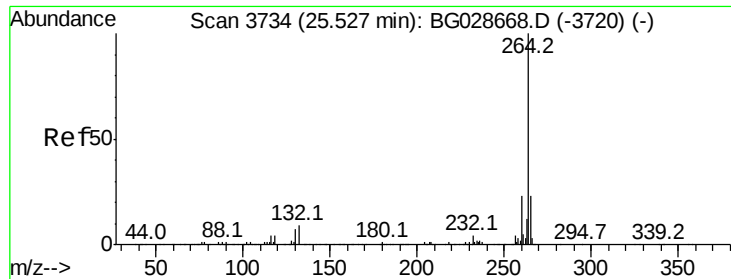

#86
 Pervlene-d12
 Concen: 20.000 ng
 RT: 25.37 min Scan# 3707
 Delta R.T. -0.16 min
 Lab File: BG028990.D
 Acq: 30 Sep 2017 22:04

Instrument :
 BNA_G
 ClientSampleId :

Tot Ion:	264	Resp:	340025
Ion	Ratio	Lower	Upper
264	100		
260	22.3	21.8	32.8
265	23.0	18.2	27.4

