

Data Path : Z:\HPCHEM1\BNA G\DATA\BG093017\
 Data File : BG028986.D
 Acq On : 30 Sep 2017 19:26
 Operator : SJ/JU
 Sample : PB102778TB
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB102778TB

Quant Time: Oct 01 02:35:51 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG091217.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Oct 01 02:30:17 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.25	152	35367	20.00	ng	0.00
21) Naphthalene-d8	11.08	136	136201	20.00	ng	0.00
38) Acenaphthene-d10	14.88	164	92757	20.00	ng	0.00
63) Phenanthrene-d10	17.63	188	251303	20.00	ng	0.00
75) Chrysene-d12	21.94	240	298174	20.00	ng	-0.01
86) Perylene-d12	25.37	264	312764	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.82	112	317220	148.00	ng	0.00
7) Phenol-d6	7.41	99	412384	127.79	ng	0.00
23) Nitrobenzene-d5	9.42	82	256253	90.00	ng	0.00
41) 2,4,6-Tribromophenol	16.37	330	204946	133.59	ng	0.00
44) 2-Fluorobiphenyl	13.50	172	658929	94.72	ng	0.00
78) Terphenyl-d14	20.22	244	1274055	91.12	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG093017\
Data File : BG028986.D
Acq On : 30 Sep 2017 19:26
Operator : SJ/JU
Sample : PB102778TB
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB102778TB

Quant Time: Oct 01 02:35:51 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG091217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Oct 01 02:30:17 2017
Response via : Initial Calibration

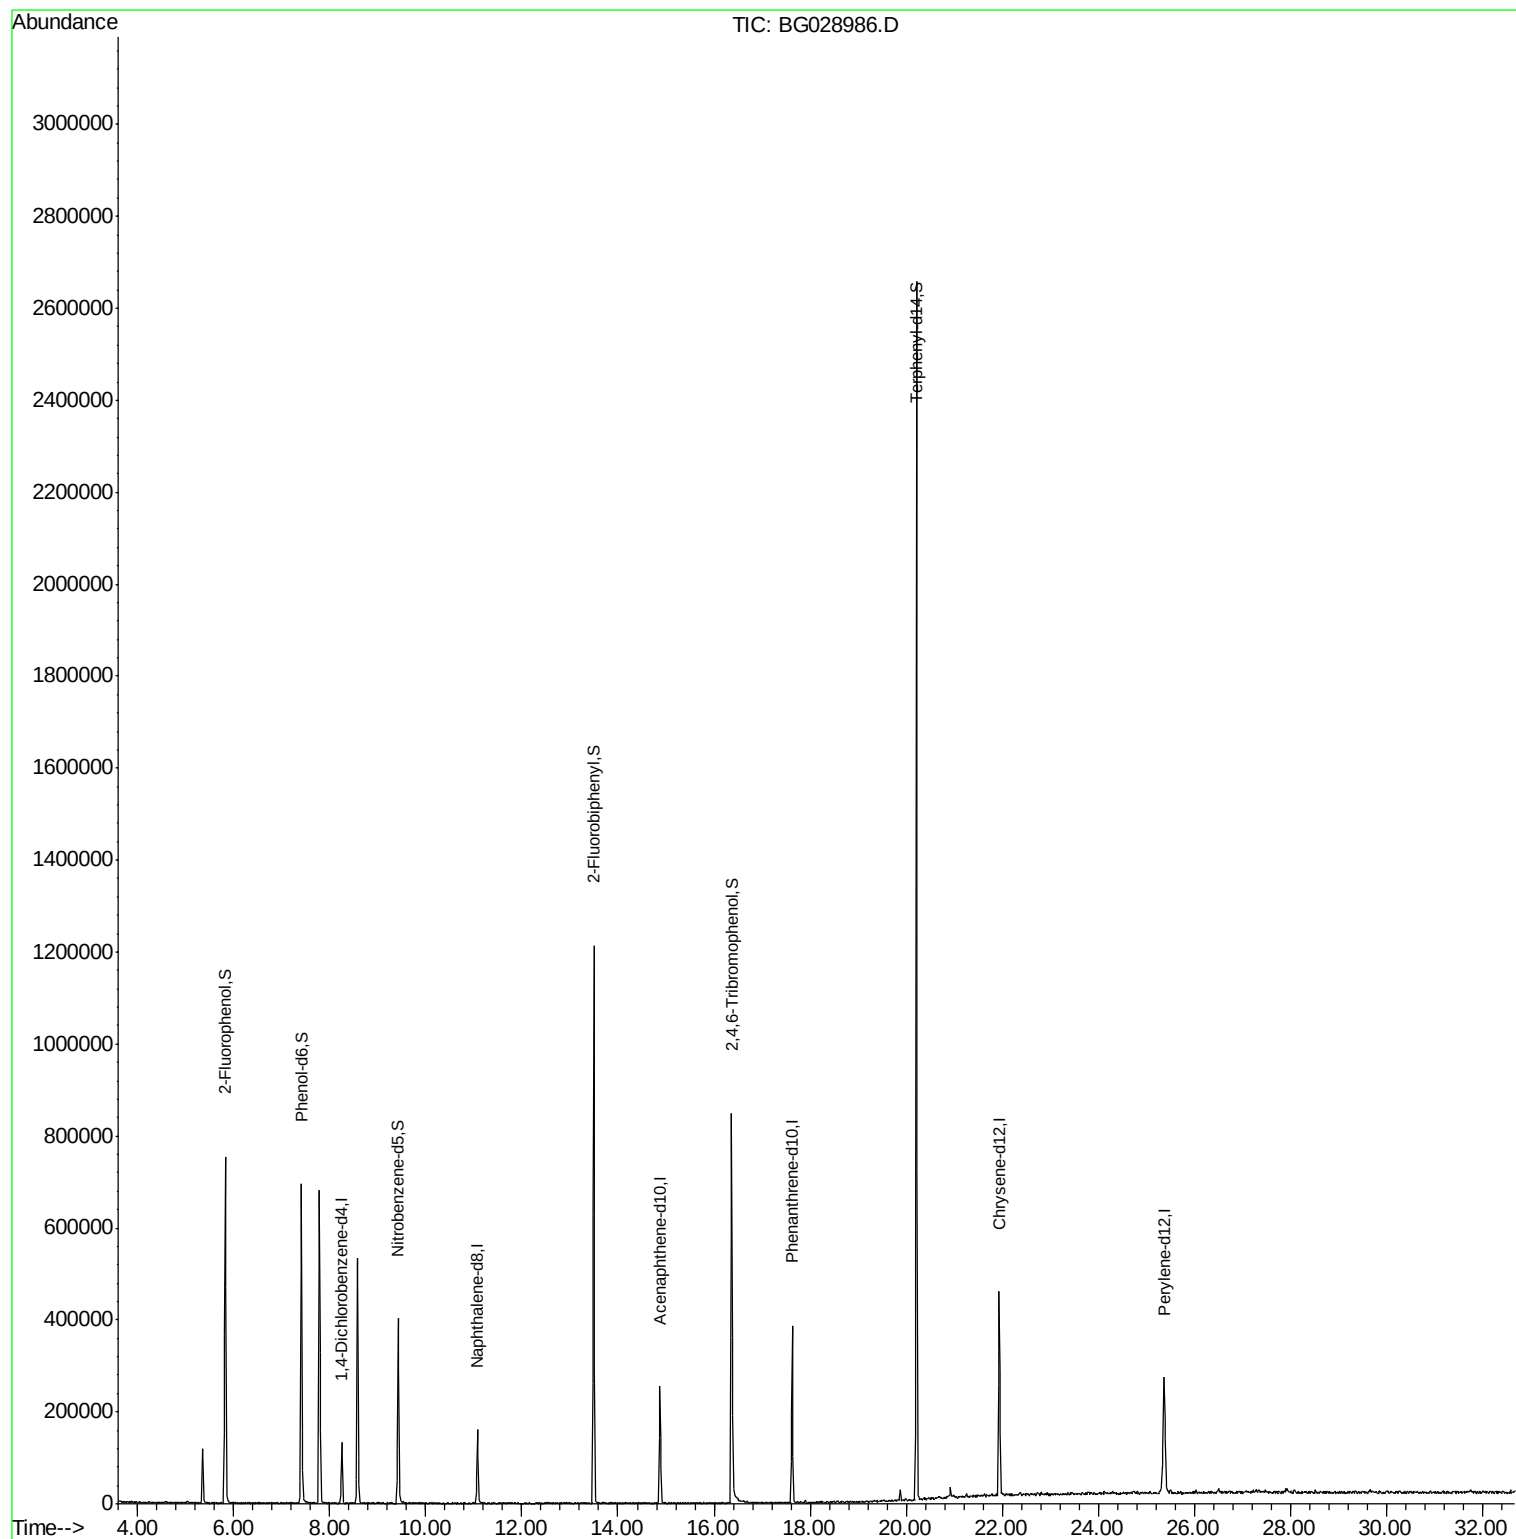




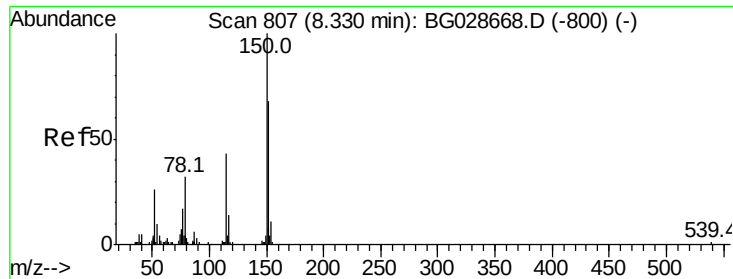


#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.25 min Scan# 793
Delta R.T. -0.01 min
Lab File: BG028986.D
Acq: 30 Sep 2017 19:26

Instrument :
BNA_G
ClientSampleId :
PB102778TB




Tot Ion:152 Resp: 35367
Ion Ratio Lower Upper
152 100
150 164.4 114.0 171.0
115 59.1 48.1 72.1

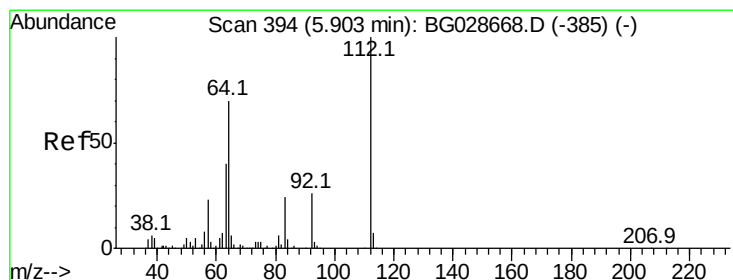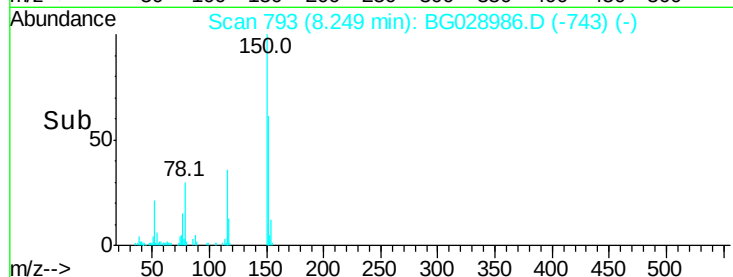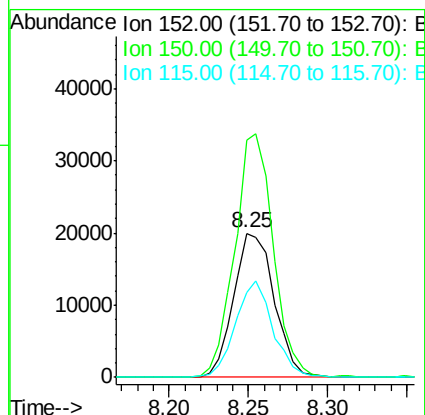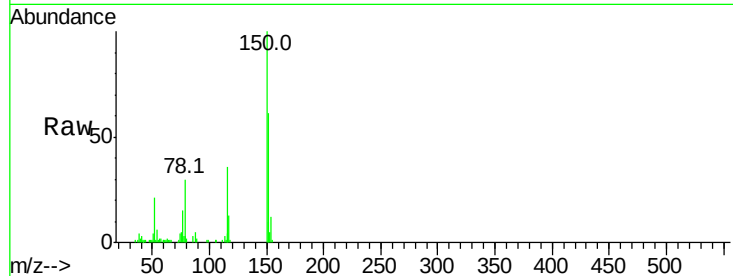


#5

2-Fluorophenol
Concen: 147.999 ng
RT: 5.82 min Scan# 380
Delta R.T. 0.00 min
Lab File: BG028986.D
Acq: 30 Sep 2017 19:26

Tgt Ion:112 Resp: 317220
Ion Ratio Lower Upper
112 100
64 67.5 61.8 92.6
63 38.5 37.2 55.8

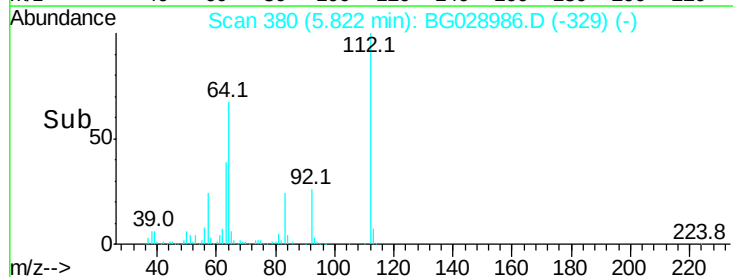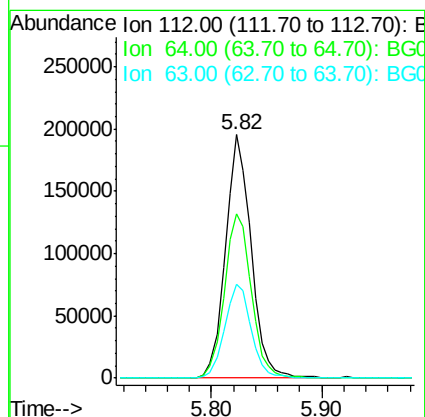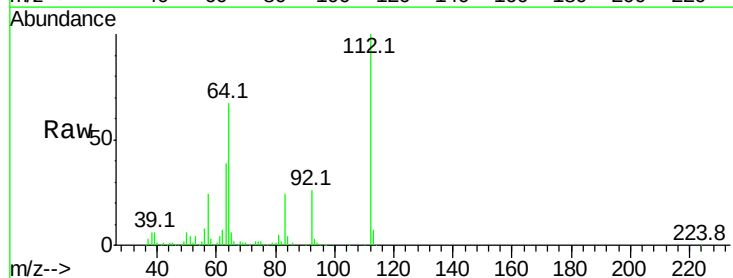

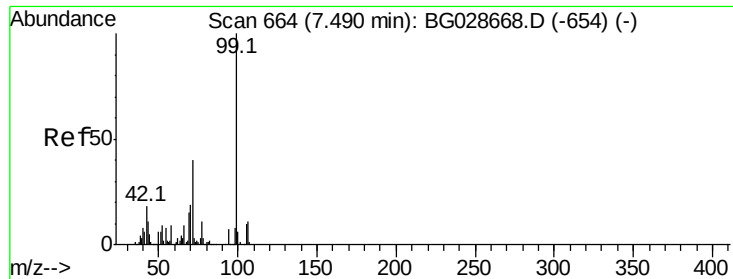

#7

Phenol-d6

Concen: 127.786 ng

RT: 7.41 min Scan# 651

Delta R.T. 0.00 min

Lab File: BG028986.D

Acq: 30 Sep 2017 19:26

Instrument :





BNA_G

ClientSampleId :

PB102778TB

Tot Ion: 99 Resp: 412384

Ion	Ratio	Lower	Upper
99	100		
42	16.8	20.5	30.7#
71	40.6	37.6	56.4

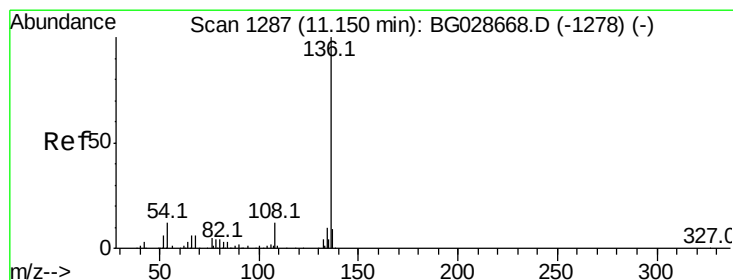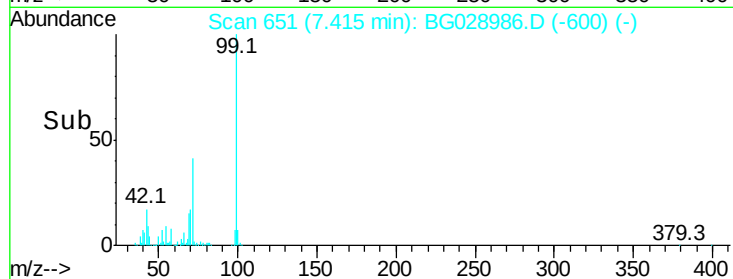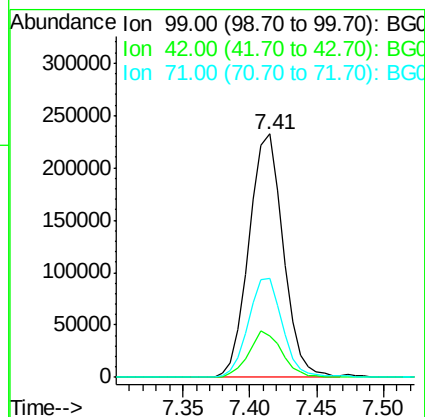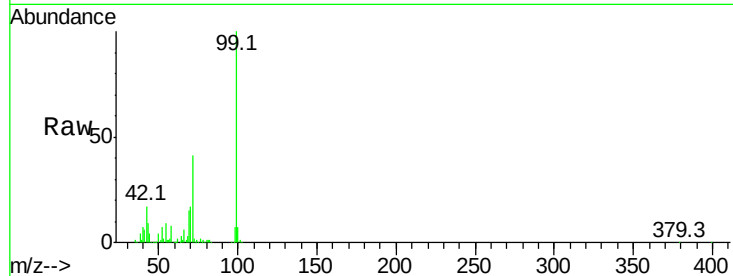

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 11.08 min Scan# 1274




Delta R.T. -0.01 min


Lab File: BG028986.D

Acq: 30 Sep 2017 19:26

Tgt Ion: 136 Resp: 136201

Ion	Ratio	Lower	Upper
136	100		
137	9.7	8.9	13.3
54	13.6	9.3	13.9
68	4.0	5.1	7.7#


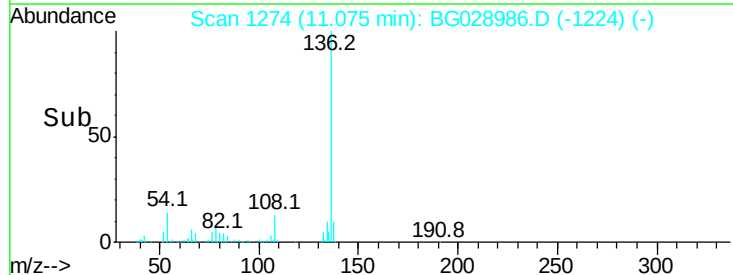
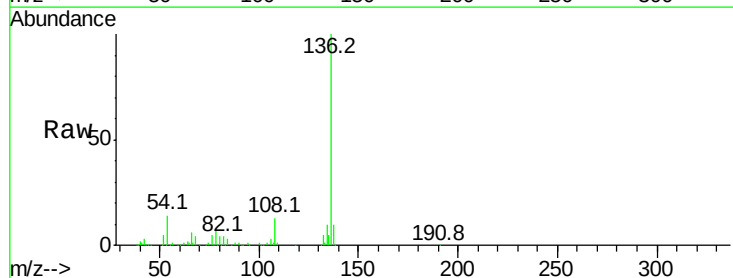
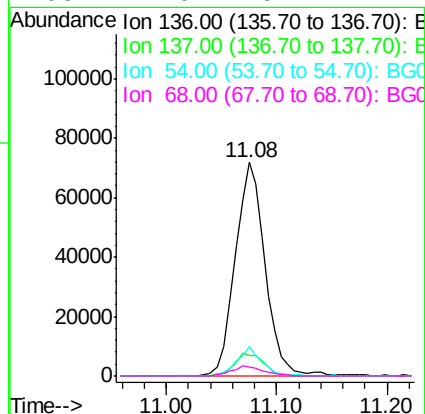


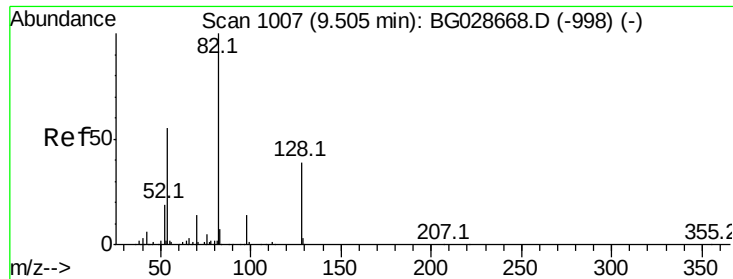

#23
 Nitrobenzene-d5
 Concen: 90.003 ng
 RT: 9.42 min Scan# 993
 Delta R.T. -0.01 min
 Lab File: BG028986.D
 Acq: 30 Sep 2017 19:26




Instrument :
 BNA_G
 ClientSampleId :
 PB102778TB


Tot Ion	82	Resp	256253
Ion	Ratio	Lower	Upper
82	100		
128	41.1	26.4	39.6#
54	58.3	49.4	74.2

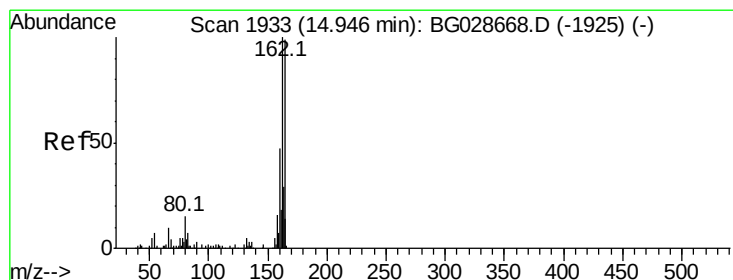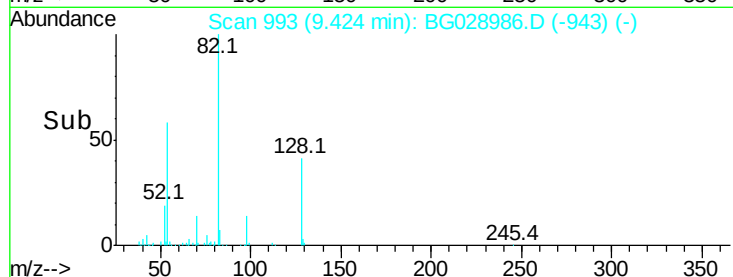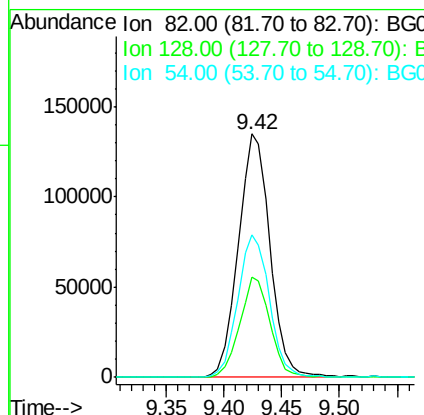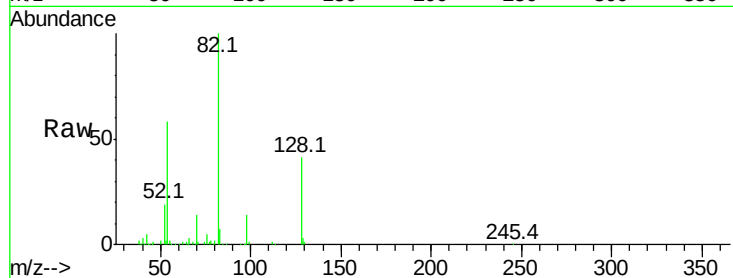

#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.88 min Scan# 1921
 Delta R.T. -0.01 min
 Lab File: BG028986.D
 Acq: 30 Sep 2017 19:26

Tgt Ion	164	Resp	92757
Ion	Ratio	Lower	Upper
164	100		
162	99.0	85.1	127.7
160	49.5	34.7	52.1

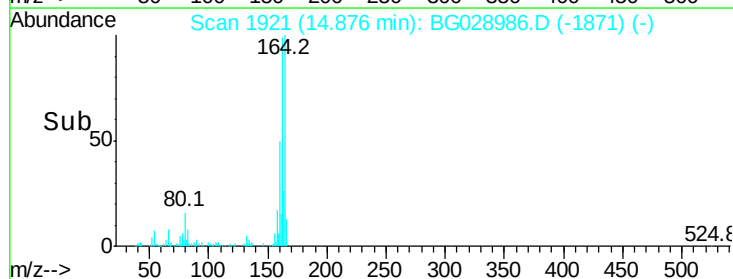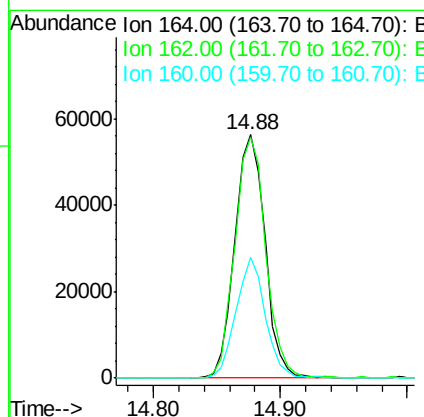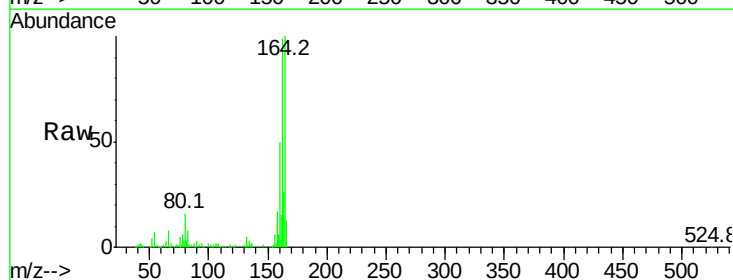


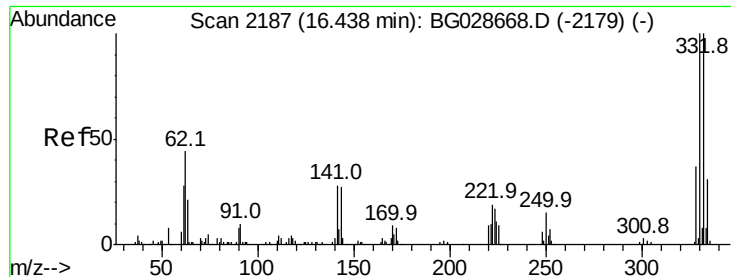

#41
 2,4,6-Tribromophenol
 Concen: 133.590 ng
 RT: 16.37 min Scan# 2175
 Delta R.T. -0.01 min
 Lab File: BG028986.D
 Acq: 30 Sep 2017 19:26

Instrument :
 BNA_G
 ClientSampleId :
 PB102778TB

Tot Ion	Ratio	Lower	Upper
330	100		
332	95.9	77.3	115.9
141	30.5	32.1	48.1#



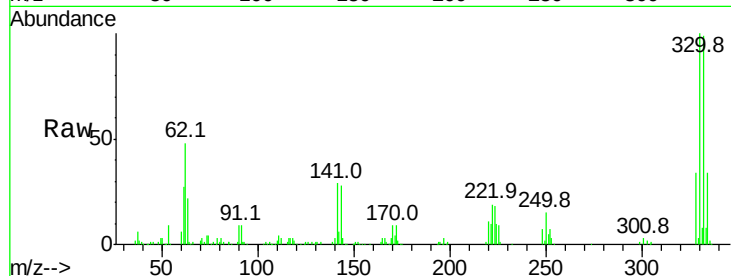


Abundance

Ion 329.80 (329.50 to 330.50): E


Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

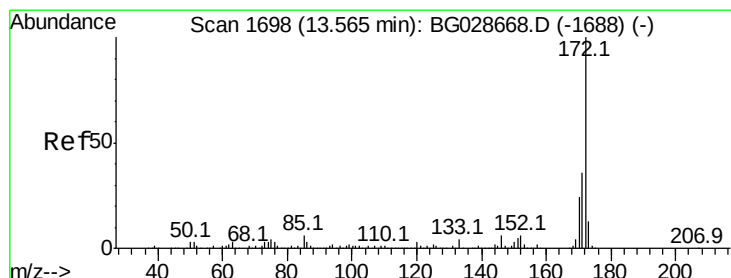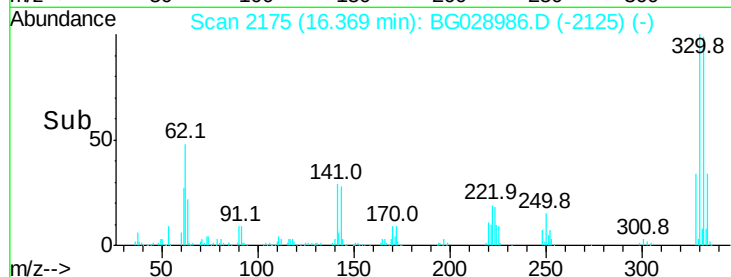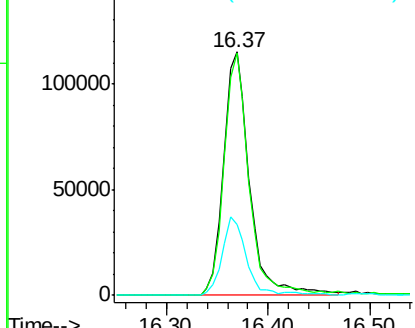

#44
 2-Fluorobiphenyl
 Concen: 94.724 ng
 RT: 13.50 min Scan# 1686
 Delta R.T. -0.01 min
 Lab File: BG028986.D
 Acq: 30 Sep 2017 19:26

Tgt Ion	Ratio	Lower	Upper
172	100		
171	35.4	32.2	48.2
170	22.4	21.8	32.6


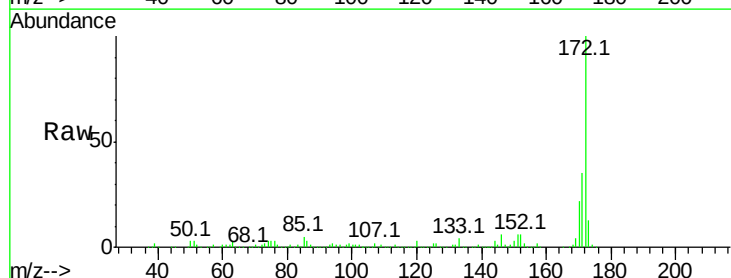



Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

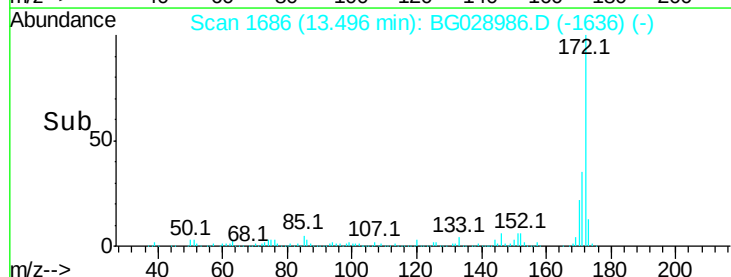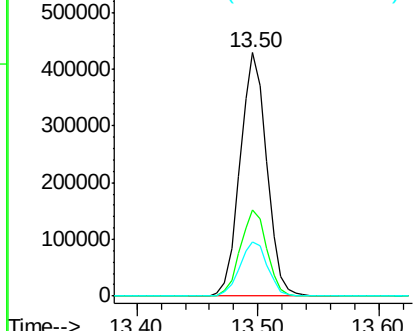

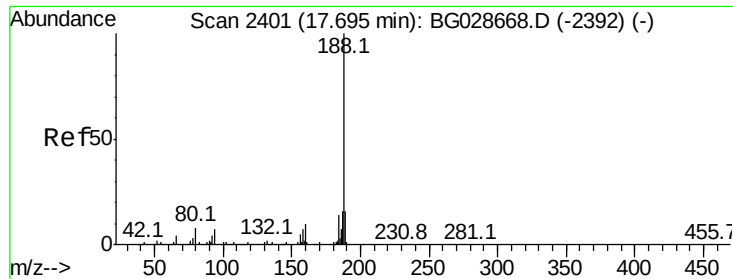

#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.63 min Scan# 2389

Delta R.T. -0.01 min

Lab File: BG028986.D

Acq: 30 Sep 2017 19:26

Instrument :

BNA_G

ClientSampleId :

PB102778TB


Tot Ion:188 Resp: 251303

Ion Ratio Lower Upper

188 100

94 6.6 5.8 8.8




80 7.1 7.5 11.3#

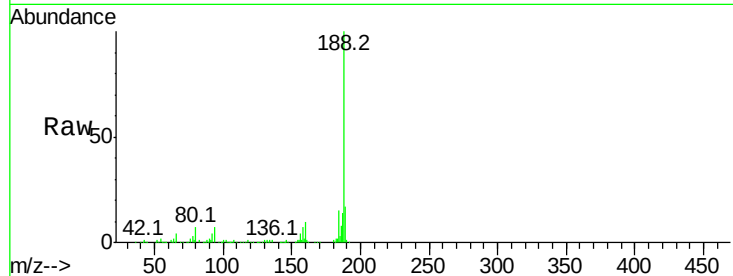

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

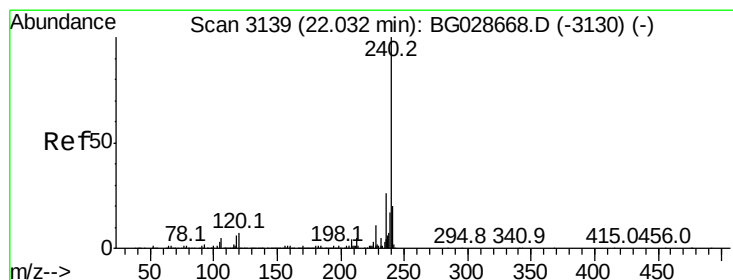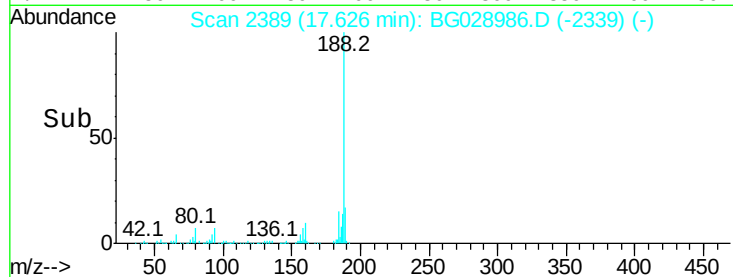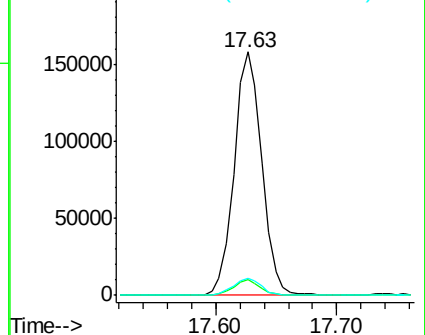

#75

Chrysene-d12

Concen: 20.000 ng

RT: 21.94 min Scan# 3123

Delta R.T. -0.01 min

Lab File: BG028986.D

Acq: 30 Sep 2017 19:26


Tgt Ion:240 Resp: 298174

Ion Ratio Lower Upper

240 100

120 6.0 5.7 8.5



236 25.1 22.2 33.4

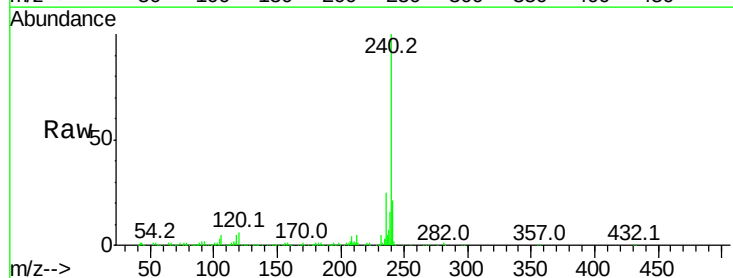


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

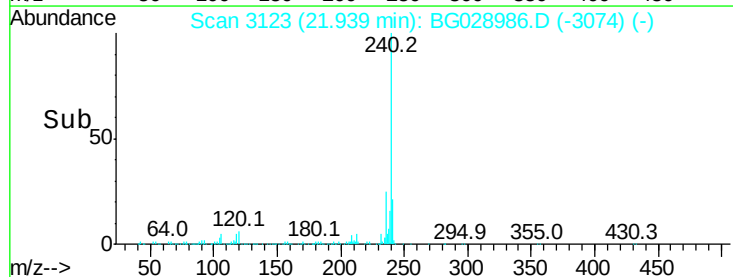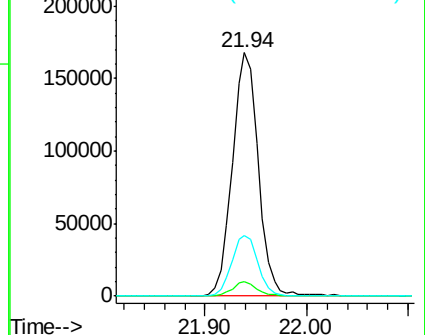

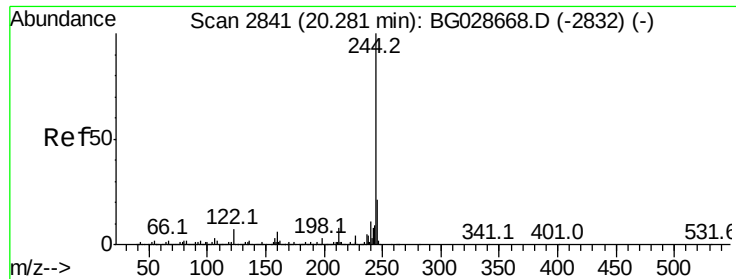

#78

Terphenyl-d14

Concen: 91.121 ng

RT: 20.22 min Scan# 2830

Delta R.T. -0.01 min

Lab File: BG028986.D

Acq: 30 Sep 2017 19:26

Instrument :

BNA_G

ClientSampleId :

PB102778TB


Tot Ion:244 Resp: 1274055

Ion Ratio Lower Upper

244 100

212 7.6 10.0 15.0#




122 7.3 8.6 12.8#

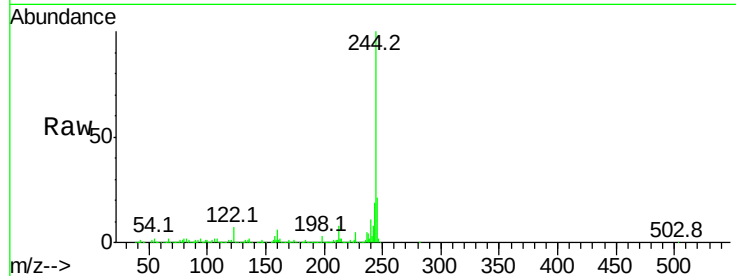

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

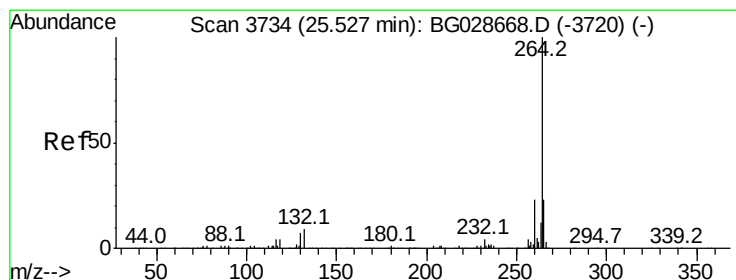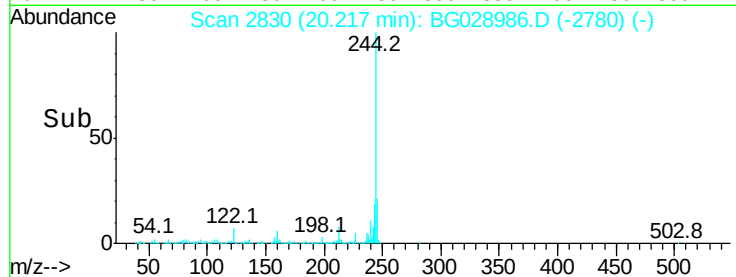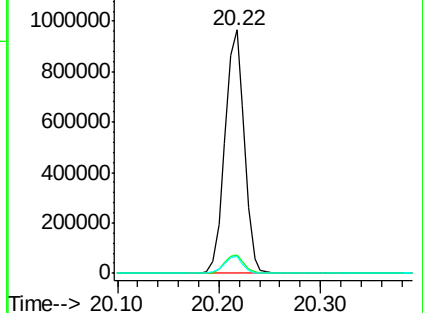

#86

Perylene-d12

Concen: 20.000 ng

RT: 25.37 min Scan# 3707

Delta R.T. -0.01 min

Lab File: BG028986.D

Acq: 30 Sep 2017 19:26


Tgt Ion:264 Resp: 312764

Ion Ratio Lower Upper

264 100

260 22.8 21.8 32.8

265 20.9 18.2 27.4

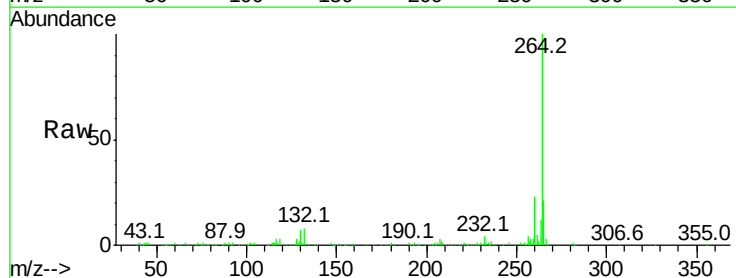

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

