

Data Path : Z:\HPCHEM1\BNA G\DATA\BG093017\
 Data File : BG028994.D
 Acq On : 1 Oct 2017 00:42
 Operator : SJ/JU
 Sample : I5511-03
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EO-01-092817

Quant Time: Oct 01 02:51:45 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG091217.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Oct 01 02:46:32 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.25	152	44800	20.00	ng	0.00
21) Naphthalene-d8	11.07	136	173751	20.00	ng	0.00
38) Acenaphthene-d10	14.88	164	115340	20.00	ng	0.00
63) Phenanthrene-d10	17.63	188	306760	20.00	ng	0.00
75) Chrysene-d12	21.94	240	356691	20.00	ng	-0.01
86) Perylene-d12	25.36	264	355794	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.83	112	389971	143.63	ng	0.00
7) Phenol-d6	7.41	99	486312	118.96	ng	0.00
23) Nitrobenzene-d5	9.42	82	351079	96.66	ng	0.00
41) 2,4,6-Tribromophenol	16.37	330	304010	159.36	ng	0.00
44) 2-Fluorobiphenyl	13.49	172	858527	99.25	ng	0.00
78) Terphenyl-d14	20.22	244	1581080	94.53	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG093017\
Data File : BG028994.D
Acq On : 1 Oct 2017 00:42
Operator : SJ/JU
Sample : I5511-03
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EO-01-092817

Quant Time: Oct 01 02:51:45 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG091217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Oct 01 02:46:32 2017
Response via : Initial Calibration

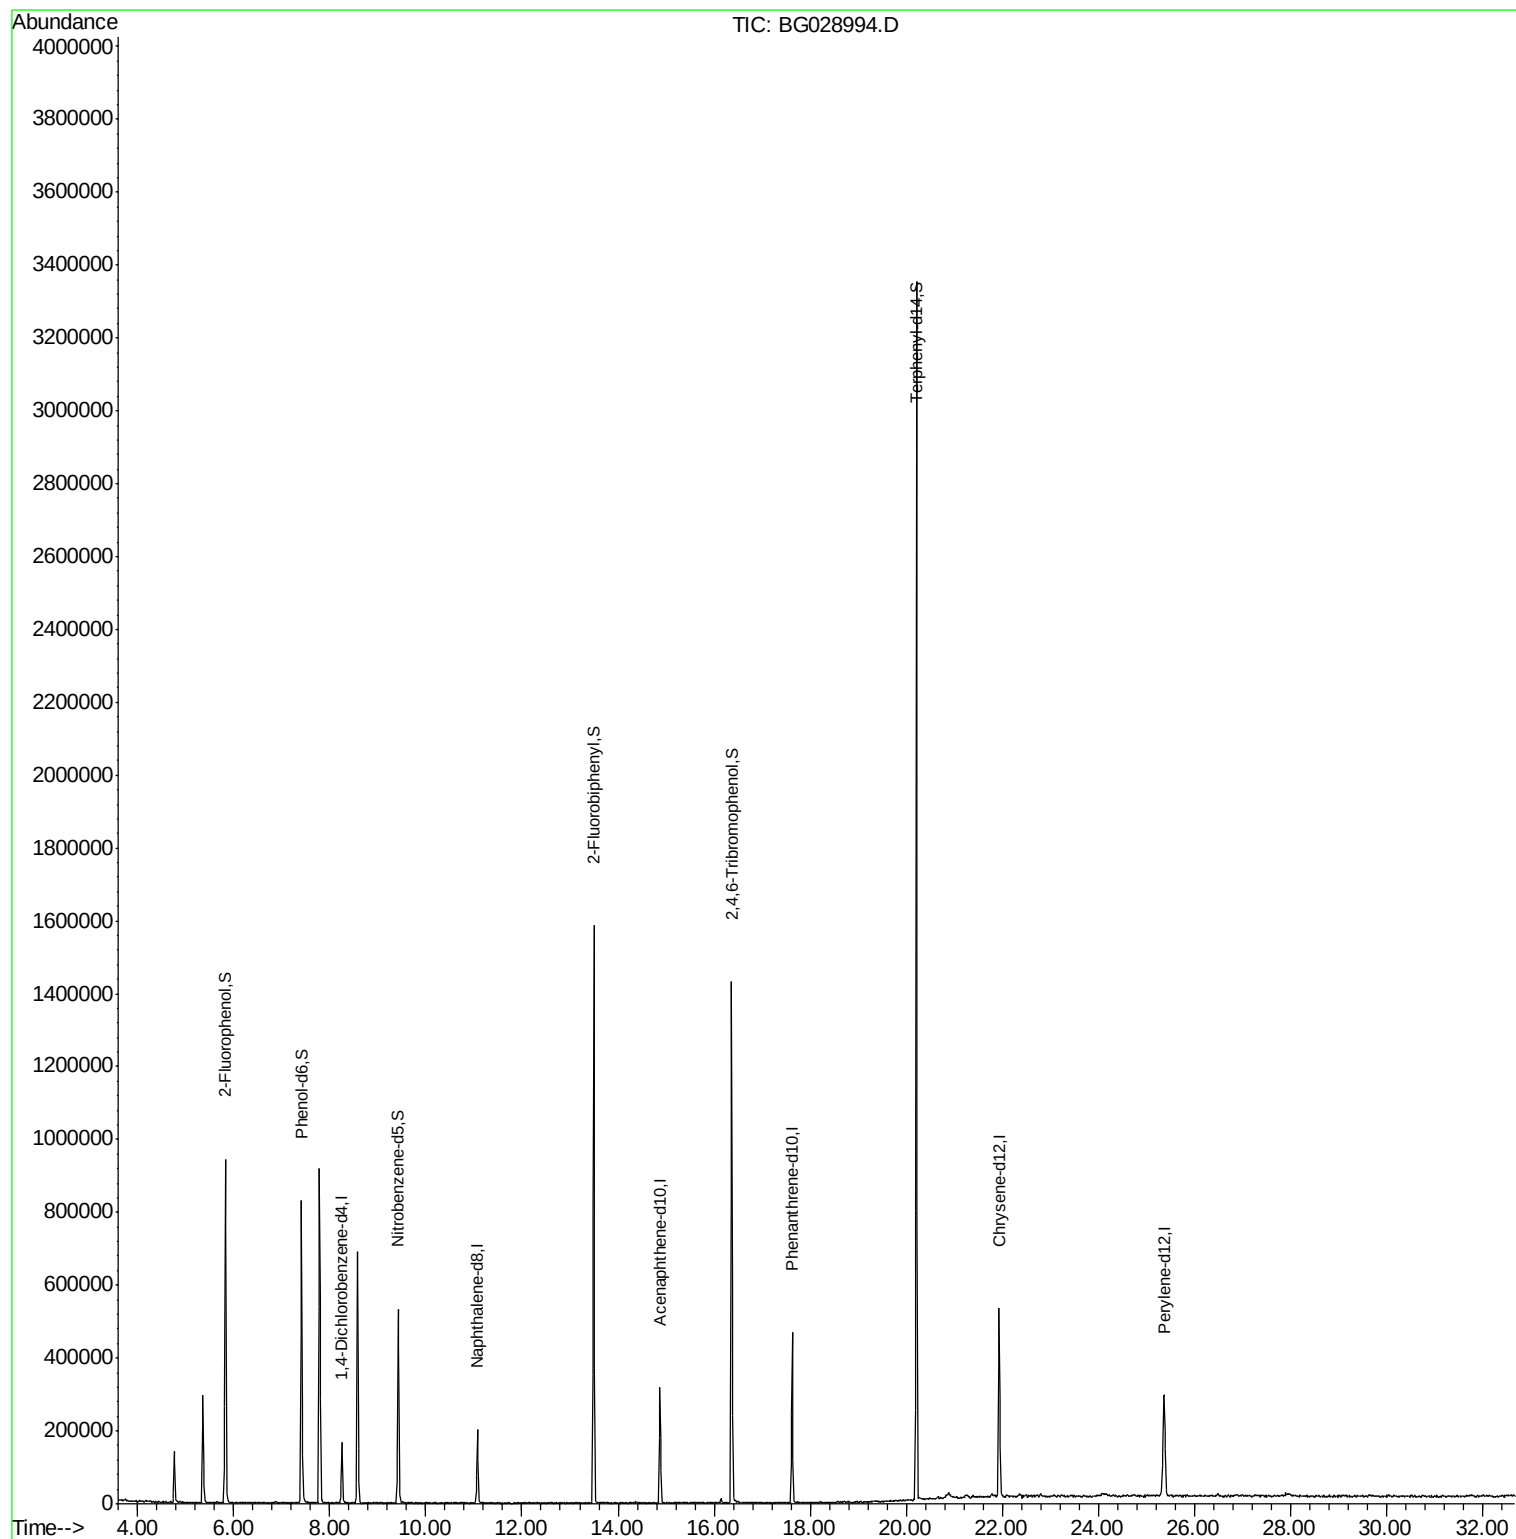







#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.25 min Scan# 794
Delta R.T. -0.00 min
Lab File: BG028994.D
Acq: 1 Oct 2017 00:42

Instrument :
BNA_G
ClientSampleId :
EO-01-092817




Tot Ion:152 Resp: 44800
Ion Ratio Lower Upper
152 100
150 163.1 114.0 171.0
115 65.3 48.1 72.1

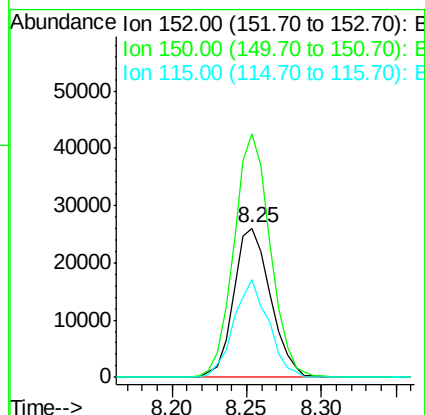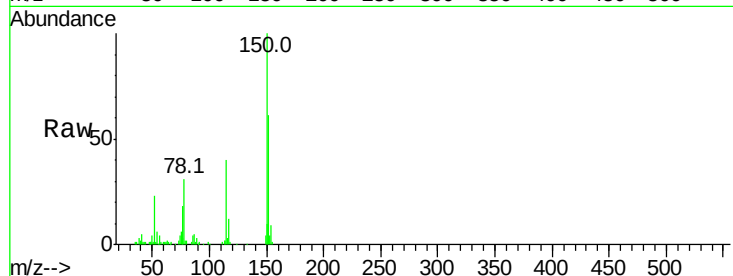


#5

2-Fluorophenol
Concen: 143.632 ng
RT: 5.83 min Scan# 381
Delta R.T. 0.01 min
Lab File: BG028994.D
Acq: 1 Oct 2017 00:42

Tgt Ion:112 Resp: 389971
Ion Ratio Lower Upper
112 100
64 68.6 61.8 92.6
63 37.0 37.2 55.8#

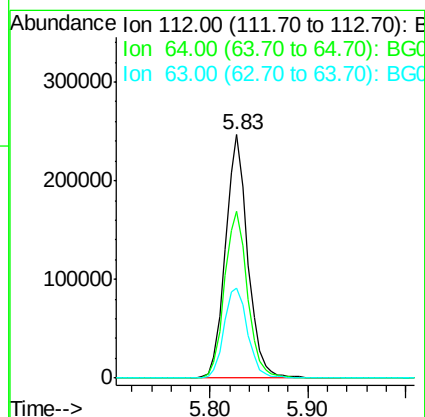

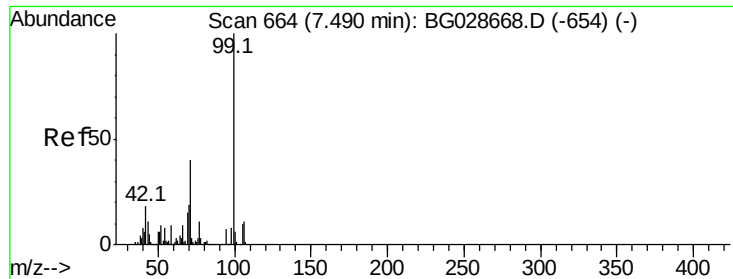

#7

Phenol-d6

Concen: 118.965 ng

RT: 7.41 min Scan# 651

Delta R.T. -0.00 min

Lab File: BG028994.D

Acq: 1 Oct 2017 00:42

Instrument :

BNA_G

ClientSampleId :

EO-01-092817





Tot Ion: 99 Resp: 486312

Ion Ratio Lower Upper

99 100

42 18.7 20.5 30.7#

71 40.3 37.6 56.4

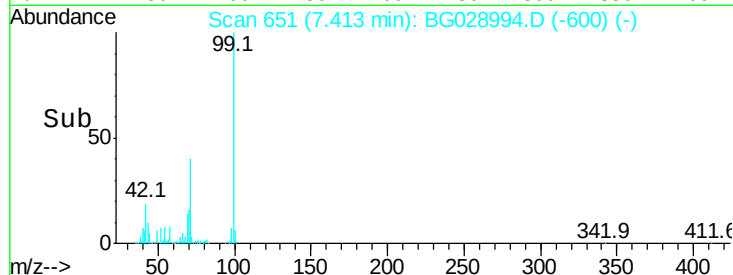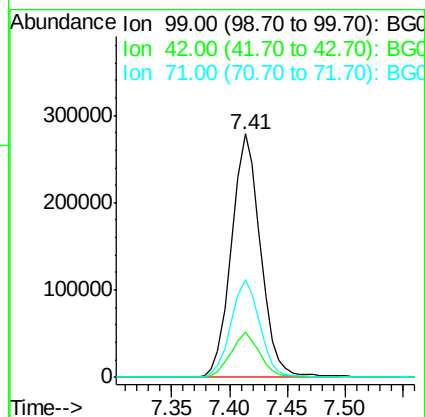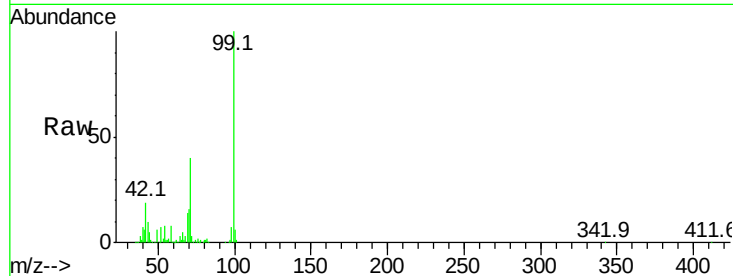

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 11.07 min Scan# 1274

Delta R.T. -0.01 min

Lab File: BG028994.D

Acq: 1 Oct 2017 00:42

Tgt Ion: 136 Resp: 173751




Ion Ratio Lower Upper


136 100

137 9.7 8.9 13.3

54 9.7 9.3 13.9

68 3.2 5.1 7.7#



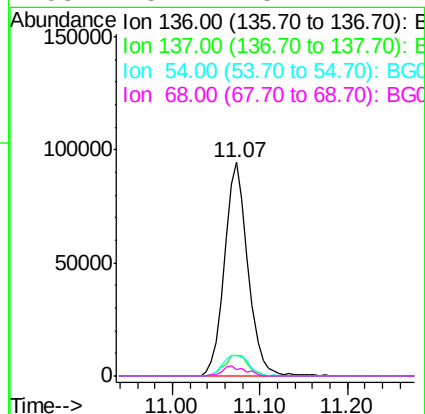





#23
 Nitrobenzene-d5
 Concen: 96.660 ng
 RT: 9.42 min Scan# 993
 Delta R.T. -0.01 min
 Lab File: BG028994.D
 Acq: 1 Oct 2017 00:42




Instrument :
 BNA_G
 ClientSampleId :
 EO-01-092817


Tot Ion	82	Resp	351079
Ion Ratio	Lower	Upper	
82	100		
128	36.1	26.4	39.6
54	56.0	49.4	74.2

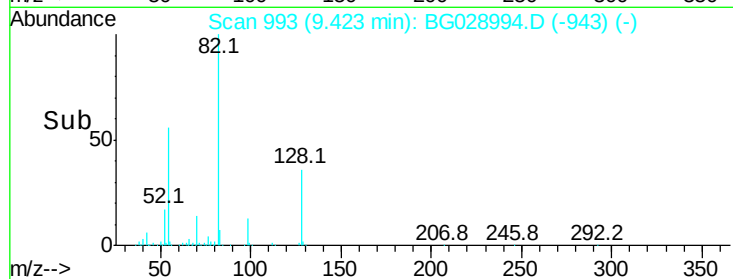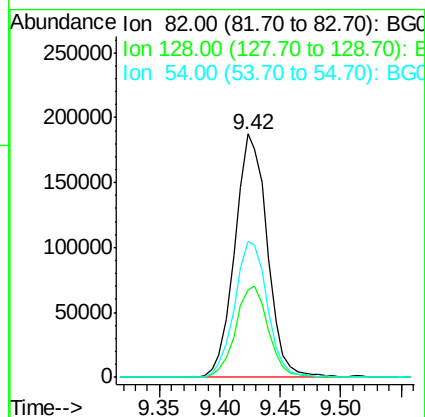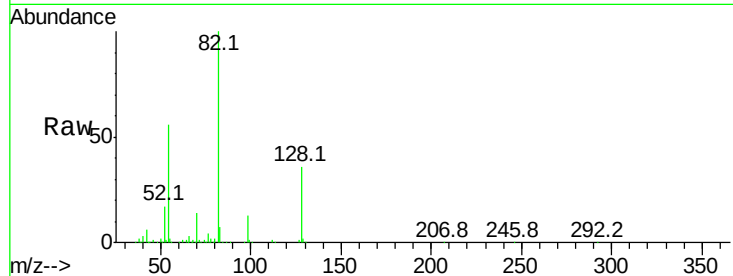

#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.88 min Scan# 1921
 Delta R.T. -0.01 min
 Lab File: BG028994.D
 Acq: 1 Oct 2017 00:42

Tgt Ion	164	Resp	115340
Ion Ratio	Lower	Upper	
164	100		
162	93.3	85.1	127.7
160	42.0	34.7	52.1

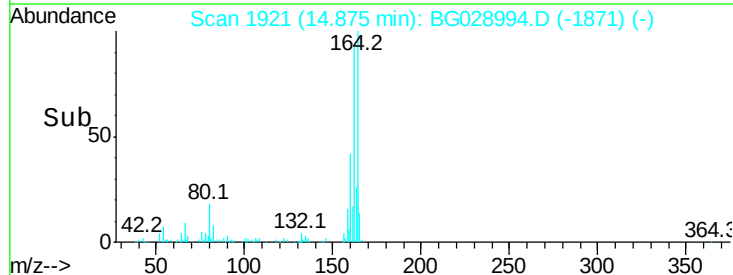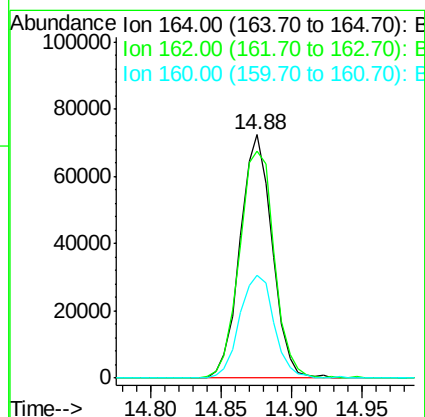

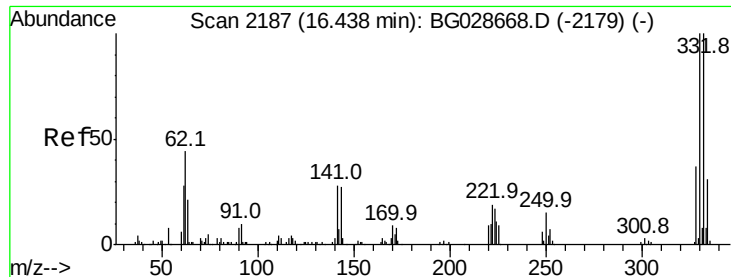

#41

2,4,6-Tribromophenol

Concen: 159.363 ng

RT: 16.37 min Scan# 2175

Delta R.T. -0.01 min

Lab File: BG028994.D

Acq: 1 Oct 2017 00:42

Instrument :

BNA_G

ClientSampleId :

EO-01-092817


Tot Ion:330 Resp: 304010

Ion Ratio Lower Upper

330 100

332 96.3 77.3 115.9




141 29.6 32.1 48.1#

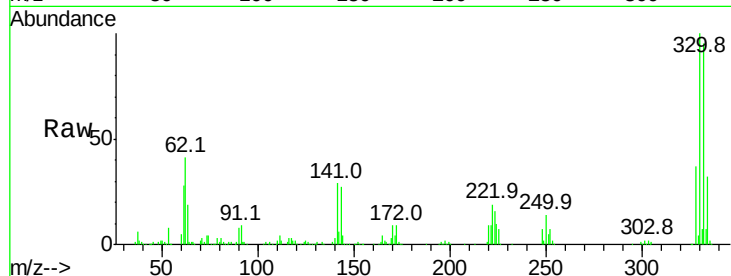

Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

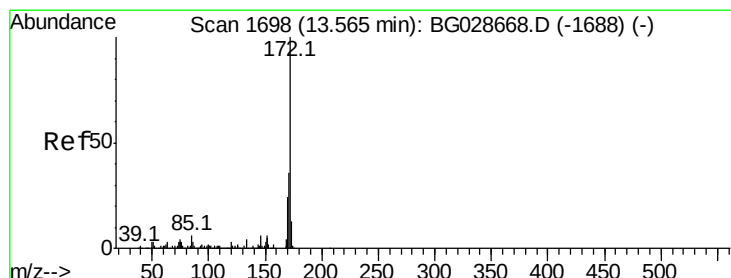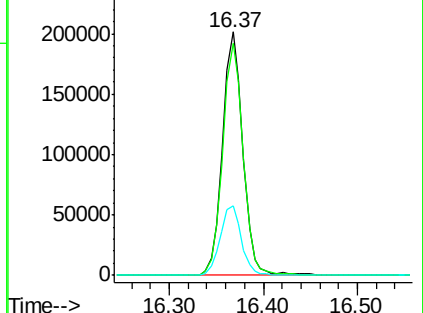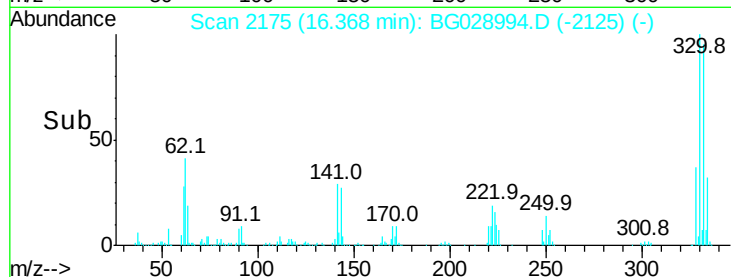

#44

2-Fluorobiphenyl

Concen: 99.253 ng

RT: 13.49 min Scan# 1686

Delta R.T. -0.01 min

Lab File: BG028994.D

Acq: 1 Oct 2017 00:42


Tgt Ion:172 Resp: 858527

Ion Ratio Lower Upper

172 100

171 35.7 32.2 48.2



170 22.3 21.8 32.6

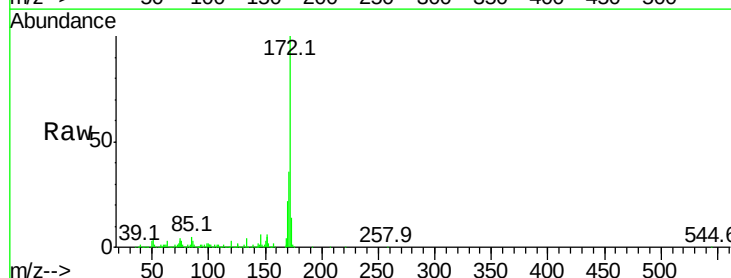


Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

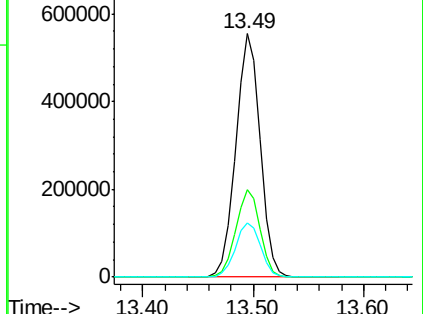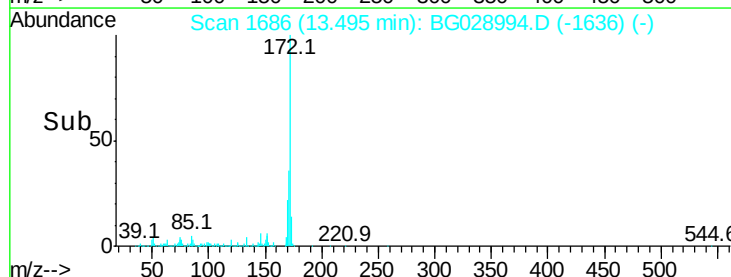



#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.63 min Scan# 2389

Delta R.T. -0.01 min

Lab File: BG028994.D

Acq: 1 Oct 2017 00:42

Instrument :

BNA_G

ClientSampled :

EO-01-092817


Tot Ion:188 Resp: 306760

Ion Ratio Lower Upper

188 100

94 6.2 5.8 8.8




80 7.0 7.5 11.3#

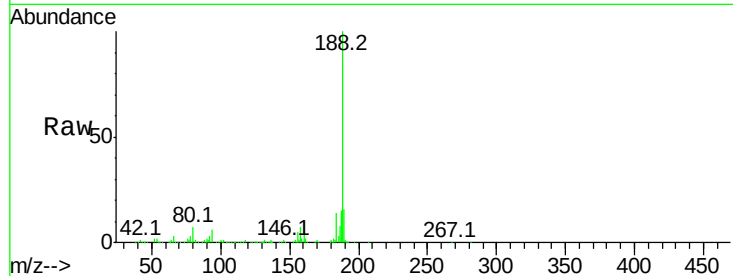

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

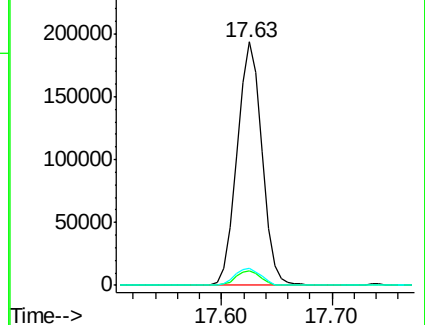

#75

Chrysene-d12

Concen: 20.000 ng

RT: 21.94 min Scan# 3123

Delta R.T. -0.01 min

Lab File: BG028994.D

Acq: 1 Oct 2017 00:42


Tgt Ion:240 Resp: 356691

Ion Ratio Lower Upper

240 100

120 6.1 5.7 8.5



236 26.3 22.2 33.4

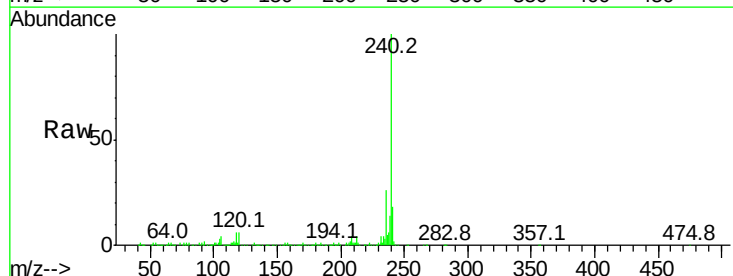


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

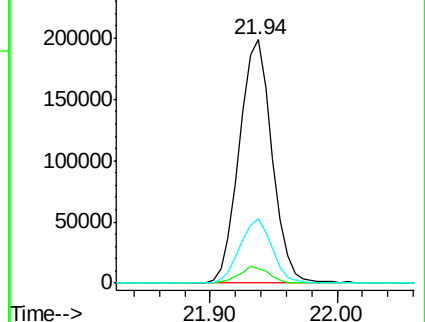



#78

Terphenyl-d14

Concen: 94.529 ng

RT: 20.22 min Scan# 2830

Delta R.T. -0.01 min

Lab File: BG028994.D

Acq: 1 Oct 2017 00:42

Instrument :


BNA_G

ClientSampleId :

EO-01-092817

Tot Ion:244 Resp: 1581080

Ion	Ratio	Lower	Upper
244	100		
212	8.0	10.0	15.0#
122	7.4	8.6	12.8#






Abundance

Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

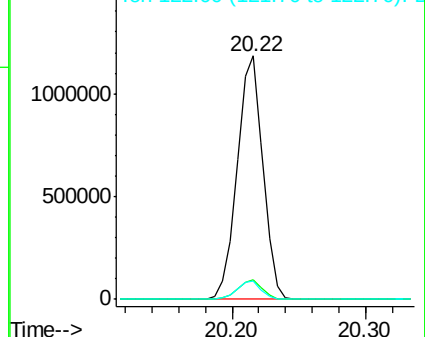

#86

Perylene-d12

Concen: 20.000 ng

RT: 25.36 min Scan# 3706


Delta R.T. -0.01 min

Lab File: BG028994.D

Acq: 1 Oct 2017 00:42

Tgt Ion:264 Resp: 355794

Ion	Ratio	Lower	Upper
264	100		
260	22.4	21.8	32.8
265	20.5	18.2	27.4



Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

