


Data Path : Z:\HPCHEM1\BNA G\Data\BG093017\
 Data File : BG028982.D
 Acq On : 30 Sep 2017 16:47
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG091217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 12 16:57:11 2017

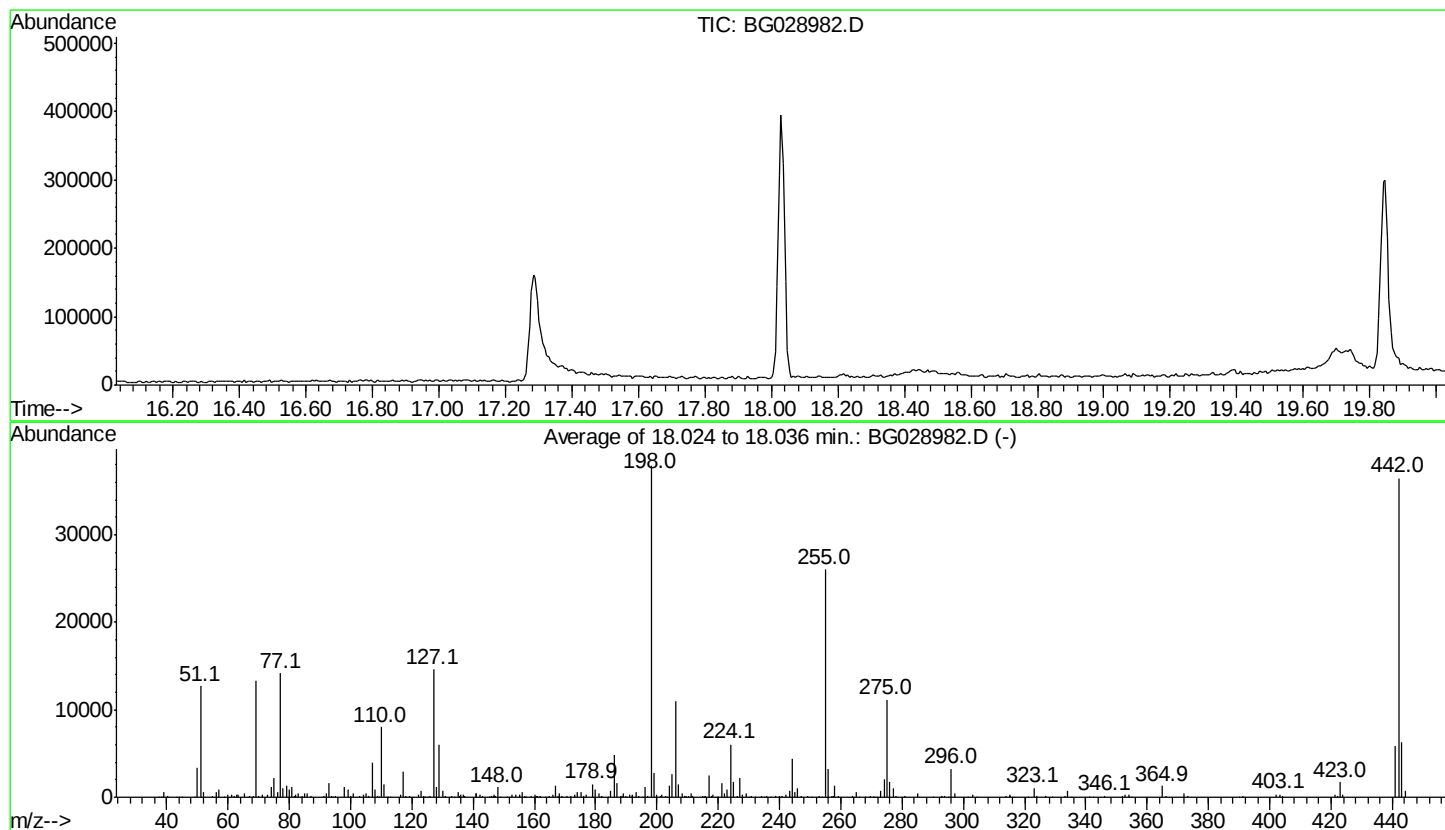

AutoFind: Scans 2457, 2458, 2459; Background Corrected with Scan 2448

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.5	12680	PASS
68	69	0.00	2	1.6	207	PASS
69	198	0.00	100	35.0	13253	PASS
70	69	0.00	2	1.1	144	PASS
127	198	10	80	38.5	14591	PASS
197	198	0.00	2	0.6	217	PASS
198	198	100	100	100.0	37885	PASS
199	198	5	9	7.4	2788	PASS
275	198	10	60	29.4	11133	PASS
365	198	1	100	3.4	1305	PASS
441	442	0.01	24	16.0	5847	PASS
442	198	50	100	96.3	36485	PASS
443	442	15	24	17.4	6346	PASS