

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG093021\
 Data File : BG050338.D
 Acq On : 1 Oct 2021 1:24
 Operator : CG/JU
 Sample : M3777-17
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AG2

Quant Time: Oct 01 04:10:36 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG093021.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 30 16:27:24 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.276	152	41330	20.000	ng/ul	0.00
20) Naphthalene-d8	11.096	136	164708	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.892	164	112840	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.630	188	279084	20.000	ng/ul	0.00
79) Chrysene-d12	21.936	240	279683	20.000	ng/ul	-0.01
88) Perylene-d12	25.362	264	273197	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.634	96	5264	4.679	ng/uL	0.00
4) Pyridine-d5	4.063	84	33133	9.884	ng/ul	0.00
7) Phenol-d5	7.400	99	12203	3.379	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.583	67	68176	29.999	ng/ul	0.00
11) 2-Chlorophenol-d4	7.794	132	29483	11.653	ng/ul	0.00
15) 4-Methylphenol-d8	8.957	113	26218	9.593	ng/ul	0.00
21) Nitrobenzene-d5	9.439	128	38117	33.081	ng/ul	0.00
24) 2-Nitrophenol-d4	10.168	143	19377	15.669	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.702	165	36210	14.828	ng/ul	0.00
31) 4-Chloroaniline-d4	11.225	131	81667	23.411	ng/ul	0.00
46) Dimethylphthalate-d6	14.281	166	252475	32.693	ng/ul	-0.01
49) Acenaphthylene-d8	14.586	160	309206	31.883	ng/ul	0.00
54) 4-Nitrophenol-d4	15.044	143	4831	3.248	ng/ul	-0.01
60) Fluorene-d10	15.879	176	238757	34.316	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.979	200	19378	13.921	ng/ul	0.00
73) Anthracene-d10	17.729	188	429811	36.455	ng/ul	0.00
81) Pyrene-d10	20.003	212	536619	36.083	ng/ul	0.00
92) Benzo(a)pyrene-d12	25.127	264	473520	34.470	ng/ul	-0.01
Target Compounds						Qvalue
8) Phenol	7.430	94	4798	1.296	ng/ul	92
86) Bis(2-ethylhexyl)phtha...	21.801	149	11537	1.183	ng/ul#	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG093021\
Data File : BG050338.D
Acq On : 1 Oct 2021 1:24
Operator : CG/JU
Sample : M3777-17
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AG2

Quant Time: Oct 01 04:10:36 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG093021.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Sep 30 16:27:24 2021
Response via : Initial Calibration




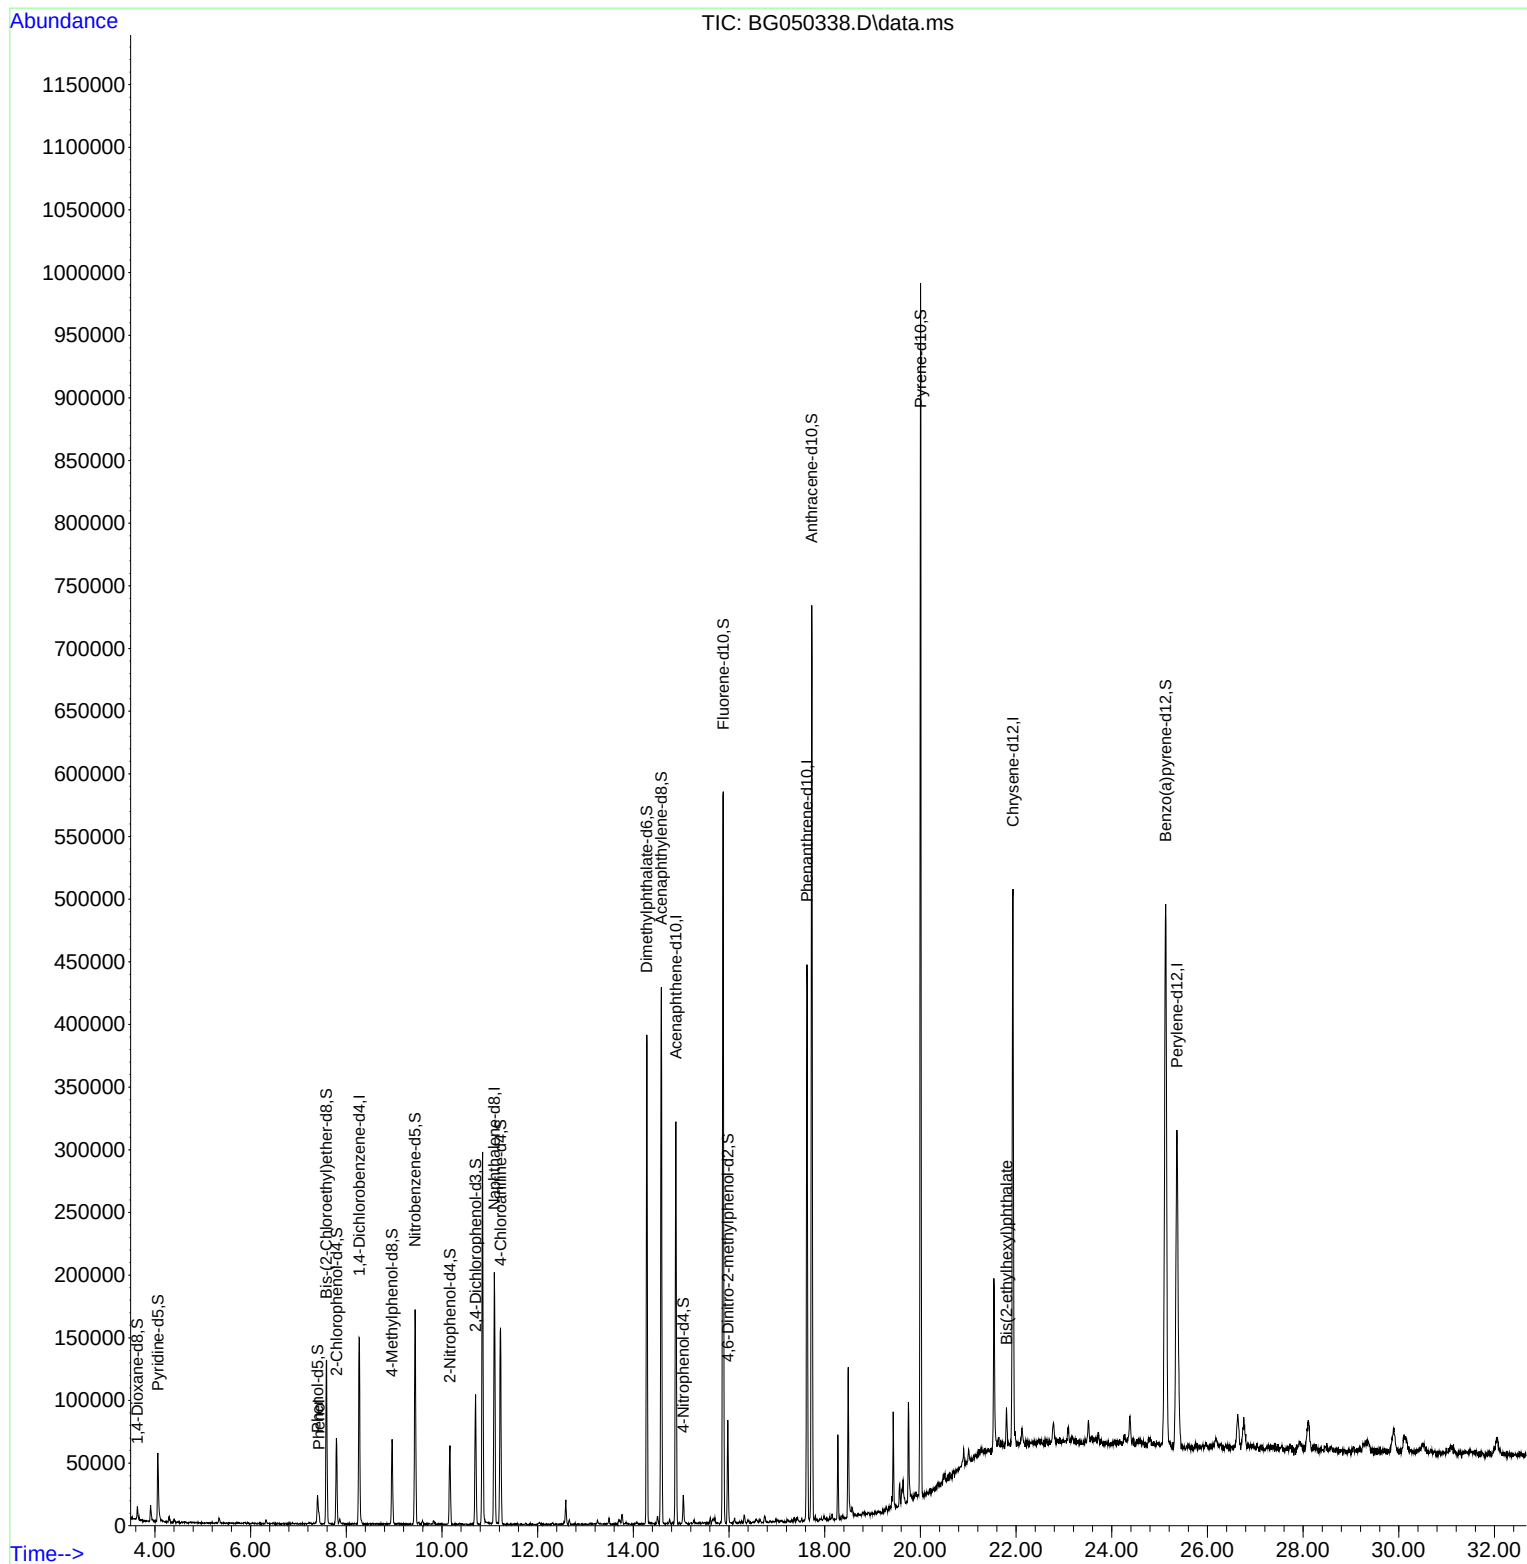


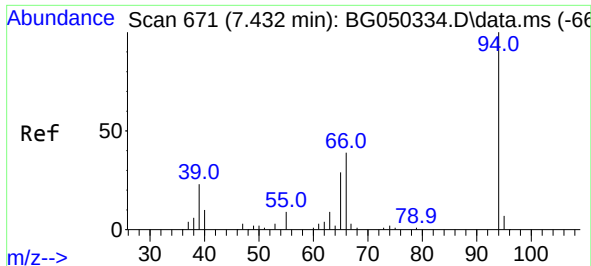

#8
Phenol
Concen: 1.296 ng/ul
RT: 7.430 min Scan# 671
Delta R.T. -0.006 min
Lab File: BG050338.D
Acq: 1 Oct 2021 1:24

Instrument :
BNA_G
ClientSampled :
C0AG2

Tgt Ion: 94 Resp: 4798
Ion Ratio Lower Upper
94 100
65 33.7 25.3 37.9
66 36.3 34.9 52.3

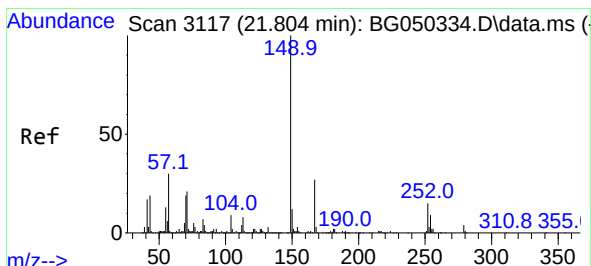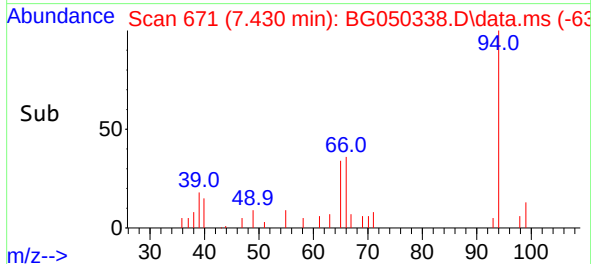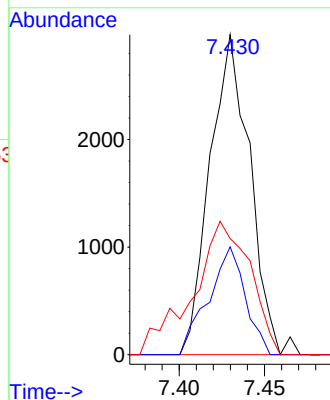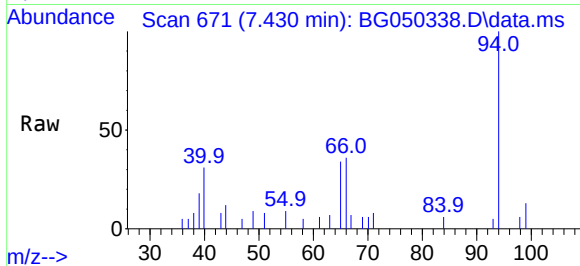

#86
Bis(2-ethylhexyl)phthalate
Concen: 1.183 ng/ul
RT: 21.801 min Scan# 3117
Delta R.T. -0.006 min
Lab File: BG050338.D
Acq: 1 Oct 2021 1:24

Tgt Ion:149 Resp: 11537
Ion Ratio Lower Upper
149 100
167 22.1 21.3 31.9
279 5.3 2.8 4.2#

