

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG093021\
 Data File : BG050402.D
 Acq On : 2 Oct 2021 23:48
 Operator : CG/JU
 Sample : M3877-03
 Misc :
 ALS Vial : 88 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EW2L8

Manual Integrations
 APPROVED

mohammad
 10/4/2021 11:52:11 AM

Quant Time: Oct 04 01:10:04 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG093021.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 30 16:27:24 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.278	152	58021	20.00	ng/ul	0.00
20) Naphthalene-d8	11.098	136	242053	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.888	164	157565	20.00	ng/ul	0.00
64) Phenanthrene-d10	17.632	188	317840	20.00	ng/ul	0.00
79) Chrysene-d12	21.933	240	273251	20.00	ng/ul	-0.02
88) Perylene-d12	25.364	264	272019	20.00	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.642	96	3874	2.45	ng/uL	0.00
4) Pyridine-d5	4.071	84	40233	8.55	ng/ul	0.00
7) Phenol-d5	7.402	99	84324	16.63	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.585	67	53543	16.78	ng/ul	0.00
11) 2-Chlorophenol-d4	7.796	132	59804	16.84	ng/ul	0.00
15) 4-Methylphenol-d8	8.959	113	63553	16.56	ng/ul	0.00
21) Nitrobenzene-d5	9.441	128	30976	18.29	ng/ul	0.00
24) 2-Nitrophenol-d4	10.170	143	33051	18.19	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.704	165	59155	16.48	ng/ul	0.00
31) 4-Chloroaniline-d4	11.222	131	73935	14.42	ng/ul	0.00
46) Dimethylphthalate-d6	14.283	166	186397	17.29	ng/ul	0.00
49) Acenaphthylene-d8	14.588	160	233748	17.26	ng/ul	0.00
54) 4-Nitrophenol-d4	15.052	143	31617m	15.22	ng/ul	0.00
60) Fluorene-d10	15.875	176	163868	16.87	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.981	200	10992	6.93	ng/ul	0.00
73) Anthracene-d10	17.732	188	250594	18.66	ng/ul	0.00
81) Pyrene-d10	20.005	212	287729	19.80	ng/ul	0.00
92) Benzo(a)pyrene-d12	25.129	264	257684	18.84	ng/ul	0.00
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.797	149	13082	1.37	ng/ul#	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG093021\
Data File : BG050402.D
Acq On : 2 Oct 2021 23:48
Operator : CG/JU
Sample : M3877-03
Misc :
ALS Vial : 88 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
EW2L8

Manual Integrations
APPROVED

mohammad
10/4/2021 11:52:11 AM


Quant Time: Oct 04 01:10:04 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG093021.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Sep 30 16:27:24 2021
Response via : Initial Calibration

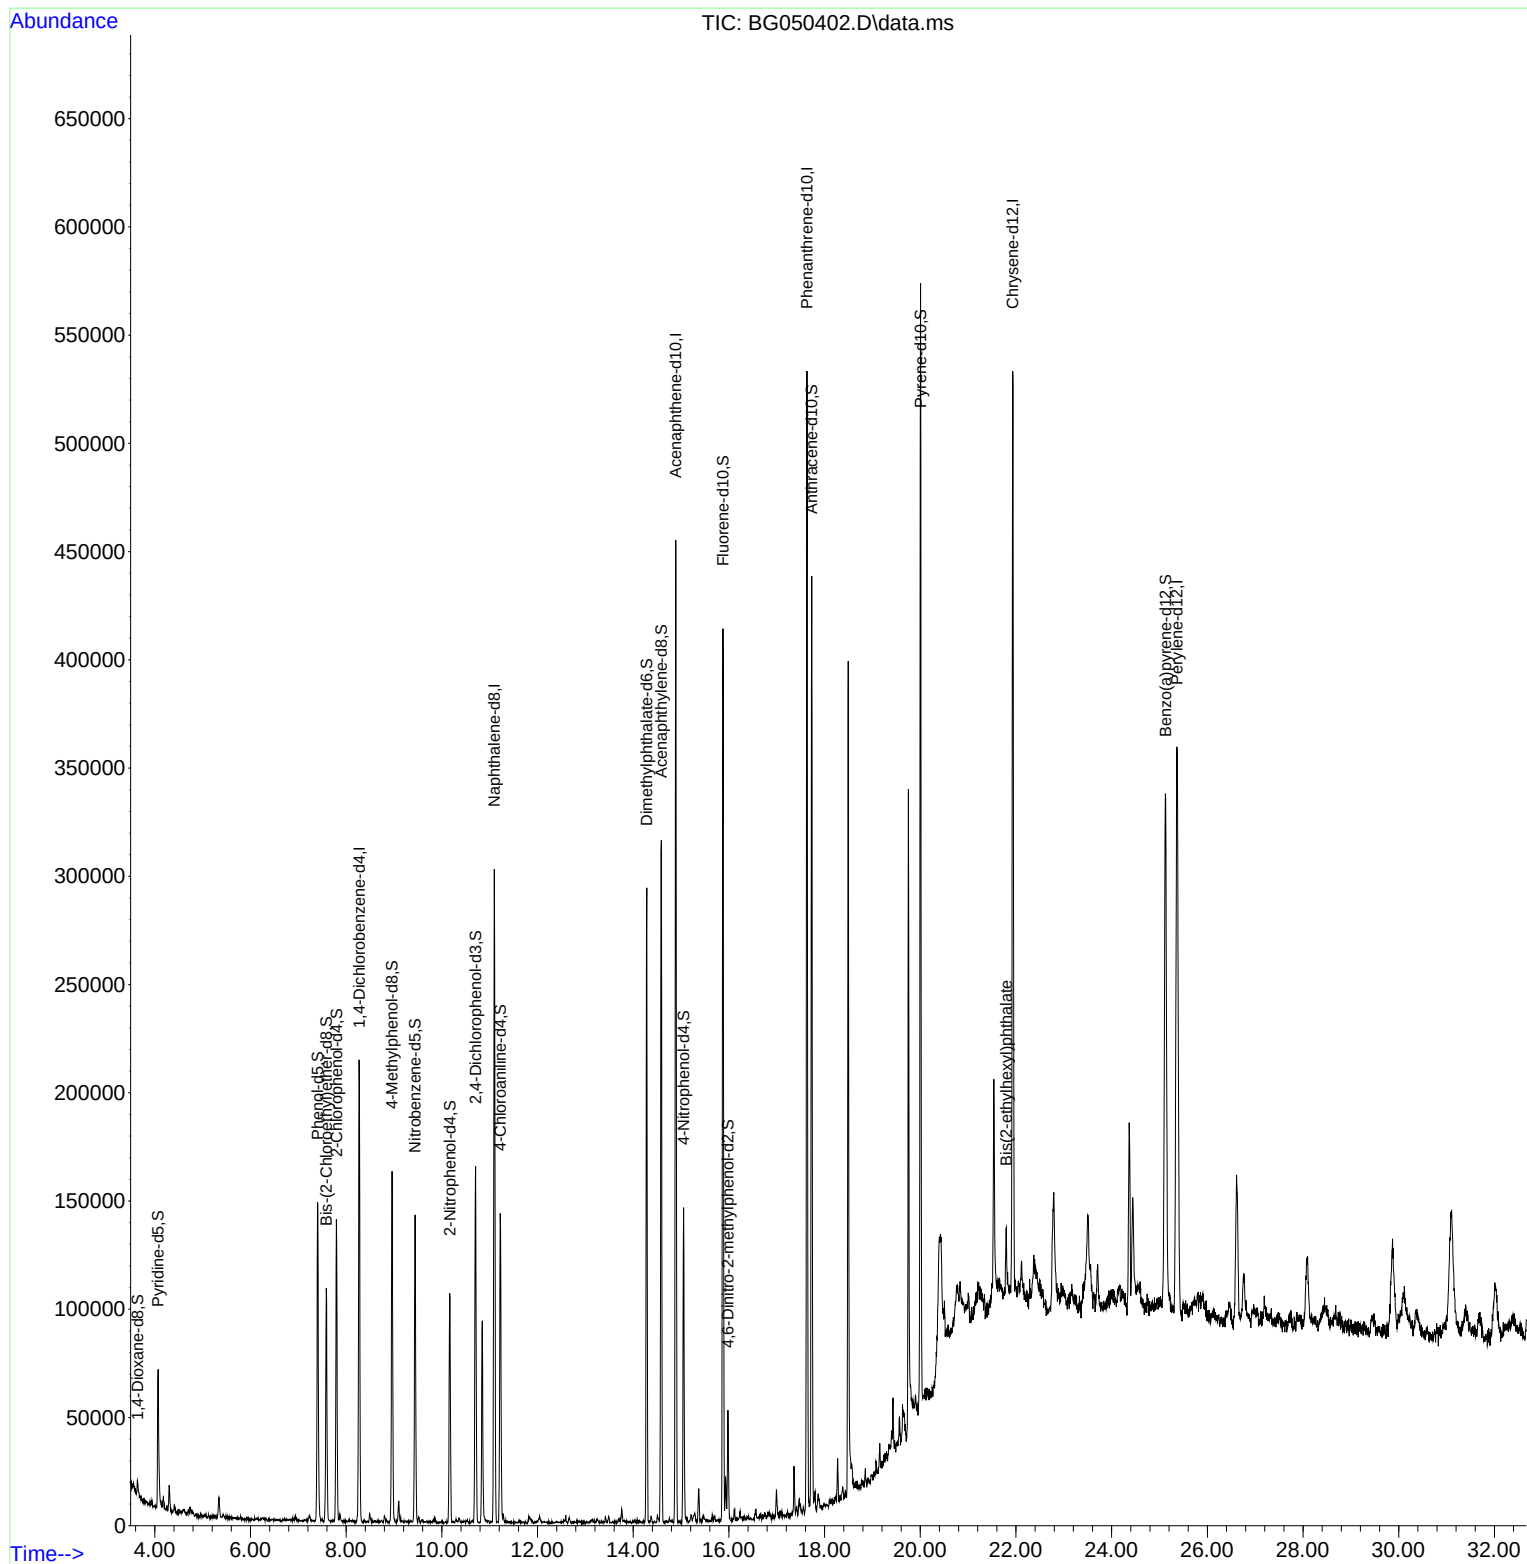

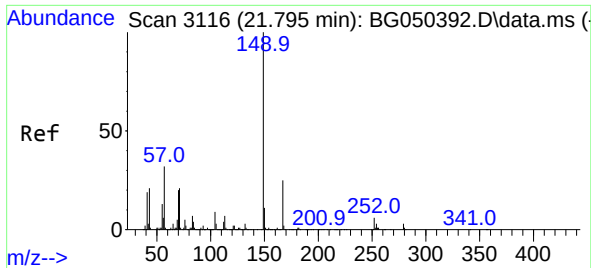

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 1.37 ng/ul
 RT: 21.797 min Scan# 3116
 Delta R.T. -0.010 min
 Lab File: BG050402.D
 Acq: 2 Oct 2021 23:48

Instrument :
 BNA_G
 ClientSampleId :
 EW2L8

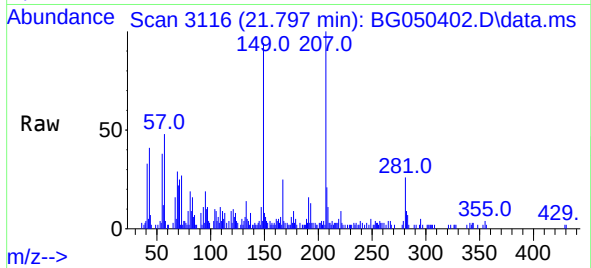

Tgt Ion	Ratio	Lower	Upper
149	100		
167	26.8	21.3	31.9
279	4.3	2.8	4.2#

Manual Integrations
 APPROVED

mohammad
 10/4/2021 11:52:11 AM

