

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG093021\
 Data File : BG050336.D
 Acq On : 1 Oct 2021 00:02
 Operator : CG/JU
 Sample : PB139333BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK333

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG093021.M
 Title : SVOA CALIBRATION

Signal : TIC: BG050336.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.643	22	26	33	rVB	14108	22255	1.47%	0.155%
2	4.066	93	98	114	rVV	191490	344362	22.75%	2.404%
3	4.406	150	156	158	rBV4	3438	5443	0.36%	0.038%
4	5.435	328	331	334	rBV3	1571	2081	0.14%	0.015%
5	5.887	404	408	411	rVB4	1486	2192	0.14%	0.015%
6	7.403	659	666	675	rVB	241455	418416	27.64%	2.921%
7	7.585	688	697	708	rBV	172043	306870	20.27%	2.142%
8	7.797	726	733	743	rVB	220778	385394	25.46%	2.691%
9	8.272	807	814	825	rBV	147971	253780	16.76%	1.772%
10	8.960	922	931	941	rBV	275833	479559	31.68%	3.348%
11	9.442	1005	1013	1023	rVB	219130	397305	26.25%	2.774%
12	10.170	1129	1137	1144	rVB	171184	308577	20.38%	2.154%
13	10.705	1220	1228	1238	rVB	258938	474710	31.36%	3.314%
14	11.099	1286	1295	1306	rVB	194903	357093	23.59%	2.493%
15	11.222	1308	1316	1325	rBV	266844	496653	32.81%	3.467%
16	12.315	1496	1502	1505	rBV2	907	1536	0.10%	0.011%
17	12.667	1555	1562	1567	rBV4	4142	7806	0.52%	0.054%
18	12.891	1597	1600	1606	rBV	1074	2013	0.13%	0.014%
19	14.283	1829	1837	1846	rBV	497655	723366	47.79%	5.050%
20	14.589	1882	1889	1898	rVB	516968	857124	56.62%	5.984%
21	14.888	1932	1940	1948	rVB	318767	498462	32.93%	3.480%
22	15.047	1960	1967	1977	rBV	254588	411867	27.21%	2.875%
23	15.117	1977	1979	1984	rVB5	1660	2641	0.17%	0.018%
24	15.875	2101	2108	2117	rVB	665467	1067563	70.52%	7.453%
25	15.975	2119	2125	2133	rBV	205487	302311	19.97%	2.111%
26	16.116	2143	2149	2154	rBV3	4158	6378	0.42%	0.045%
27	16.657	2239	2241	2245	rBV4	1921	2311	0.15%	0.016%
28	16.739	2250	2255	2257	rBV3	1795	2397	0.16%	0.017%
29	17.227	2332	2338	2340	rVB3	1074	2096	0.14%	0.015%
30	17.421	2369	2371	2376	rVB6	2132	2836	0.19%	0.020%
31	17.632	2400	2407	2415	rVB	412011	642737	42.46%	4.487%
32	17.732	2417	2424	2431	rVB	793272	1207942	79.80%	8.433%
33	17.861	2443	2446	2449	rVB3	1807	1815	0.12%	0.013%
34	18.079	2477	2483	2484	rBV3	1659	1514	0.10%	0.011%
35	18.572	2564	2567	2570	rVB4	1652	1831	0.12%	0.013%
36	18.613	2570	2574	2575	rBV3	2017	2592	0.17%	0.018%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG093021\
 Data File : BG050336.D
 Acq On : 1 Oct 2021 00:02
 Operator : CG/JU
 Sample : PB139333BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK333

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG093021.M
 Title : SVOA CALIBRATION

37	18.760	2596	2599	2602	rBV4	1472	1832	0.12%	0.013%
38	18.884	2619	2620	2623	rBV3	2053	2273	0.15%	0.016%
39	18.948	2628	2631	2633	rBV3	1504	2280	0.15%	0.016%
40	19.030	2641	2645	2649	rBV4	2146	4301	0.28%	0.030%
41	19.136	2661	2663	2665	rVB3	2113	1707	0.11%	0.012%
42	19.201	2673	2674	2676	rBV2	2375	1741	0.12%	0.012%
43	19.224	2676	2678	2682	rBV4	1550	2303	0.15%	0.016%
44	19.354	2698	2700	2705	rBV6	2602	4443	0.29%	0.031%
45	19.500	2724	2725	2727	rBV2	2143	1550	0.10%	0.011%
46	19.577	2734	2738	2743	rBV5	8660	12342	0.82%	0.086%
47	19.641	2745	2749	2754	rVB2	10755	16132	1.07%	0.113%
48	20.006	2804	2811	2818	rBV	1049893	1513765	100.00%	10.568%
49	20.270	2854	2856	2857	rBV2	4375	2107	0.14%	0.015%
50	21.933	3133	3139	3146	rVB2	407994	693077	45.78%	4.839%
51	25.123	3672	3682	3695	rVB2	447453	1336154	88.27%	9.328%
52	25.364	3712	3723	3741	rVB2	230119	724134	47.84%	5.055%




Sum of corrected areas: 14323969

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG093021\
Data File : BG050336.D
Acq On : 1 Oct 2021 00:02
Operator : CG/JU
Sample : PB139333BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK333

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG093021.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

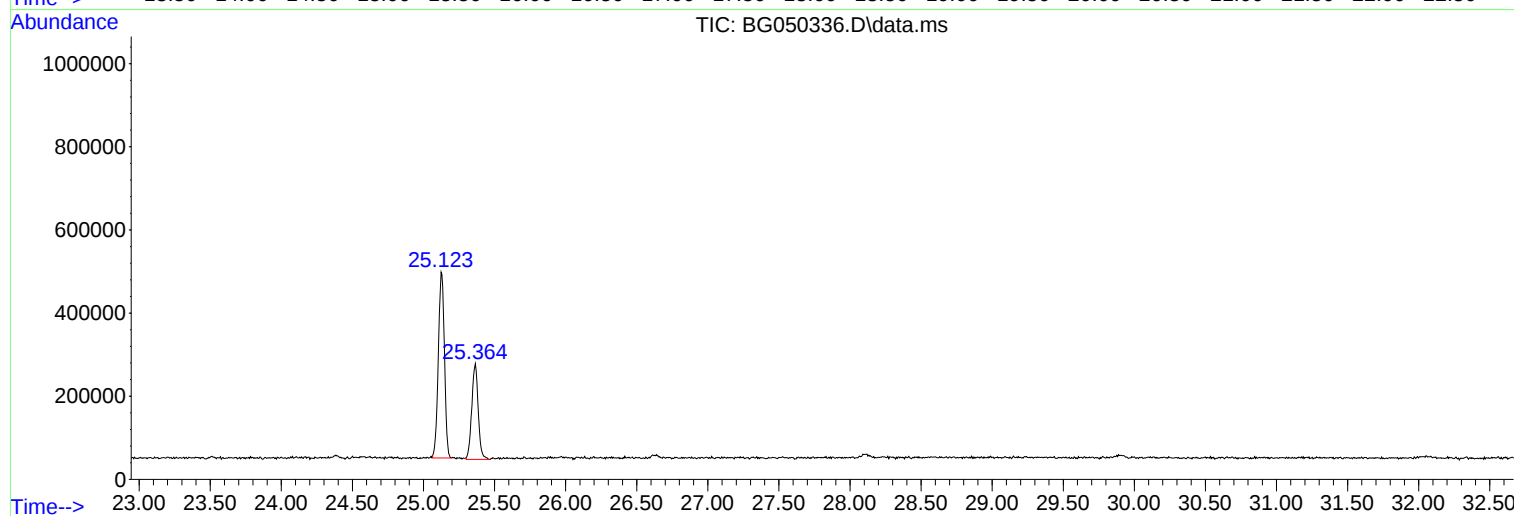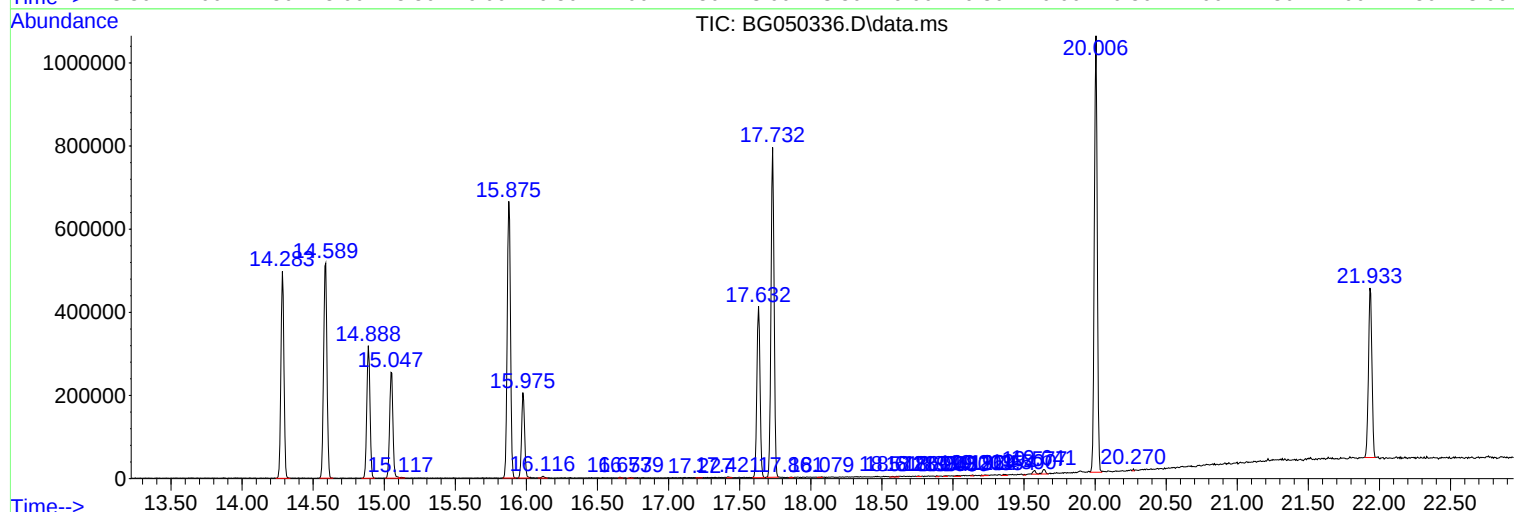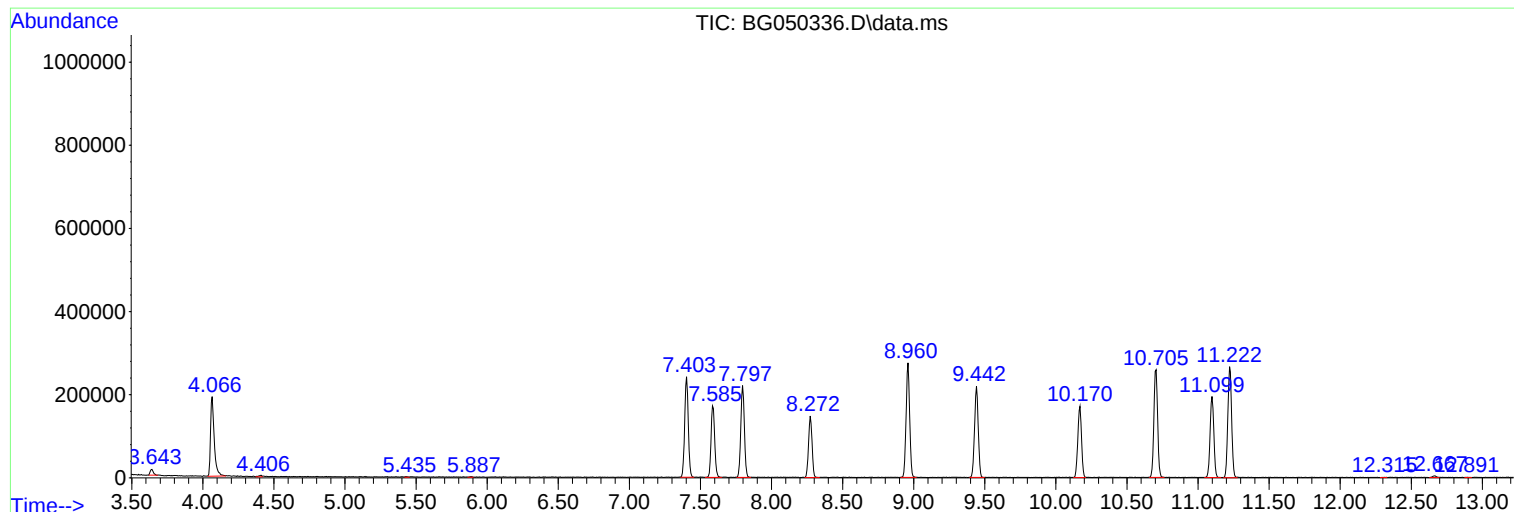

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG093021\
Data File : BG050336.D
Acq On : 1 Oct 2021 00:02
Operator : CG/JU
Sample : PB139333BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK333

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG093021.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG093021\
Data File : BG050336.D
Acq On : 1 Oct 2021 00:02
Operator : CG/JU
Sample : PB139333BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK333

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG093021.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------