

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG093021\
 Data File : BG050350.D
 Acq On : 1 Oct 2021 9:33
 Operator : CG/JU
 Sample : PB139436BL
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK436

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG093021.M
 Title : SVOA CALIBRATION

Signal : TIC: BG050350.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.636	21	25	35	rVB4	12208	20618	1.70%	0.171%
2	4.059	93	97	112	rBV	144581	261427	21.57%	2.171%
3	4.329	140	143	147	rVB2	1324	1487	0.12%	0.012%
4	4.394	151	154	158	rBV4	2646	3704	0.31%	0.031%
5	4.647	194	197	201	rBV4	873	1322	0.11%	0.011%
6	5.551	346	351	354	rVB2	1407	2542	0.21%	0.021%
7	5.575	354	355	358	rBV3	1249	1462	0.12%	0.012%
8	5.745	379	384	386	rBV2	872	1296	0.11%	0.011%
9	5.775	386	389	392	rVB2	1213	1215	0.10%	0.010%
10	6.550	518	521	524	rVB3	987	1251	0.10%	0.010%
11	6.585	524	527	529	rBV	1155	1435	0.12%	0.012%
12	7.402	657	666	674	rVV	178432	312772	25.80%	2.597%
13	7.455	674	675	680	rVB2	1128	1477	0.12%	0.012%
14	7.584	690	697	706	rBV	133550	227442	18.76%	1.888%
15	7.796	725	733	742	rVB	163389	288515	23.80%	2.395%
16	8.272	807	814	823	rVB	140559	244407	20.16%	2.029%
17	8.959	923	931	938	rBV	205183	365247	30.13%	3.033%
18	9.441	1005	1013	1024	rVB	162562	299988	24.75%	2.491%
19	10.164	1127	1136	1144	rVB	127662	233322	19.25%	1.937%
20	10.698	1220	1227	1236	rBV	200306	359999	29.70%	2.989%
21	11.098	1287	1295	1304	rVB	193813	354739	29.26%	2.945%
22	11.221	1309	1316	1326	rVV	210888	385052	31.76%	3.197%
23	12.661	1556	1561	1566	rVB3	3769	5931	0.49%	0.049%
24	13.847	1759	1763	1770	rBV2	947	2116	0.17%	0.018%
25	14.282	1830	1837	1843	rVB	405693	589556	48.63%	4.895%
26	14.582	1880	1888	1897	rVB	432308	687965	56.75%	5.712%
27	14.887	1931	1940	1947	rVB	326363	515183	42.50%	4.277%
28	15.046	1960	1967	1977	rBV	221747	345053	28.46%	2.865%
29	15.875	2101	2108	2118	rVB	583394	887177	73.18%	7.366%
30	15.974	2119	2125	2133	rVV	175081	257457	21.24%	2.138%
31	16.115	2145	2149	2155	rVB4	5107	7780	0.64%	0.065%
32	16.662	2240	2242	2247	rVB2	1300	1263	0.10%	0.010%
33	16.773	2259	2261	2266	rBV	828	1292	0.11%	0.011%
34	17.073	2308	2312	2313	rBV2	1515	1388	0.11%	0.012%
35	17.302	2344	2351	2356	rBV5	967	2612	0.22%	0.022%
36	17.426	2367	2372	2377	rVB5	2572	4606	0.38%	0.038%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG093021\
 Data File : BG050350.D
 Acq On : 1 Oct 2021 9:33
 Operator : CG/JU
 Sample : PB139436BL
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK436

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG093021.M
 Title : SVOA CALIBRATION

37	17.631	2400	2407	2413	rVB	438950	675333	55.71%	5.607%
38	17.731	2413	2424	2432	rVV	666355	1025273	84.58%	8.513%
39	18.283	2515	2518	2519	rVB2	1533	1567	0.13%	0.013%
40	18.524	2558	2559	2562	rBV3	1932	1544	0.13%	0.013%
41	18.571	2562	2567	2572	rVV3	3382	4936	0.41%	0.041%
42	18.642	2577	2579	2583	rBV4	1504	1609	0.13%	0.013%
43	18.777	2601	2602	2603	rBV	2513	1224	0.10%	0.010%
44	18.801	2603	2606	2607	rVV3	1831	2027	0.17%	0.017%
45	18.818	2607	2609	2613	rVV4	1160	1625	0.13%	0.013%
46	18.865	2615	2617	2620	rVB3	1368	1398	0.12%	0.012%
47	18.989	2636	2638	2641	rBV3	1554	1740	0.14%	0.014%
48	19.071	2648	2652	2656	rBV5	1576	2912	0.24%	0.024%
49	19.106	2656	2658	2662	rVV3	1366	1776	0.15%	0.015%
50	19.365	2698	2702	2705	rBV5	1749	2781	0.23%	0.023%
51	19.494	2721	2724	2725	rBV3	2075	1706	0.14%	0.014%
52	19.570	2733	2737	2744	rBV5	8380	13808	1.14%	0.115%
53	19.635	2744	2748	2751	rBV2	9462	12587	1.04%	0.105%
54	19.746	2765	2767	2768	rBV2	2979	1400	0.12%	0.012%
55	19.782	2771	2773	2775	rBV3	2718	1881	0.16%	0.016%
56	20.005	2804	2811	2820	rBV	815596	1212240	100.00%	10.065%
57	20.087	2823	2825	2826	rBV2	3452	2408	0.20%	0.020%
58	21.932	3132	3139	3146	rBV	413543	696053	57.42%	5.779%
59	25.123	3672	3682	3694	rVB	350580	1016721	83.87%	8.442%
60	25.352	3713	3721	3735	rVB2	217288	679649	56.07%	5.643%




Sum of corrected areas: 12044296

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG093021\
Data File : BG050350.D
Acq On : 1 Oct 2021 9:33
Operator : CG/JU
Sample : PB139436BL
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK436

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG093021.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

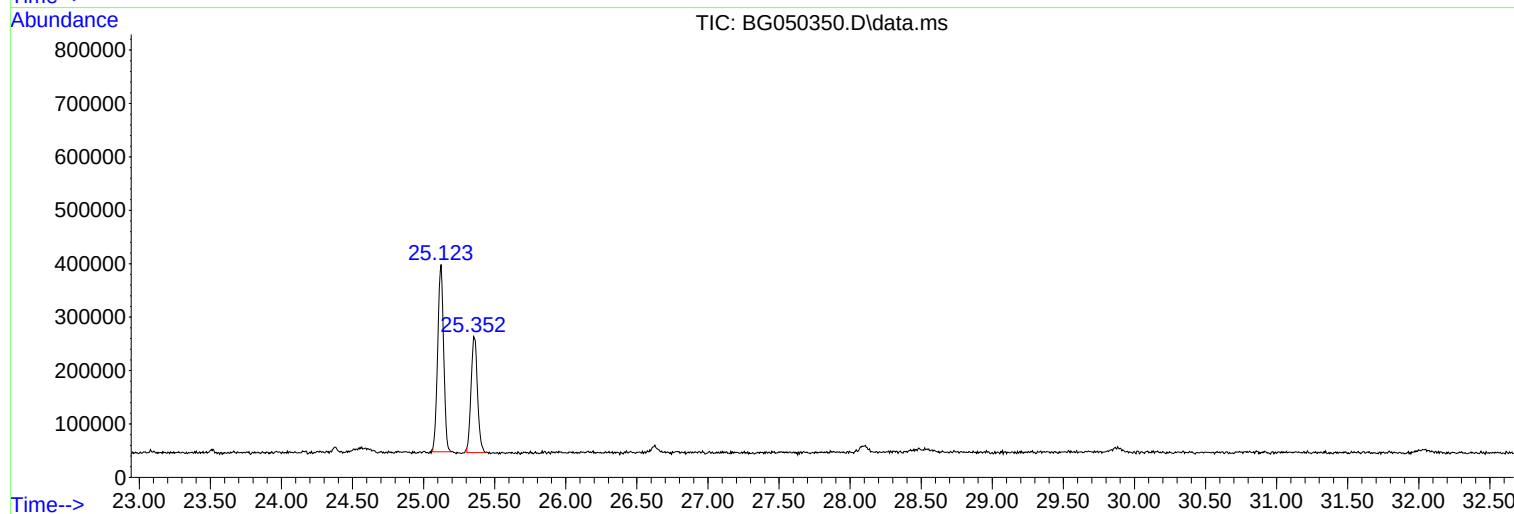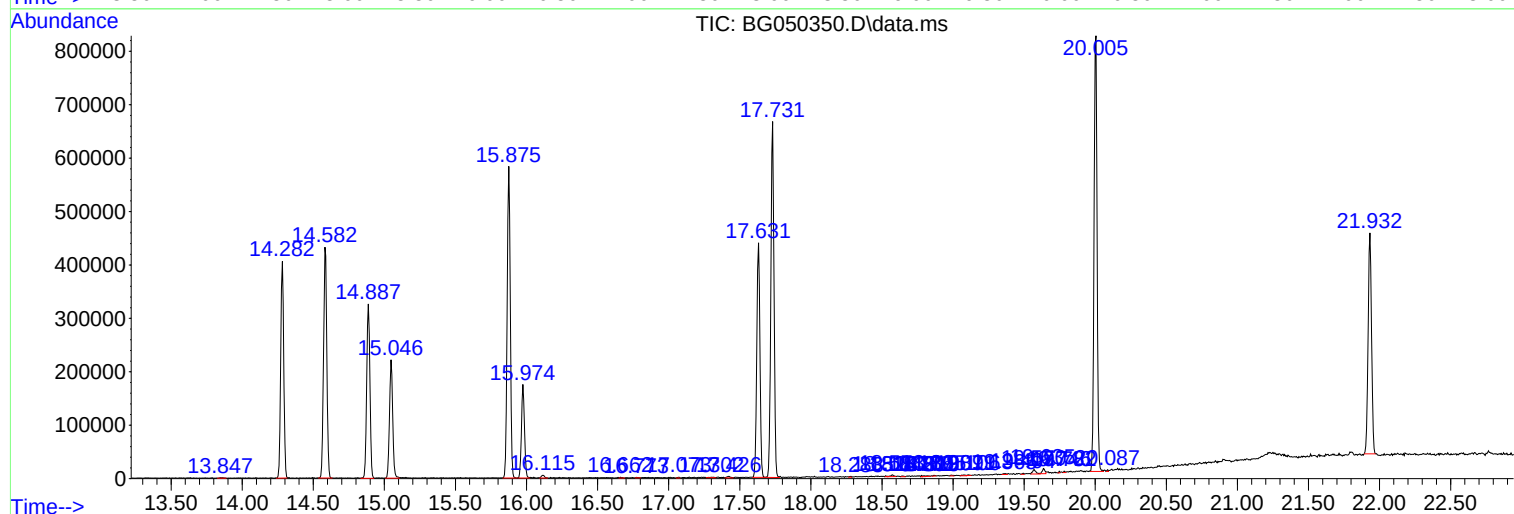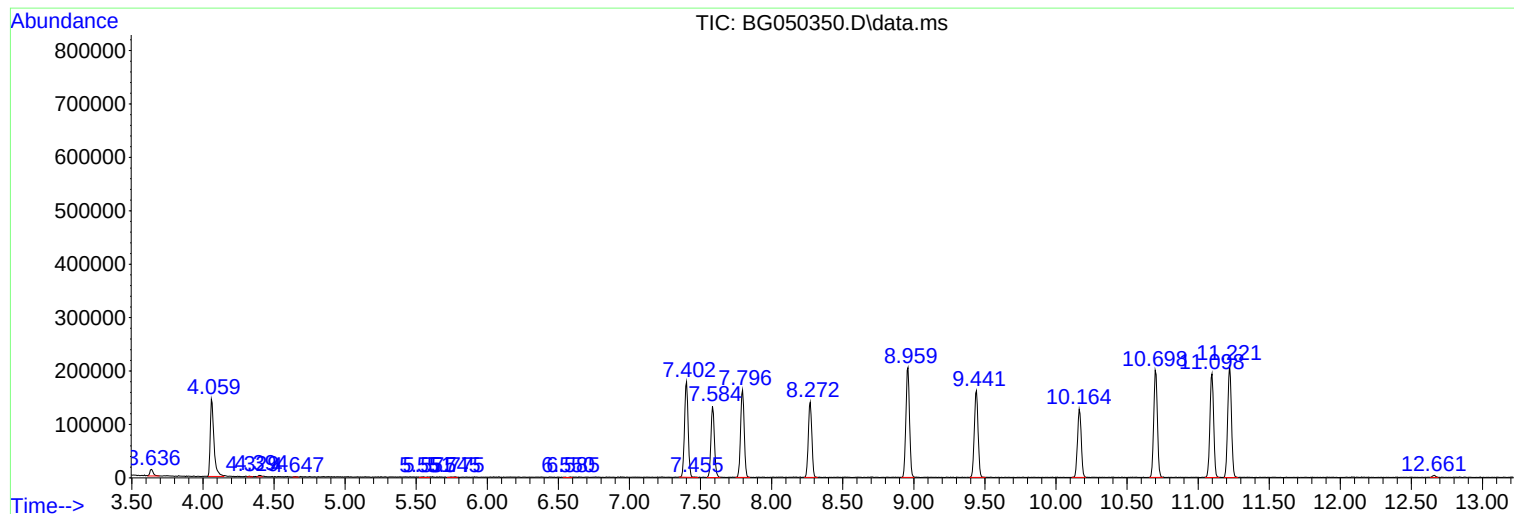

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG093021\
Data File : BG050350.D
Acq On : 1 Oct 2021 9:33
Operator : CG/JU
Sample : PB139436BL
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK436

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG093021.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG093021\
Data File : BG050350.D
Acq On : 1 Oct 2021 9:33
Operator : CG/JU
Sample : PB139436BL
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK436

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG093021.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------