

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG093021\
 Data File : BG050351.D
 Acq On : 1 Oct 2021 10:13
 Operator : CG/JU
 Sample : PB139436BS
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SLCS436

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG093021.M
 Title : SVOA CALIBRATION

Signal : TIC: BG050351.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.635	20	25	27	rBV2	11336	16699	0.81%	0.027%
2	3.670	27	31	39	rVB2	26135	45861	2.22%	0.075%
3	4.076	92	100	113	rBV2	214575	586263	28.35%	0.963%
4	4.405	150	156	160	rBV4	4614	8553	0.41%	0.014%
5	7.401	658	666	679	rBV2	421087	1098280	53.12%	1.805%
6	7.589	691	698	707	rBV	143034	248914	12.04%	0.409%
7	7.678	707	713	723	rVB	156879	267766	12.95%	0.440%
8	7.795	726	733	736	rBV	191192	362957	17.55%	0.596%
9	7.830	736	739	746	rVB	199083	316780	15.32%	0.521%
10	8.271	807	814	822	rVB	149366	257672	12.46%	0.423%
11	8.694	879	886	895	rVV	263000	468488	22.66%	0.770%
12	8.800	895	904	911	rVV3	145990	364192	17.61%	0.598%
13	8.847	911	912	919	rVB4	5885	6640	0.32%	0.011%
14	8.958	922	931	937	rBV	232603	424661	20.54%	0.698%
15	9.023	937	942	947	rVV	246728	473194	22.88%	0.778%
16	9.094	947	954	965	rVB2	314730	821919	39.75%	1.350%
17	9.370	994	1001	1007	rBV	171749	319096	15.43%	0.524%
18	9.440	1007	1013	1017	rVV	184597	355315	17.18%	0.584%
19	9.487	1017	1021	1028	rVB	197542	342082	16.54%	0.562%
20	10.010	1102	1110	1117	rBV	290302	507131	24.53%	0.833%
21	10.169	1126	1137	1139	rBV	153694	278680	13.48%	0.458%
22	10.198	1139	1142	1145	rVV	169962	289894	14.02%	0.476%
23	10.239	1145	1149	1158	rVB	306988	526474	25.46%	0.865%
24	10.316	1158	1162	1167	rBV2	3315	5673	0.27%	0.009%
25	10.486	1183	1191	1199	rVB	210837	348203	16.84%	0.572%
26	10.709	1218	1229	1230	rBV	253288	443480	21.45%	0.729%
27	11.097	1286	1295	1299	rBV	204420	387262	18.73%	0.636%
28	11.150	1299	1304	1310	rVV	338451	625909	30.27%	1.028%
29	11.232	1310	1318	1329	rVB2	274236	815282	39.43%	1.340%
30	11.426	1344	1351	1359	rBV	249635	437786	21.17%	0.719%
31	12.014	1441	1451	1455	rBV	97508	224475	10.86%	0.369%
32	12.337	1498	1506	1514	rBV	297628	503350	24.34%	0.827%
33	12.607	1543	1552	1559	rBV3	52735	134273	6.49%	0.221%
34	12.660	1559	1561	1566	rVV4	3977	6131	0.30%	0.010%
35	12.736	1566	1574	1582	rVB	428503	738122	35.70%	1.213%
36	12.848	1589	1593	1598	rVB3	10066	15124	0.73%	0.025%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG093021\
 Data File : BG050351.D
 Acq On : 1 Oct 2021 10:13
 Operator : CG/JU
 Sample : PB139436BS
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SLCS436

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG093021.M
 Title : SVOA CALIBRATION

37	12.948	1603	1610	1618	rVB	428344	724525	35.04%	1.190%
38	13.089	1624	1634	1642	rVB2	401395	963200	46.58%	1.583%
39	13.324	1667	1674	1680	rBV	329307	516142	24.96%	0.848%
40	13.394	1680	1686	1695	rVB	315376	519996	25.15%	0.854%
41	13.694	1730	1737	1739	rBV	398297	631970	30.56%	1.038%
42	13.723	1739	1742	1746	rVV	509173	820696	39.69%	1.348%
43	13.770	1746	1750	1758	rVB	409830	681657	32.97%	1.120%
44	13.970	1773	1784	1792	rBV	264373	435973	21.08%	0.716%
45	14.188	1816	1821	1825	rBV3	6125	8910	0.43%	0.015%
46	14.282	1830	1837	1841	rBV	419754	643283	31.11%	1.057%
47	14.329	1841	1845	1853	rVB	431352	663479	32.09%	1.090%
48	14.452	1859	1866	1874	rVB	300892	471007	22.78%	0.774%
49	14.587	1882	1889	1891	rBV	490074	795694	38.48%	1.307%
50	14.611	1891	1893	1902	rVB	449067	676076	32.70%	1.111%
51	14.781	1916	1922	1930	rVB	257330	413158	19.98%	0.679%
52	14.887	1933	1940	1946	rBV	344550	548018	26.50%	0.900%
53	14.951	1946	1951	1962	rVV2	548642	1114460	53.90%	1.831%
54	15.063	1962	1970	1980	rVV3	400382	815347	39.43%	1.340%
55	15.198	1983	1993	1997	rVV	414268	758701	36.69%	1.247%
56	15.233	1997	1999	2003	rVV	303814	408272	19.75%	0.671%
57	15.286	2003	2008	2015	rVB	503106	793006	38.35%	1.303%
58	15.498	2038	2044	2055	rVB	360392	560054	27.09%	0.920%
59	15.686	2070	2076	2083	rBV	527893	749594	36.25%	1.232%
60	15.874	2101	2108	2112	rBV	603029	975479	47.18%	1.603%
61	15.927	2112	2117	2123	rVV3	944515	2067712	100.00%	3.397%
62	15.991	2123	2128	2138	rVB3	324636	633591	30.64%	1.041%
63	16.132	2144	2152	2158	rBV	630414	945425	45.72%	1.553%
64	16.179	2158	2160	2166	rVB3	4556	6462	0.31%	0.011%
65	16.520	2214	2218	2222	rVV4	4626	6391	0.31%	0.011%
66	16.814	2261	2268	2276	rVB	505792	717338	34.69%	1.179%
67	16.931	2281	2288	2295	rVV	463964	701738	33.94%	1.153%
68	17.072	2306	2312	2322	rVB	549185	748615	36.20%	1.230%
69	17.272	2336	2346	2358	rBV	352598	552646	26.73%	0.908%
70	17.425	2366	2372	2379	rBV3	15964	25223	1.22%	0.041%
71	17.631	2400	2407	2411	rVV	452111	745132	36.04%	1.224%
72	17.678	2411	2415	2420	rVV	719319	1122492	54.29%	1.844%
73	17.730	2420	2424	2427	rVV	678014	1078316	52.15%	1.772%
74	17.766	2427	2430	2437	rVV	724178	1087143	52.58%	1.786%
75	18.030	2467	2475	2481	rBV	661750	1021954	49.42%	1.679%
76	18.271	2513	2516	2522	rVB6	4166	5246	0.25%	0.009%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG093021\
 Data File : BG050351.D
 Acq On : 1 Oct 2021 10:13
 Operator : CG/JU
 Sample : PB139436BS
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SLCS436

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG093021.M
 Title : SVOA CALIBRATION

77	18.577	2560	2568	2574	rBV	744567	950200	45.95%	1.561%
78	19.334	2695	2697	2700	rBV4	3083	4378	0.21%	0.007%
79	19.423	2705	2712	2714	rBV5	5315	9871	0.48%	0.016%
80	19.570	2731	2737	2742	rBV8	9440	16915	0.82%	0.028%
81	19.669	2742	2754	2762	rVV	944965	1364003	65.97%	2.241%
82	19.904	2789	2794	2801	rVB2	60982	89963	4.35%	0.148%
83	20.004	2803	2811	2814	rBV	863806	1487841	71.96%	2.445%
84	20.034	2814	2816	2822	rVB	924488	1100969	53.25%	1.809%
85	20.139	2829	2834	2838	rVB	76002	96185	4.65%	0.158%
86	20.909	2959	2965	2971	rBV	747107	943539	45.63%	1.550%
87	21.150	3003	3006	3011	rVB2	34956	51816	2.51%	0.085%
88	21.802	3111	3117	3128	rVB2	900622	1912806	92.51%	3.143%
89	21.920	3129	3137	3144	rVV2	828120	2054944	99.38%	3.376%
90	21.984	3144	3148	3156	rVB	781457	1281187	61.96%	2.105%
91	22.290	3196	3200	3206	rVB8	26478	47294	2.29%	0.078%
92	23.024	3320	3325	3329	rBV2	64036	121234	5.86%	0.199%
93	23.089	3329	3336	3346	rVB	599607	1110765	53.72%	1.825%
94	24.264	3526	3536	3542	rBV	501705	1319112	63.80%	2.167%
95	24.340	3542	3549	3563	rVB	520617	1307871	63.25%	2.149%
96	25.128	3671	3683	3689	rBV3	379086	1181469	57.14%	1.941%
97	25.198	3689	3695	3707	rVB	409778	1142498	55.25%	1.877%
98	25.357	3713	3722	3735	rVB2	233578	736317	35.61%	1.210%
99	29.293	4377	4392	4398	rBV2	249043	1144791	55.37%	1.881%
100	30.521	4584	4601	4617	rVB3	224136	1157811	55.99%	1.902%




Sum of corrected areas: 60860481

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG093021\
Data File : BG050351.D
Acq On : 1 Oct 2021 10:13
Operator : CG/JU
Sample : PB139436BS
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampled :
SLCS436

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG093021.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

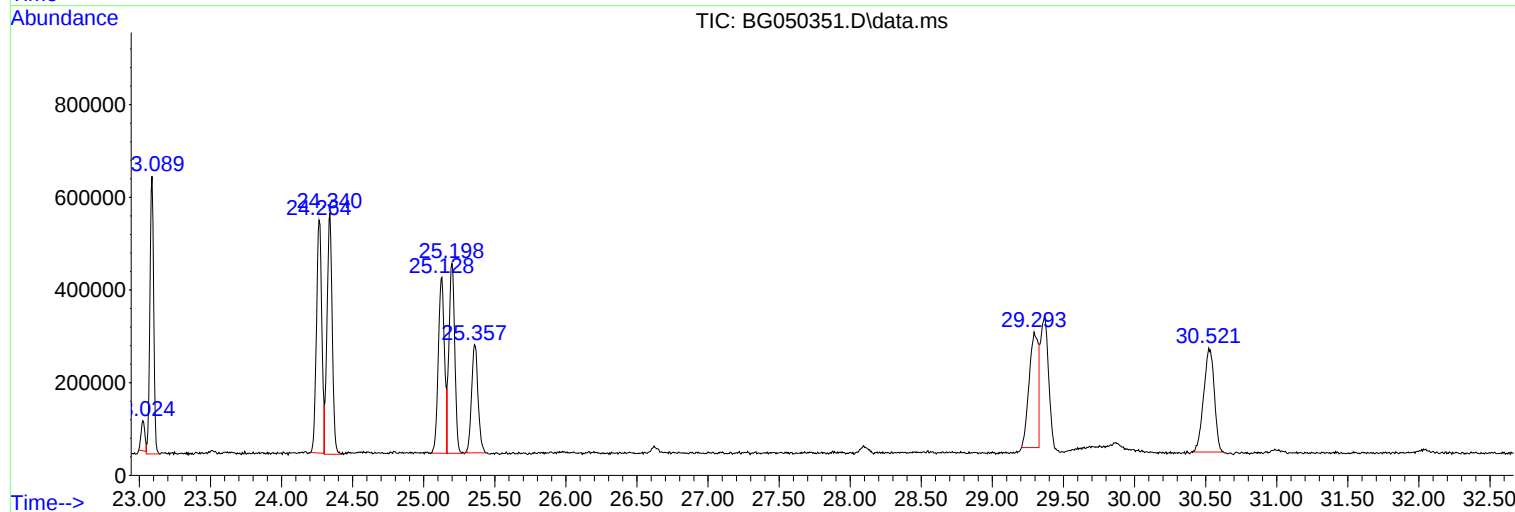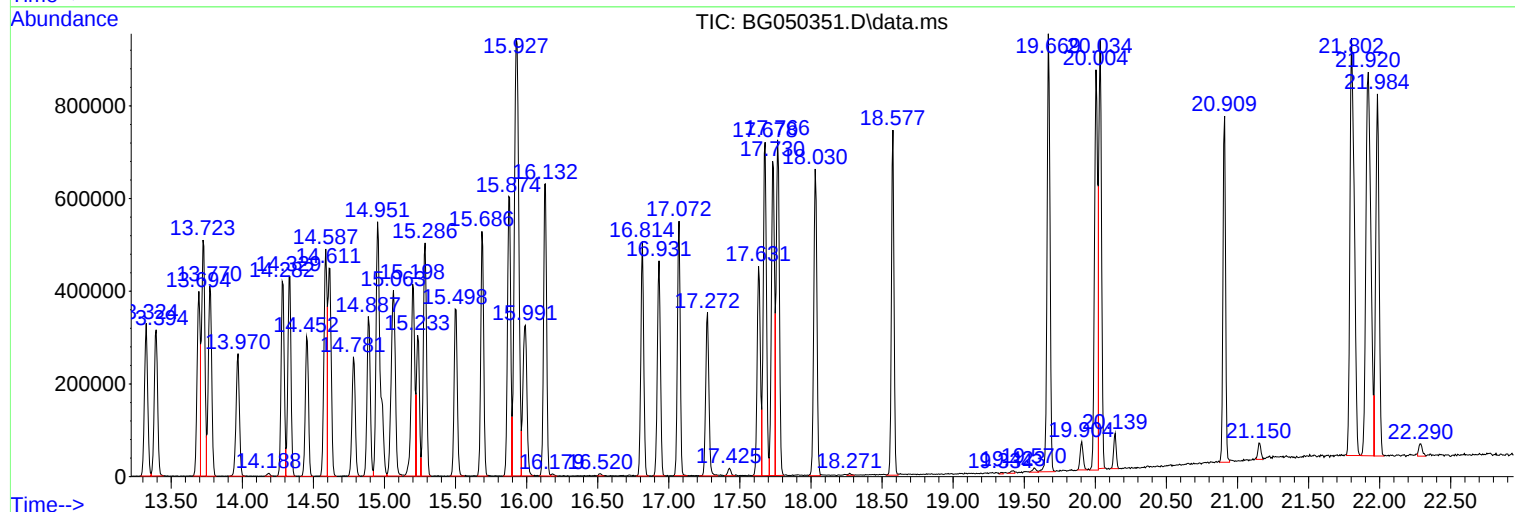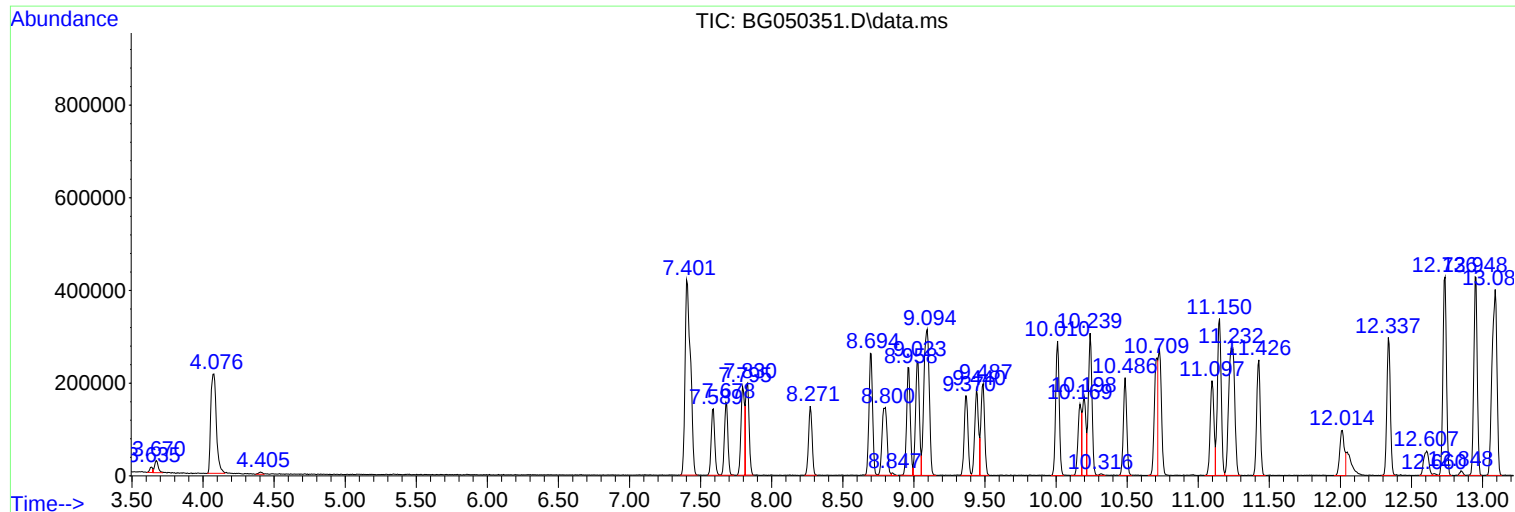

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG093021\
Data File : BG050351.D
Acq On : 1 Oct 2021 10:13
Operator : CG/JU
Sample : PB139436BS
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SLCS436










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG093021.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 4-Chloroaniline, N-isopropy... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
12.607	6.93 ng/ul	134273	Naphthalene-d8	11.097

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			4-Chloroaniline, N-isopropylidene	167	C9H10ClN	040938-43-0	90
2			Benzonitrile, 2-amino-5-chloro-	152	C7H5ClN2	005922-60-1	35
3			Chlorhexidine	504	C22H30Cl2N10	000055-56-1	32
4			Benzofuran, 7-chloro-	152	C8H5ClO	024410-55-7	30
5			Biphenylene	152	C12H8	000259-79-0	27

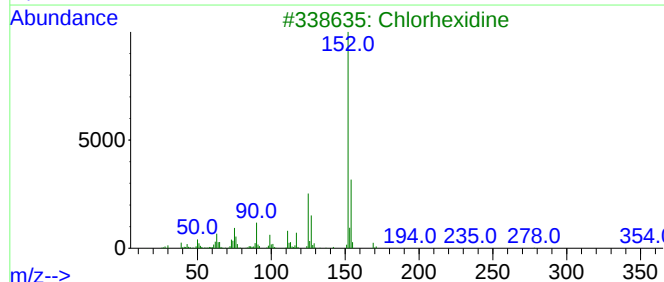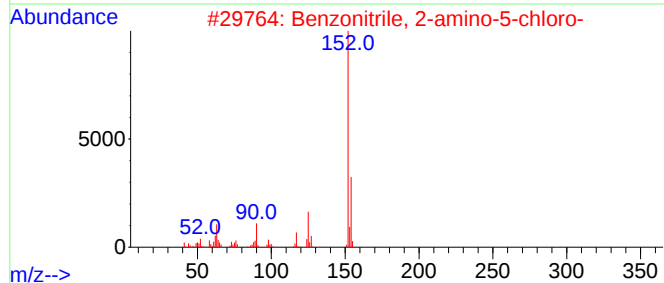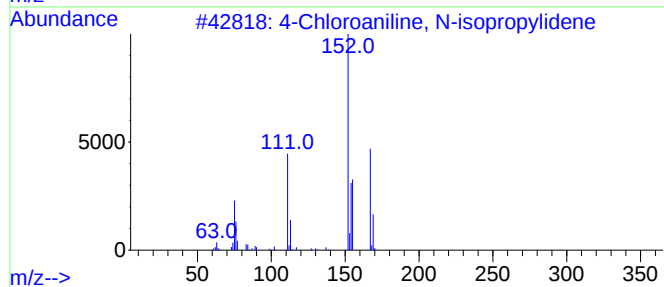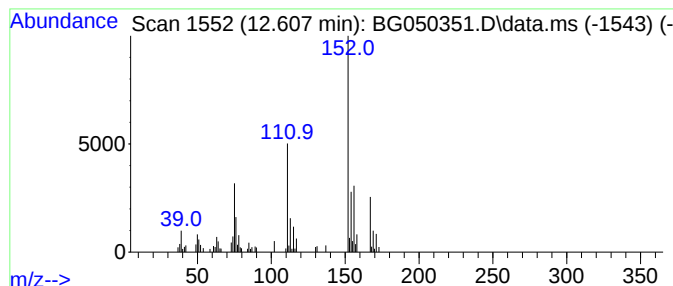

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG093021\
Data File : BG050351.D
Acq On : 1 Oct 2021 10:13
Operator : CG/JU
Sample : PB139436BS
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SLCS436

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG093021.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
4-Chloroaniline...	12.607	6.9	ng/u1	134273	2	11.097	387262	20.0